

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
 Data File : FF007354.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2020 11:24
 Operator : DD\AJ
 Sample : L3637-11 10X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 15:16:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.753	221281	1.621 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.945	156422	0.990 ug/ml
13)	N-TRIACONTANE	17.829	144109	0.919 ug/ml
14)	N-DOTRIACONTANE	18.662	132435	0.894 ug/ml
16)	N-HEXATRIACONTANE	20.226	39740	0.430 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
Data File : FF007354.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2020 11:24
Operator : DD\AJ
Sample : L3637-11 10X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 15:16:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

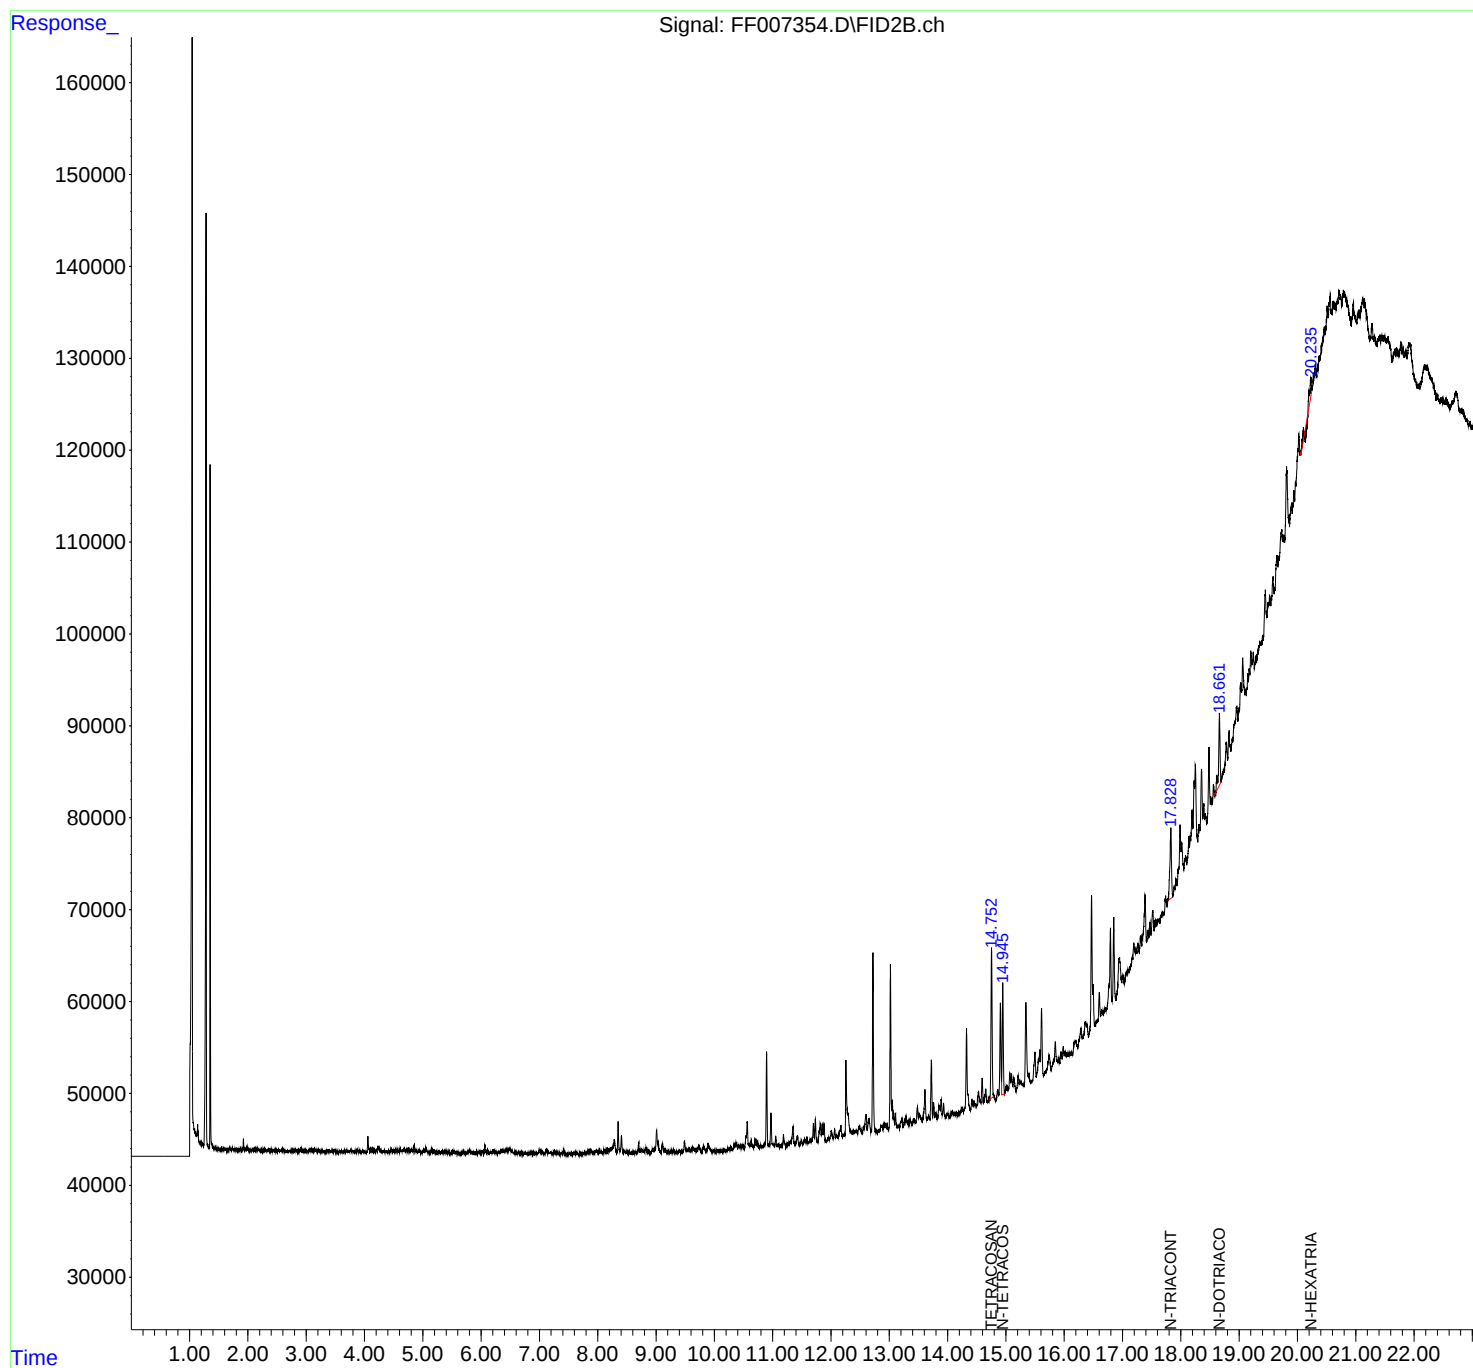


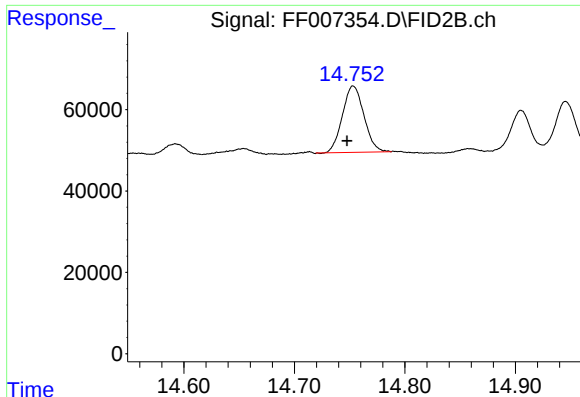

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.753 min
Delta R.T.: 0.005 min
Response: 221281
Conc: 1.62 ug/ml

Instrument :
FID_F
ClientSampleId :

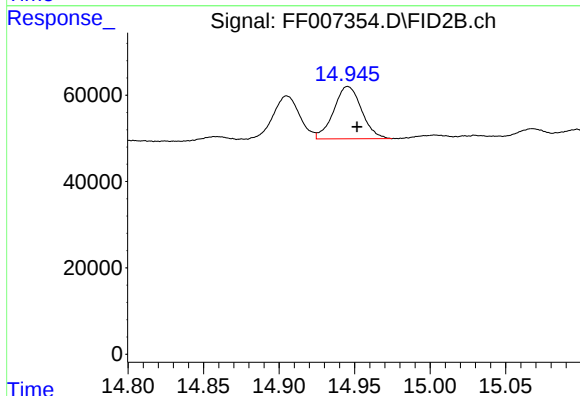


#10 N-TETRACOSANE

R.T.: 14.945 min
Delta R.T.: -0.006 min
Response: 156422
Conc: 0.99 ug/ml

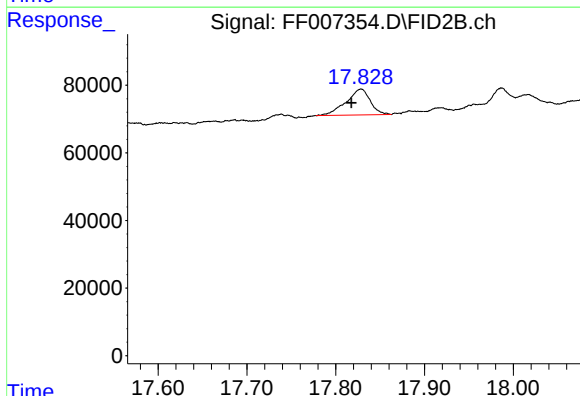


#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: 0.011 min
Response: 144109
Conc: 0.92 ug/ml

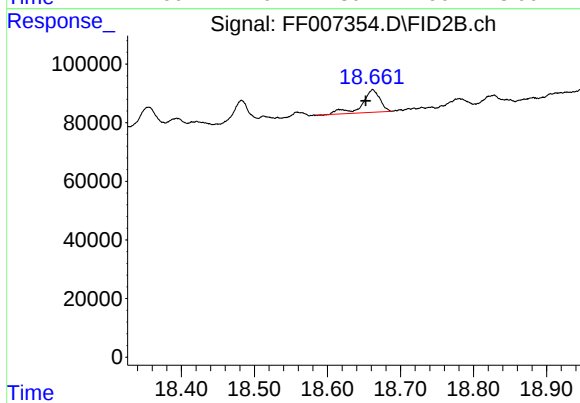

#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: 0.009 min
Response: 132435
Conc: 0.89 ug/ml

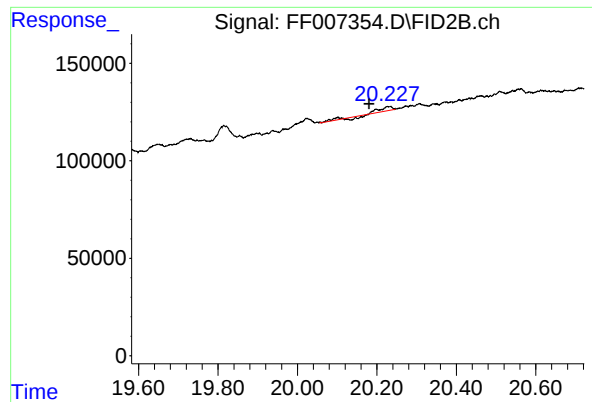

#16 N-HEXATRIACONTANE

R.T.: 20.226 min
Delta R.T.: 0.046 min
Response: 39740
Conc: 0.43 ug/ml

Instrument :
FID_F
ClientSampleId :