

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
 Data File : FF007355.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2020 11:55
 Operator : DD\AJ
 Sample : L3637-12 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 15:16:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.754	187580	1.374 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.946	163120	1.033 ug/ml
13)	N-TRIACONTANE	17.829	144378	0.921 ug/ml
16)	N-HEXATRIACONTANE	20.150	11591	0.125 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
Data File : FF007355.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2020 11:55
Operator : DD\AJ
Sample : L3637-12 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 13 15:16:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

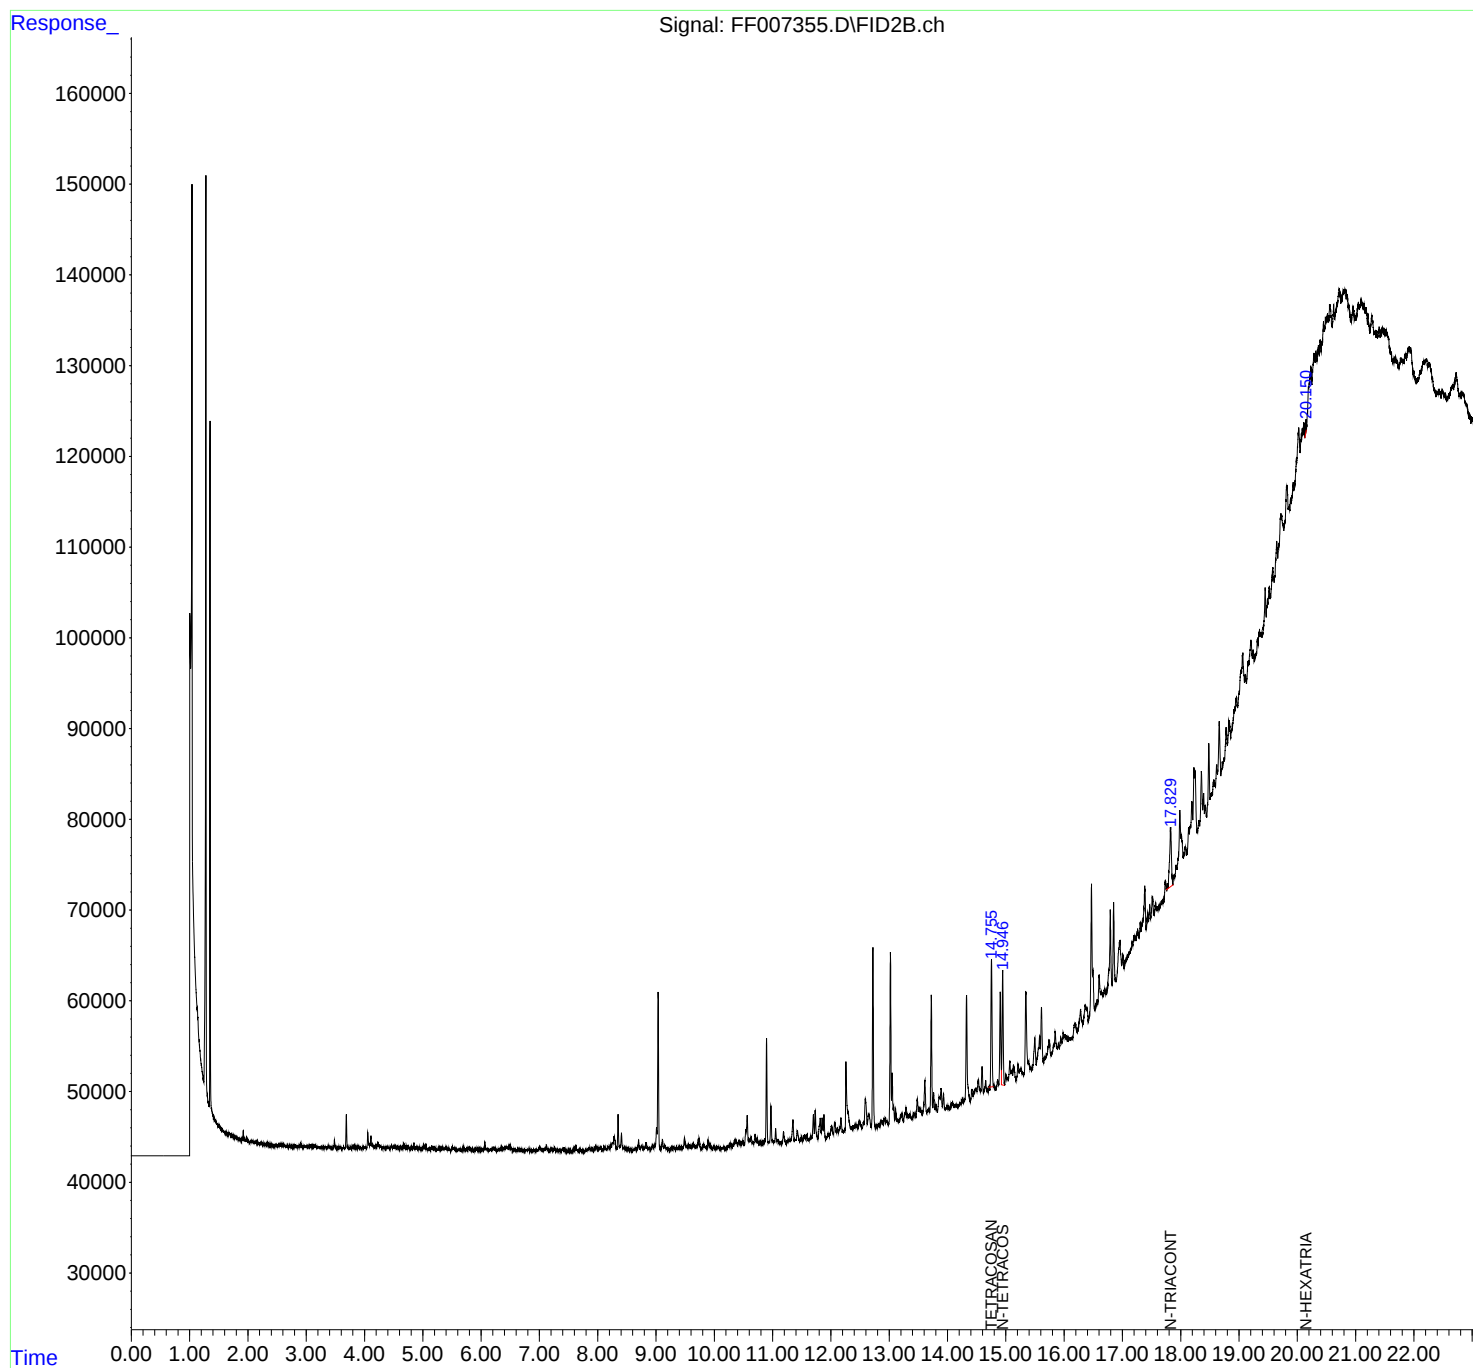


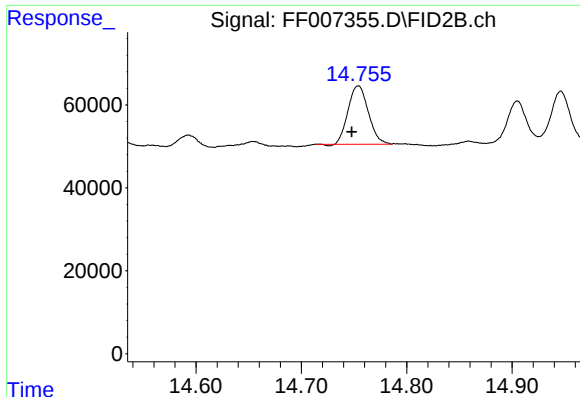

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.754 min
Delta R.T.: 0.006 min
Response: 187580
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :

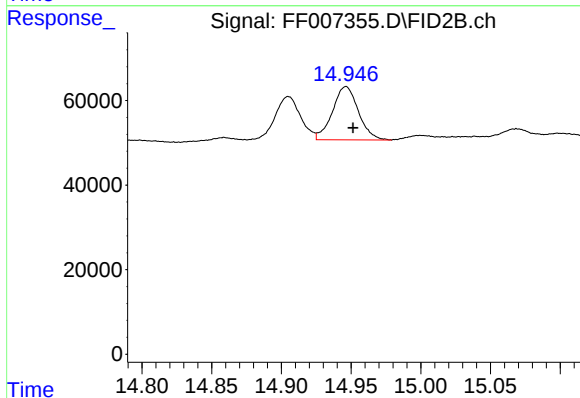


#10 N-TETRACOSANE

R.T.: 14.946 min
Delta R.T.: -0.005 min
Response: 163120
Conc: 1.03 ug/ml

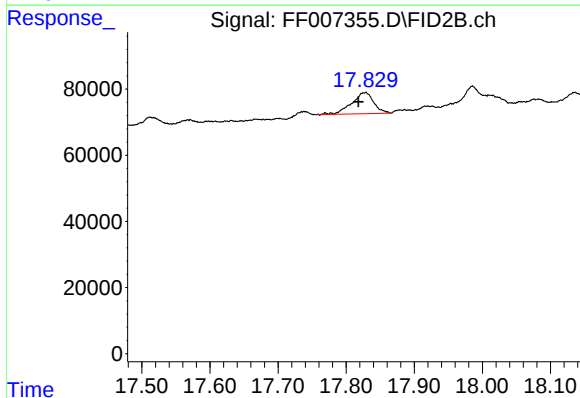

#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: 0.011 min
Response: 144378
Conc: 0.92 ug/ml

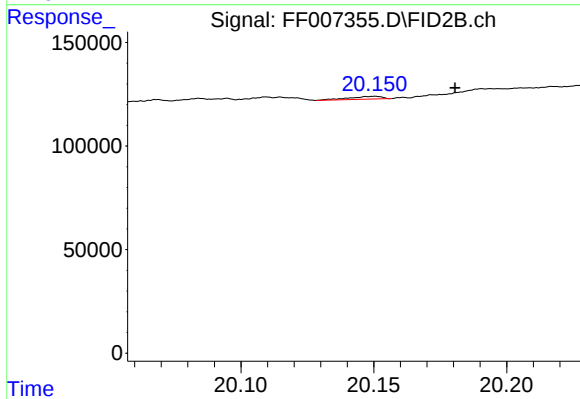

#16 N-HEXATRIACONTANE

R.T.: 20.150 min
Delta R.T.: -0.031 min
Response: 11591
Conc: 0.13 ug/ml