

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
 Data File : FF007356.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2020 12:26
 Operator : DD\AJ
 Sample : L3637-16 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 15:16:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	155771	1.141 ug/ml
Target Compounds			
3) N-DODECANE	6.447	95755	0.673 ug/ml
10) N-TETRACOSANE	14.946	236187	1.495 ug/ml
16) N-HEXATRIACONTANE	20.112f	64804	0.701 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
Data File : FF007356.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2020 12:26
Operator : DD\AJ
Sample : L3637-16 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 15:16:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

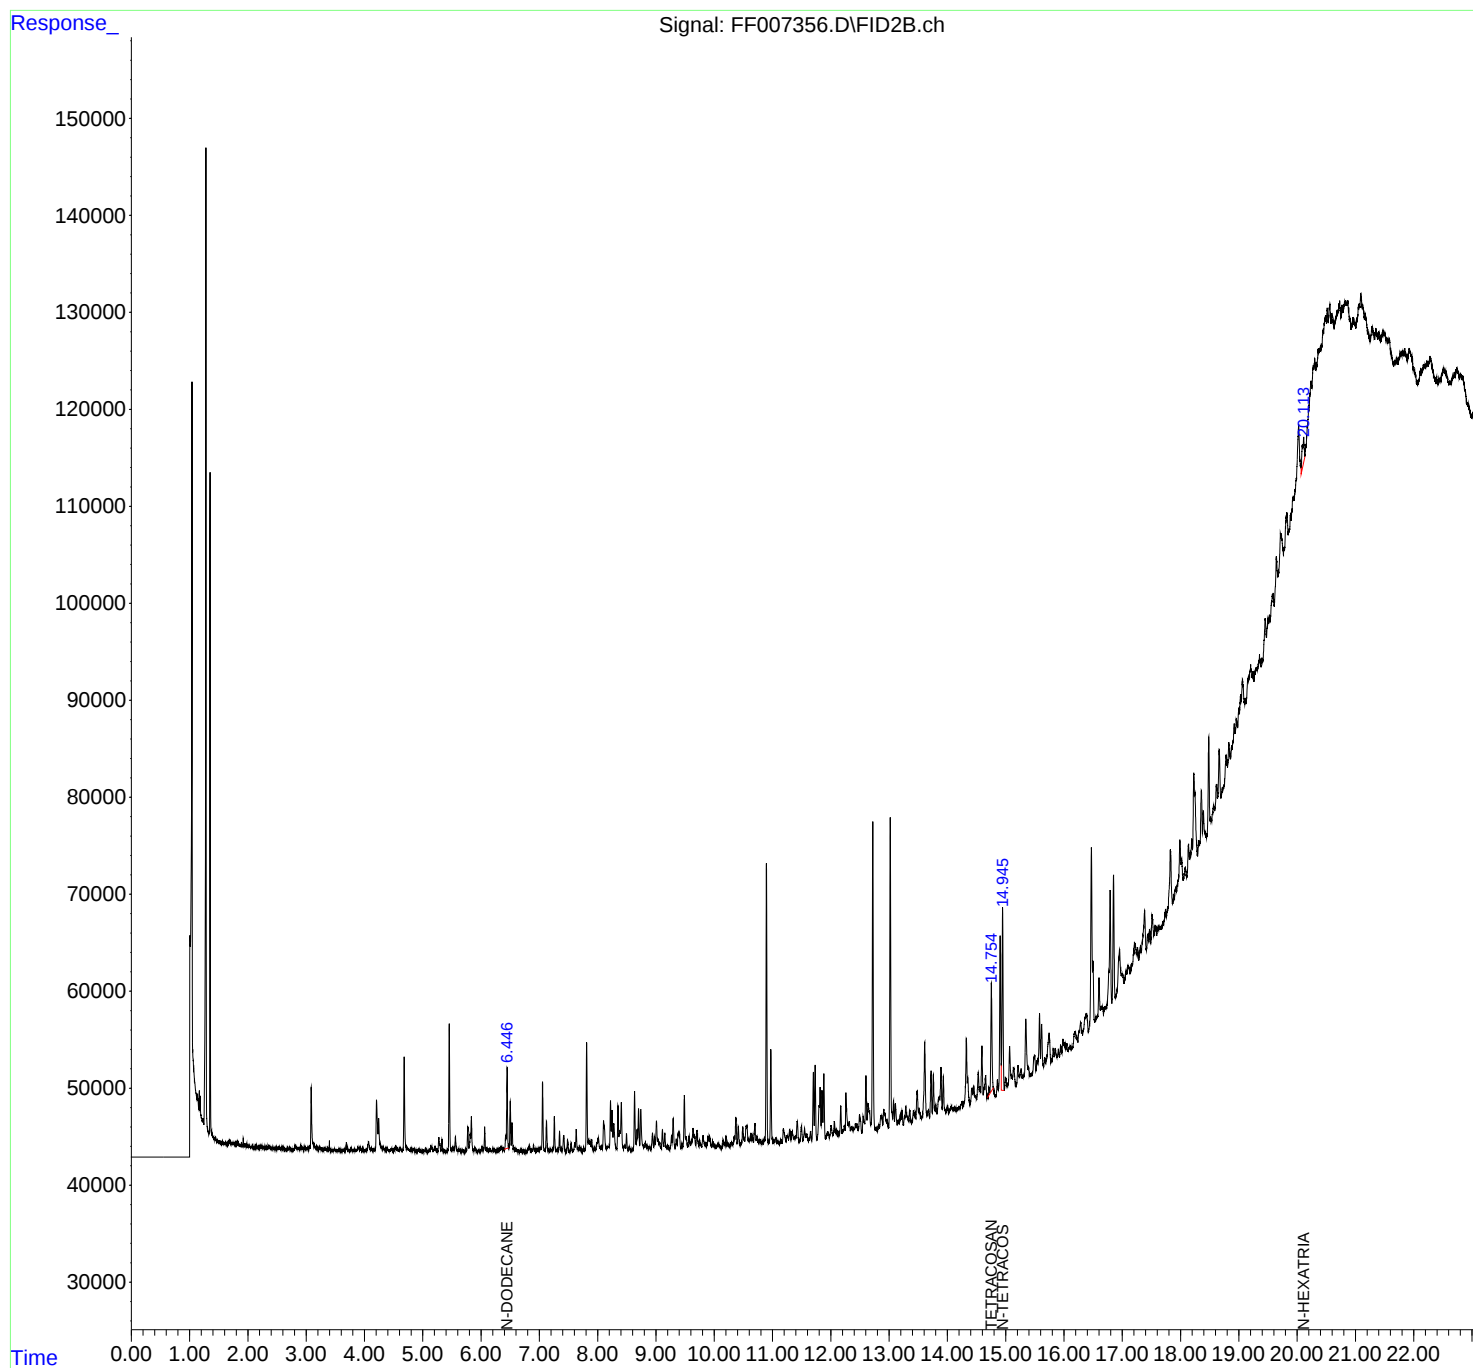


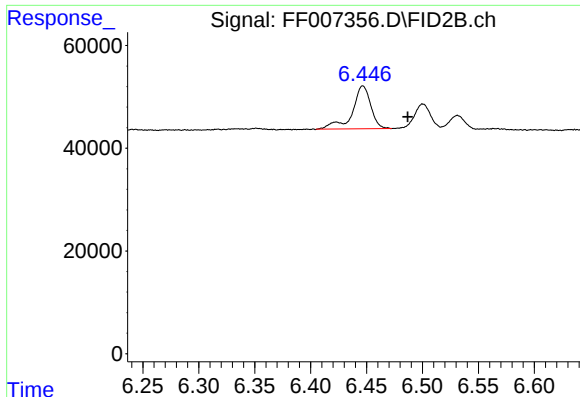

#3 N-DODECANE


R.T.: 6.447 min
Delta R.T.: -0.040 min
Response: 95755
Conc: 0.67 ug/ml

Instrument :
FID_F
ClientSampleId :

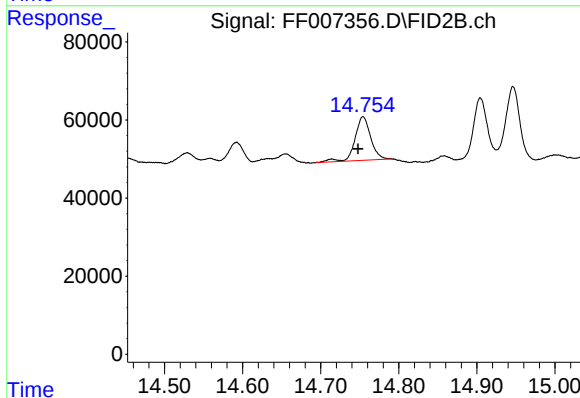


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.754 min
Delta R.T.: 0.007 min
Response: 155771
Conc: 1.14 ug/ml

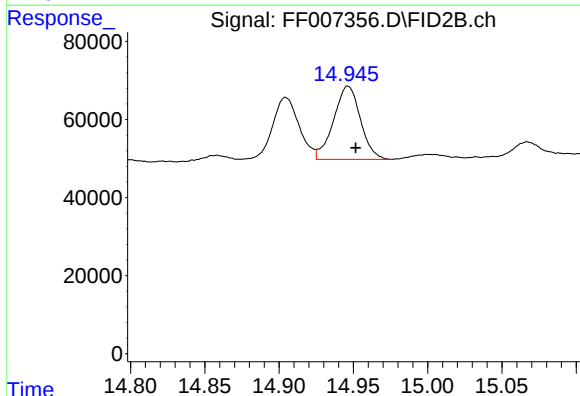

#10 N-TETRACOSANE

R.T.: 14.946 min
Delta R.T.: -0.005 min
Response: 236187
Conc: 1.50 ug/ml

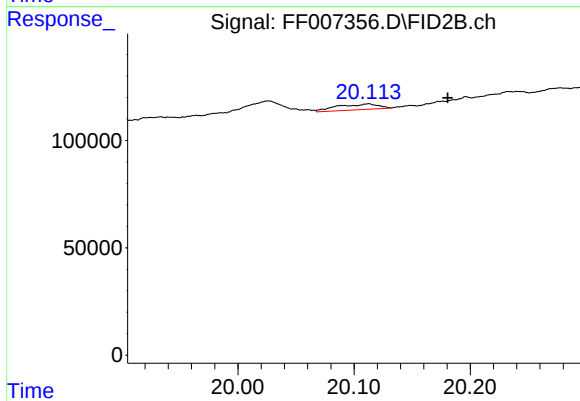

#16 N-HEXATRIACONTANE

R.T.: 20.112 min
Delta R.T.: -0.068 min
Response: 64804
Conc: 0.70 ug/ml