

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
 Data File : FF007359.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2020 14:00
 Operator : DD\AJ
 Sample : L3637-15 20X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 15:16:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.752	119480	0.875 ug/ml
Target Compounds			
7) N-EICOSANE	12.603	73706	0.476 ug/ml
10) N-TETRACOSANE	14.943	254109	1.609 ug/ml
14) N-DOTRIACONTANE	18.662	98409	0.664 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
Data File : FF007359.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2020 14:00
Operator : DD\AJ
Sample : L3637-15 20X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 13 15:16:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

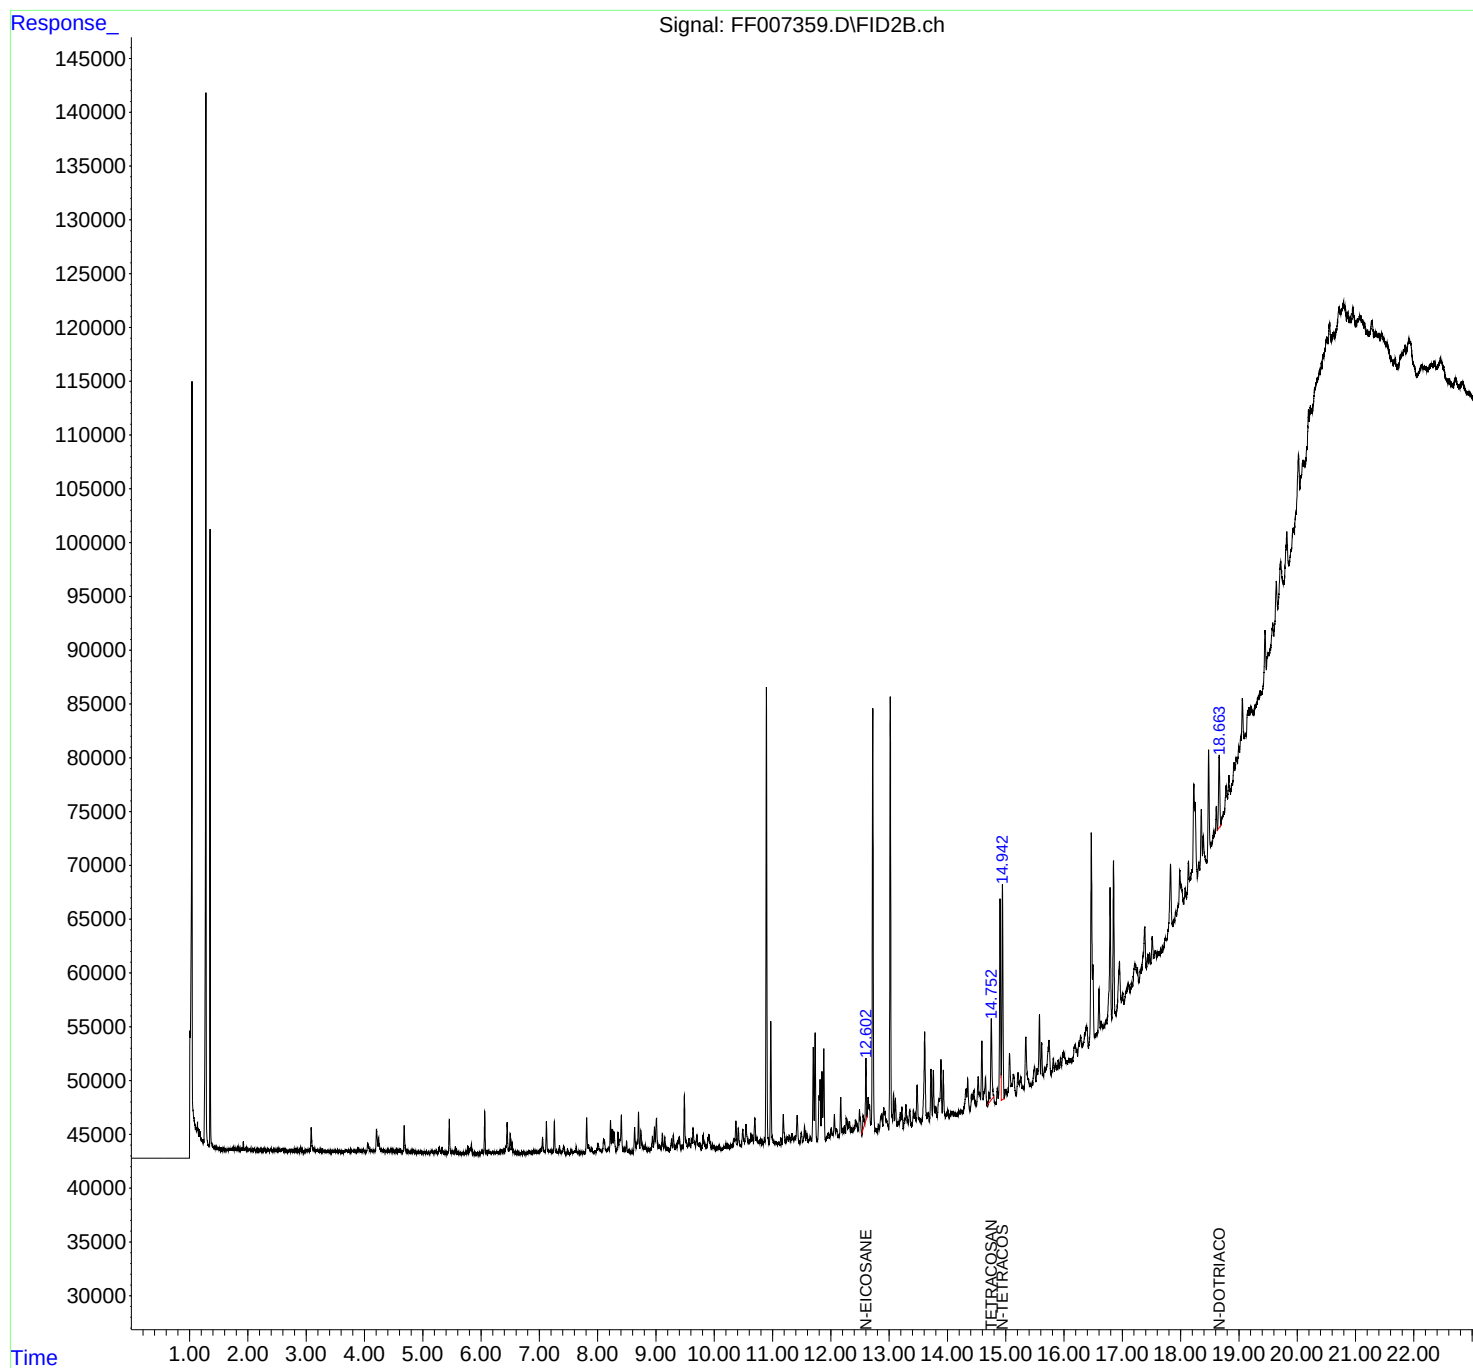


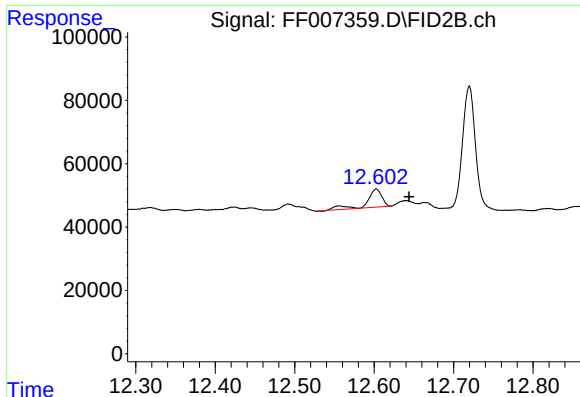

#7 N-EICOSANE


R.T.: 12.603 min
Delta R.T.: -0.041 min
Response: 73706
Conc: 0.48 ug/ml

Instrument :
FID_F
ClientSampleId :

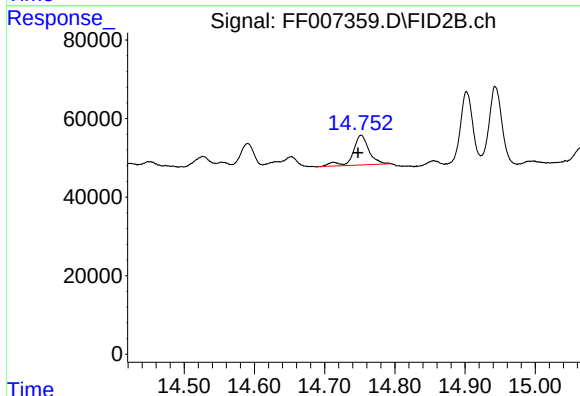


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.752 min
Delta R.T.: 0.004 min
Response: 119480
Conc: 0.88 ug/ml

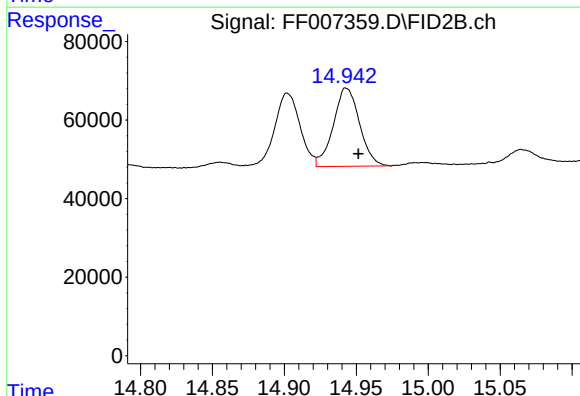

#10 N-TETRACOSANE

R.T.: 14.943 min
Delta R.T.: -0.008 min
Response: 254109
Conc: 1.61 ug/ml

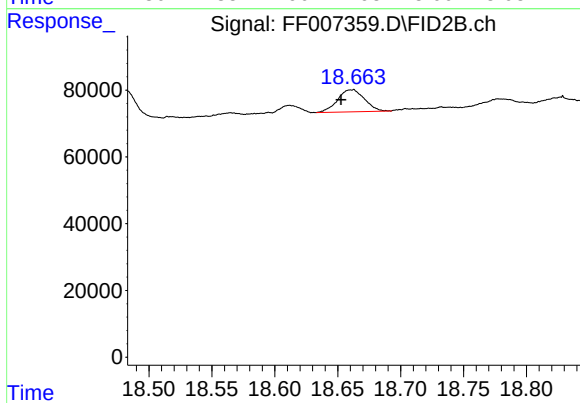

#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: 0.009 min
Response: 98409
Conc: 0.66 ug/ml