

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
 Data File : FF007367.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2020 18:39
 Operator : DD\AJ
 Sample : L3637-24MS 5X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAR-WASH-AREA-3-TPH-4MS

Manual Integrations
 APPROVED

Ankita
 8/14/2020 12:26:51 PM

Integration File: autoint1.e
 Quant Time: Aug 14 01:24:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.752	574874	4.212 ug/mlm
Target Compounds			
1) N-OCTANE	2.345	340729	2.512 ug/ml
2) N-DECANE	4.461	566671	4.060 ug/ml
3) N-DODECANE	6.487	598077	4.205 ug/ml
4) N-TETRADECANE	8.285	620090	4.261 ug/ml
5) N-HEXADECANE	9.889	614004	4.131 ug/ml
6) N-OCTADECANE	11.335	604074	3.939 ug/ml
7) N-EICOSANE	12.647	715984	4.626 ug/ml
8) N-DOCOSANE	13.849	639982	4.100 ug/mlm
10) N-TETRACOSANE	14.948	1027954	6.508 ug/ml
11) N-HEXACOSANE	15.981	605343	3.861 ug/ml
12) N-OCTACOSANE	16.935	731585	4.661 ug/ml
13) N-TRIACONTANE	17.822	740645	4.722 ug/mlm
14) N-DOTRIACONTANE	18.659	603999	4.077 ug/ml
15) N-TETRATRIACONTANE	19.447	646687	5.347 ug/mlm
16) N-HEXATRIACONTANE	20.191	649720	7.024 ug/mlm
17) N-OCTATRIACONTANE	20.955	557168	7.844 ug/ml
18) N-TETRACONTANE	21.907	673934	10.076 ug/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081320\
Data File : FF007367.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2020 18:39
Operator : DD\AJ
Sample : L3637-24MS 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1


Instrument :
FID_F
ClientSampled :
CAR-WASH-AREA-3-TPH-4MS


Manual Integrations
APPROVED

Ankita
8/14/2020 12:26:51 PM

Integration File: autoint1.e
Quant Time: Aug 14 01:24:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

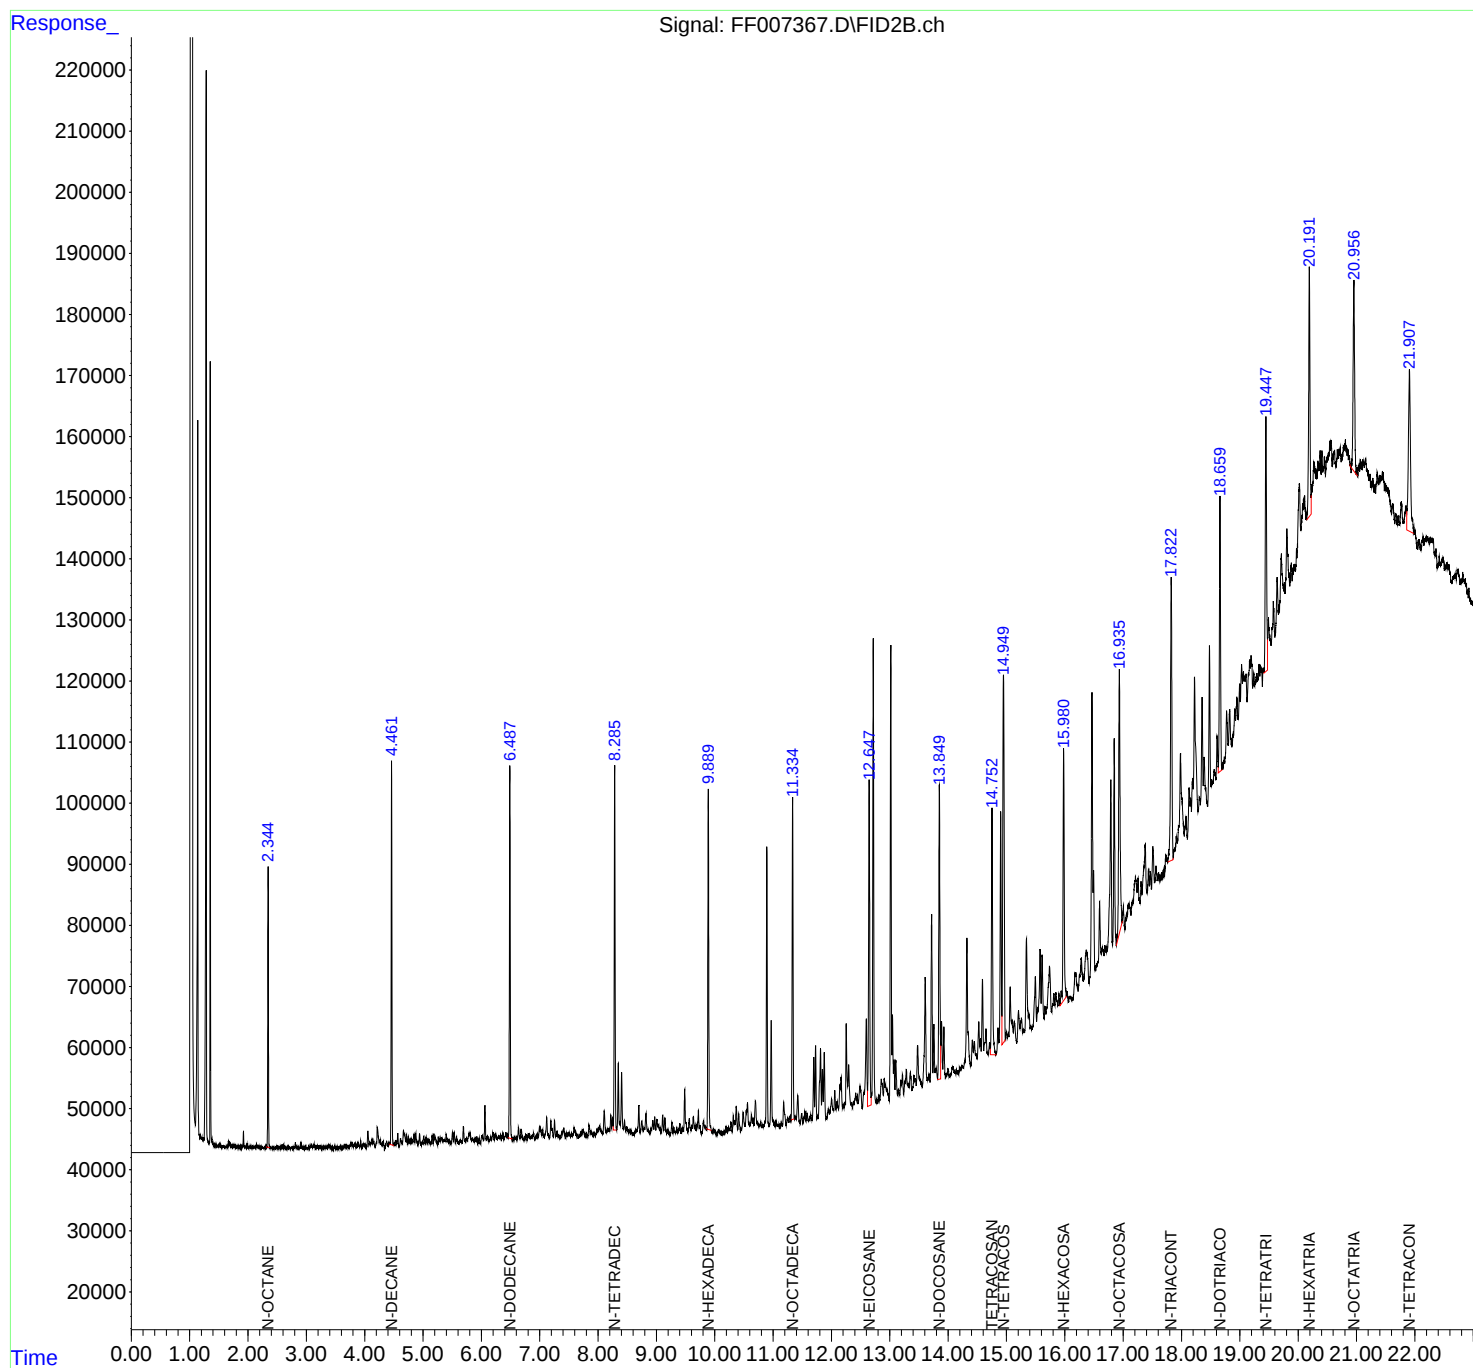

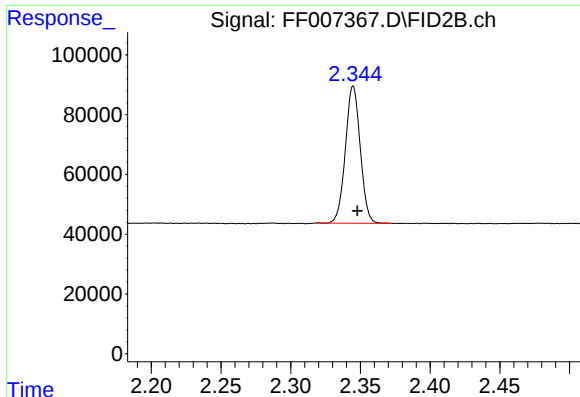


#1 N-OCTANE

R.T.: 2.345 min
Delta R.T.: -0.003 min
Response: 340729
Conc: 2.51 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-4MS


Manual Integrations
APPROVED

Ankita
8/14/2020 12:26:51 PM

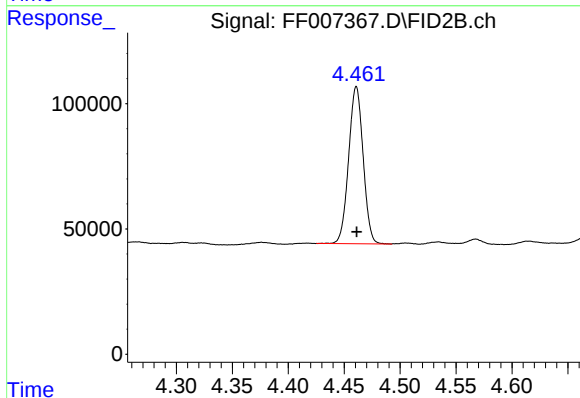


#2 N-DECANE

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 566671
Conc: 4.06 ug/ml

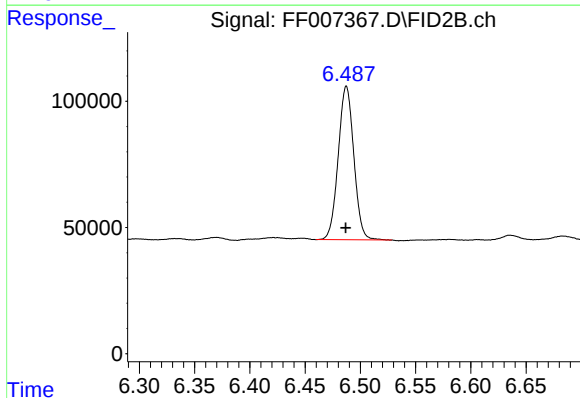


#3 N-DODECANE

R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 598077
Conc: 4.20 ug/ml

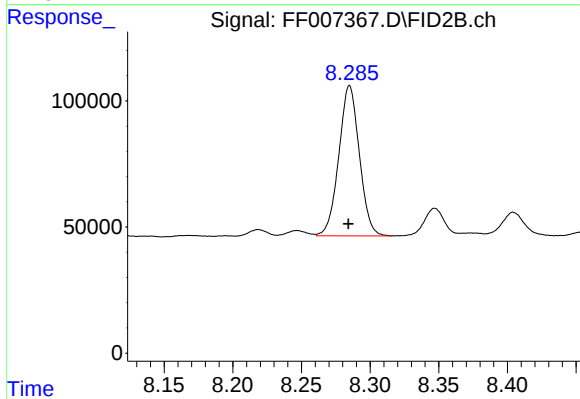

#4 N-TETRADECANE

R.T.: 8.285 min
Delta R.T.: 0.000 min
Response: 620090
Conc: 4.26 ug/ml

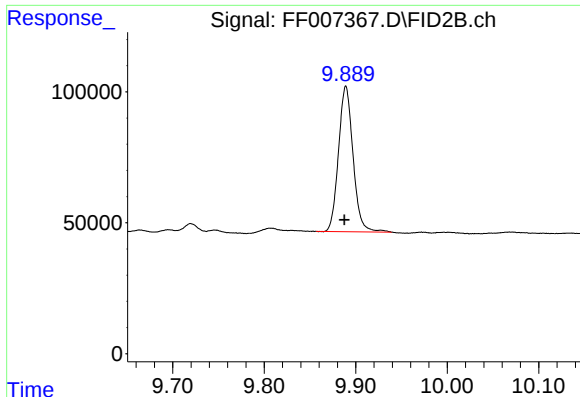


#5 N-HEXADECANE

R.T.: 9.889 min
Delta R.T.: 0.002 min
Response: 614004
Conc: 4.13 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-4MS


Manual Integrations
APPROVED

Ankita
8/14/2020 12:26:51 PM

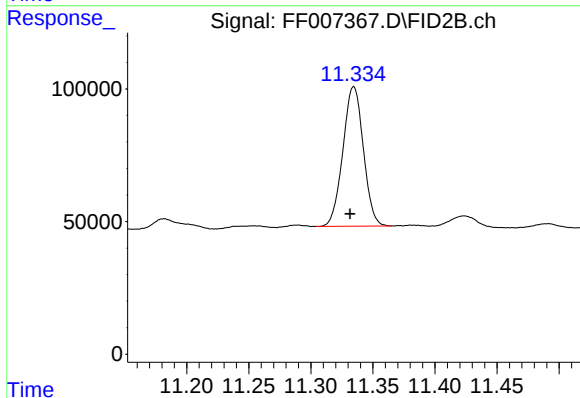


#6 N-OCTADECANE

R.T.: 11.335 min
Delta R.T.: 0.003 min
Response: 604074
Conc: 3.94 ug/ml

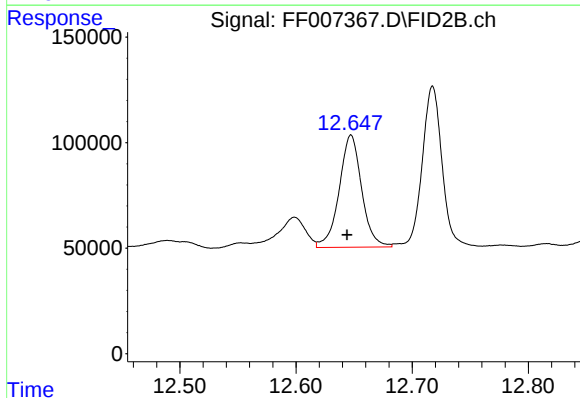


#7 N-EICOSANE

R.T.: 12.647 min
Delta R.T.: 0.003 min
Response: 715984
Conc: 4.63 ug/ml

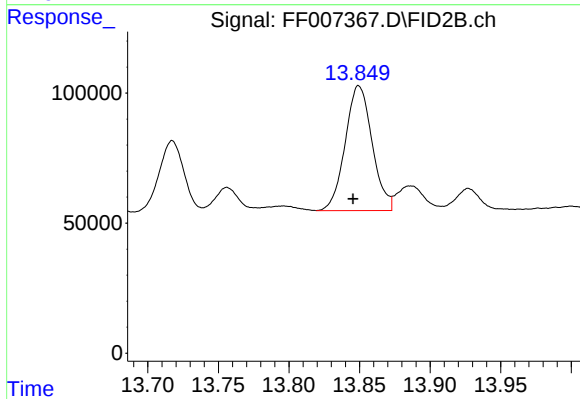

#8 N-DOCOSANE

R.T.: 13.849 min
Delta R.T.: 0.003 min
Response: 639982
Conc: 4.10 ug/ml m

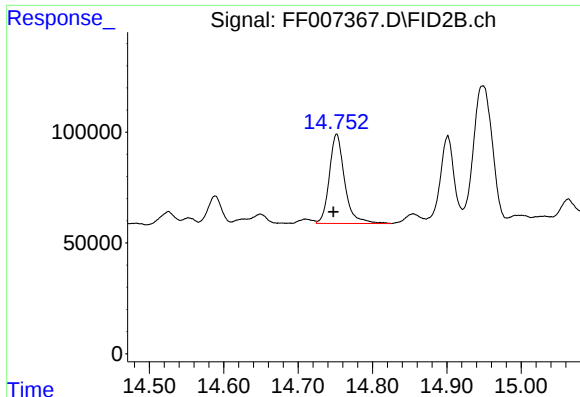


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.752 min
Delta R.T.: 0.004 min
Response: 574874
Conc: 4.21 ug/ml m

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-4MS


Manual Integrations
APPROVED

Ankita
8/14/2020 12:26:51 PM

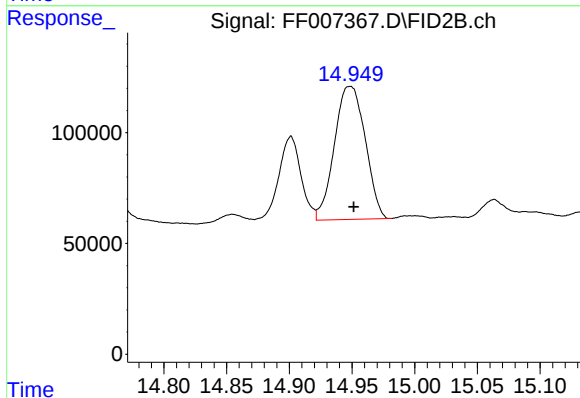


#10 N-TETRACOSANE

R.T.: 14.948 min
Delta R.T.: -0.003 min
Response: 1027954
Conc: 6.51 ug/ml

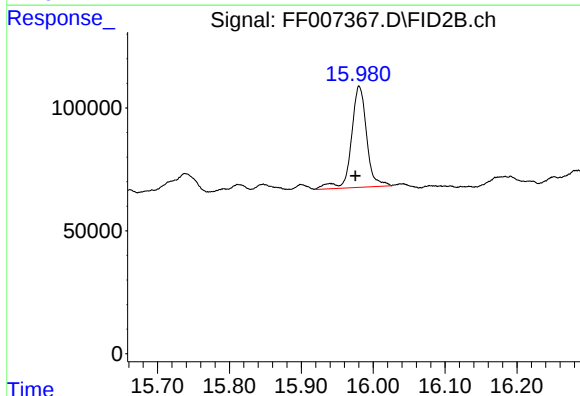


#11 N-HEXACOSANE

R.T.: 15.981 min
Delta R.T.: 0.005 min
Response: 605343
Conc: 3.86 ug/ml

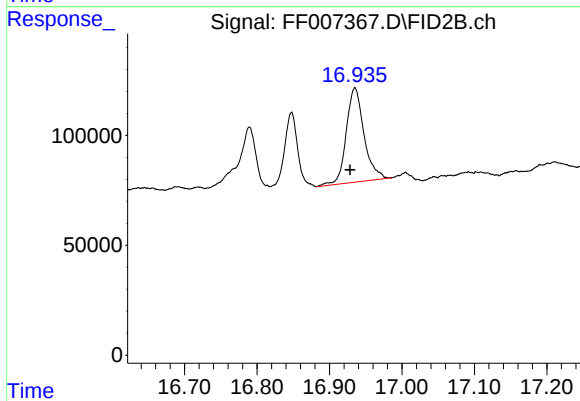

#12 N-OCTACOSANE

R.T.: 16.935 min
Delta R.T.: 0.007 min
Response: 731585
Conc: 4.66 ug/ml

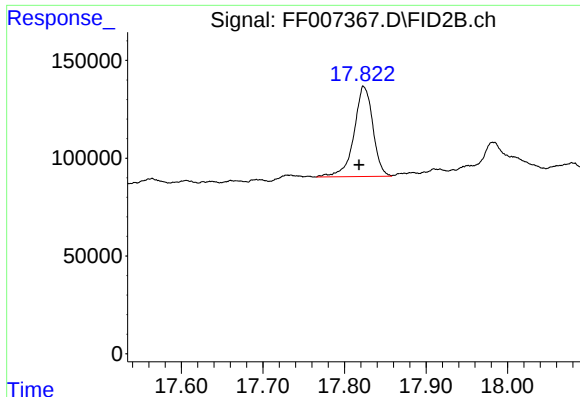


#13 N-TRIACONTANE

R.T.: 17.822 min
Delta R.T.: 0.004 min
Response: 740645
Conc: 4.72 ug/ml m

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-4MS


Manual Integrations
APPROVED

Ankita
8/14/2020 12:26:51 PM

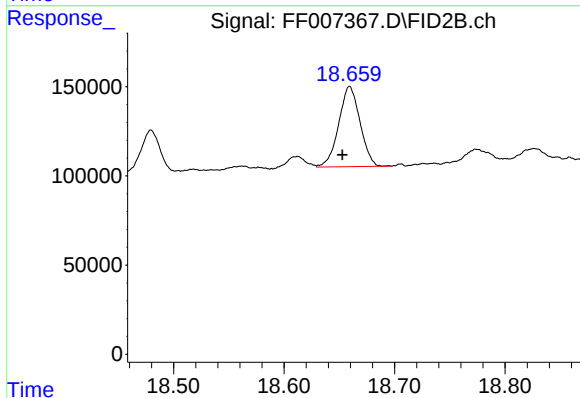


#14 N-DOTRIACONTANE

R.T.: 18.659 min
Delta R.T.: 0.007 min
Response: 603999
Conc: 4.08 ug/ml

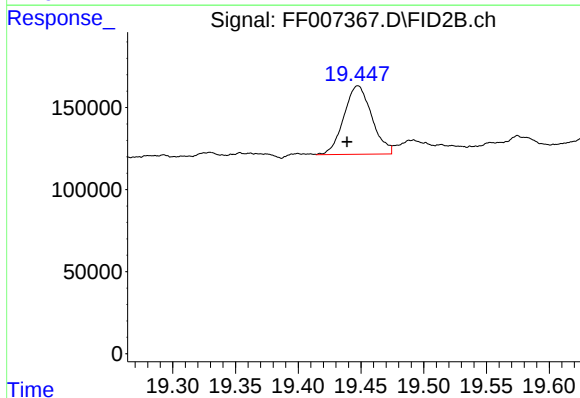


#15 N-TETRATRIACONTANE

R.T.: 19.447 min
Delta R.T.: 0.008 min
Response: 646687
Conc: 5.35 ug/ml m

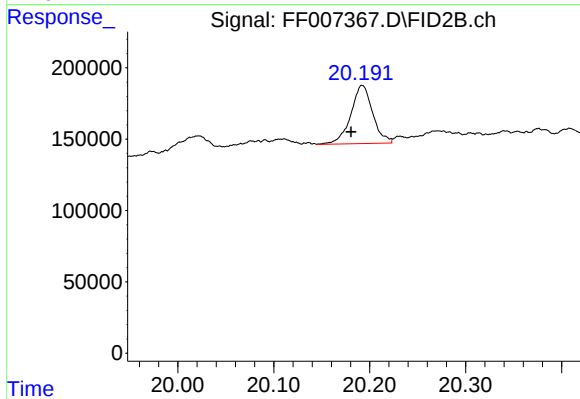

#16 N-HEXATRIACONTANE

R.T.: 20.191 min
Delta R.T.: 0.011 min
Response: 649720
Conc: 7.02 ug/ml m

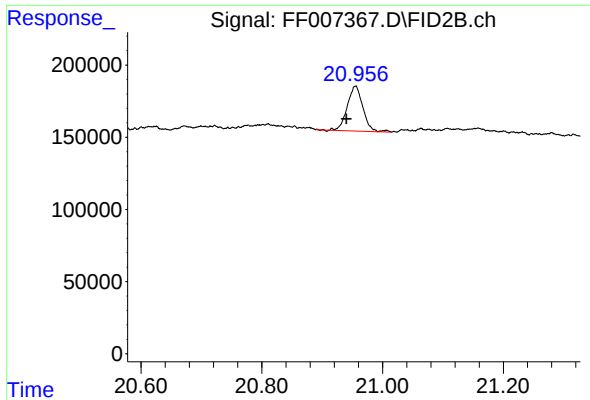


#17 N-OCTATRIACONTANE

R.T.: 20.955 min
Delta R.T.: 0.015 min
Response: 557168
Conc: 7.84 ug/ml

Instrument :
FID_F
ClientSampleId :
CAR-WASH-AREA-3-TPH-4MS

Manual Integrations
APPROVED

Ankita
8/14/2020 12:26:51 PM

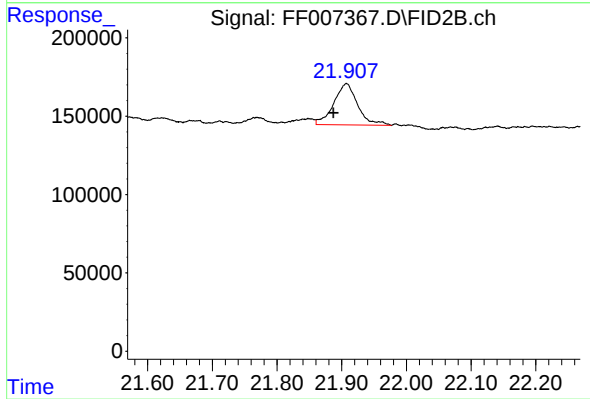

#18 N-TETRACONTANE

R.T.: 21.907 min
Delta R.T.: 0.021 min
Response: 673934
Conc: 10.08 ug/ml