

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
 Data File : FF008892.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2021 12:03
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 22:26:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3)	N-DODECANE	6.516	2461540 18.552 ug/ml
12)	N-OCTACOSANE	16.909	2509357 18.758 ug/ml
13)	N-TRIACONTANE	17.794	103706 0.793 ug/ml
14)	N-DOTRIACONTANE	18.624	131435 1.062 ug/ml
15)	N-TETRATRIACONTANE	19.406	121713 1.045 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
Data File : FF008892.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2021 12:03
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 22:26:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

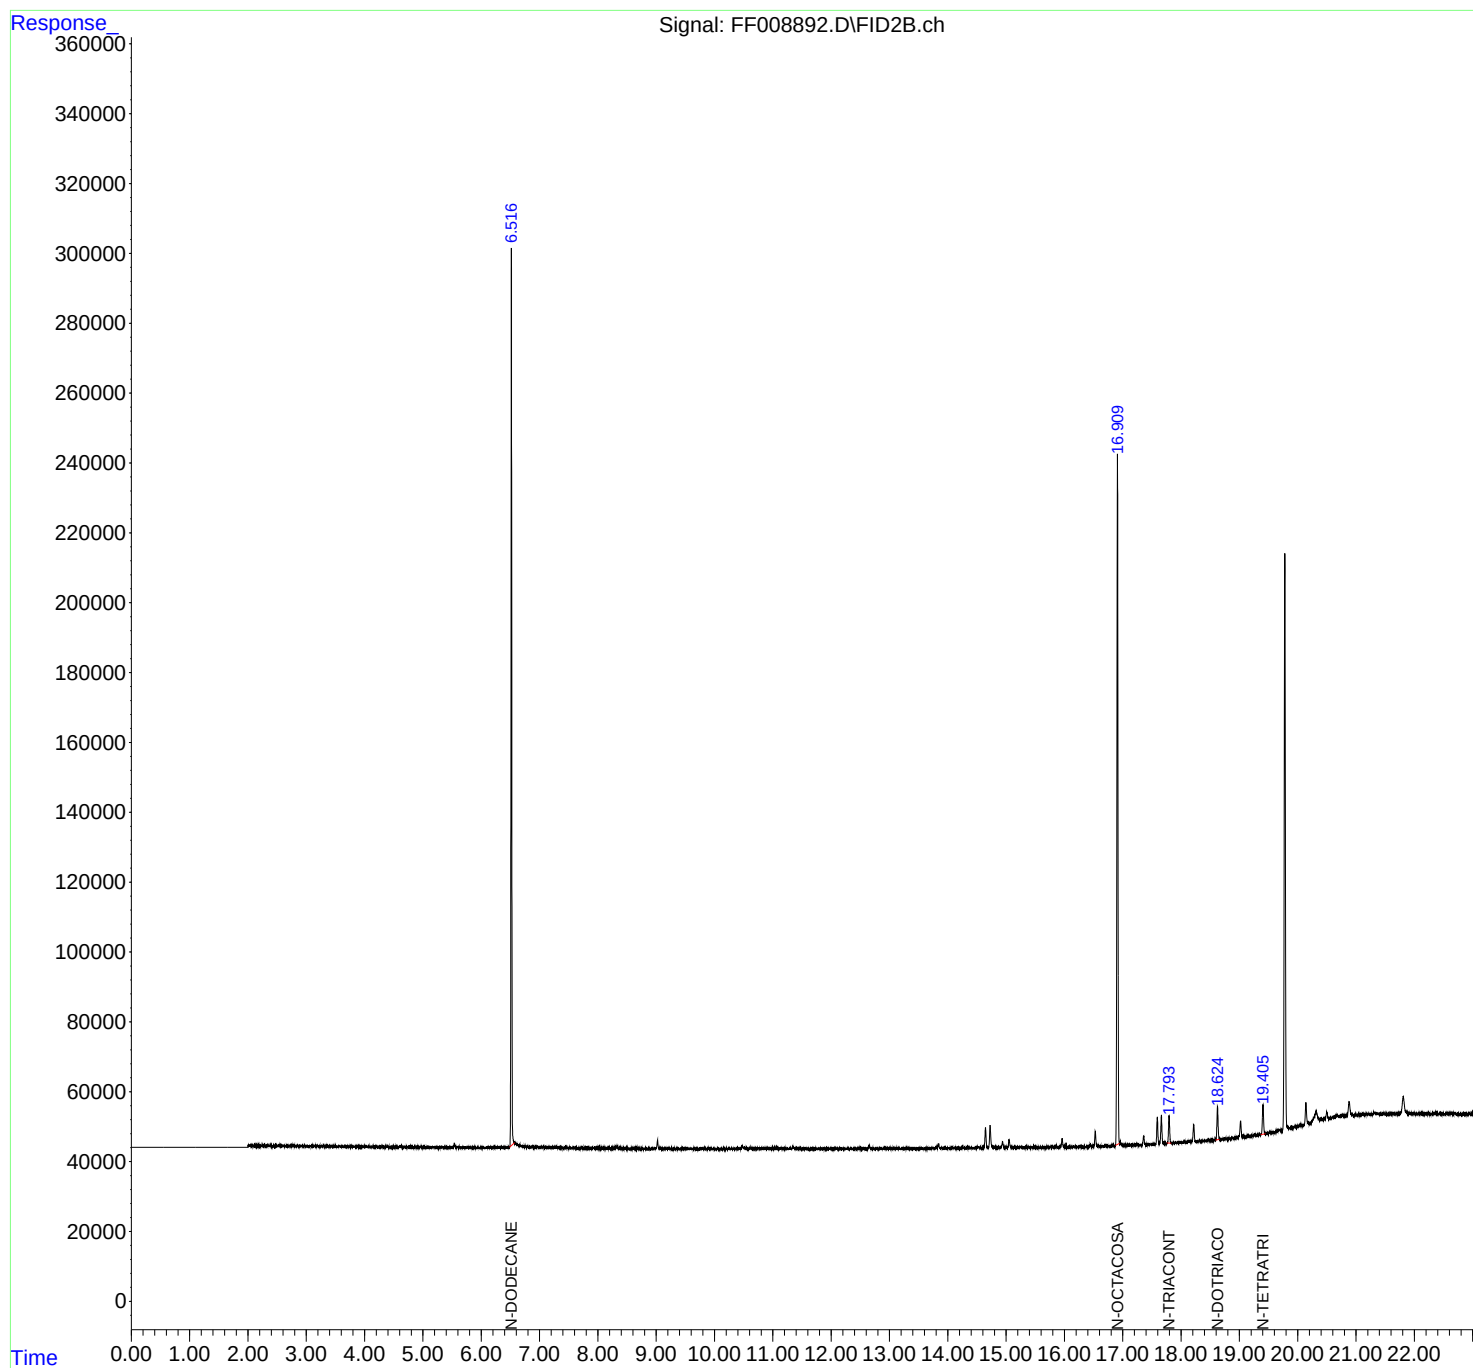


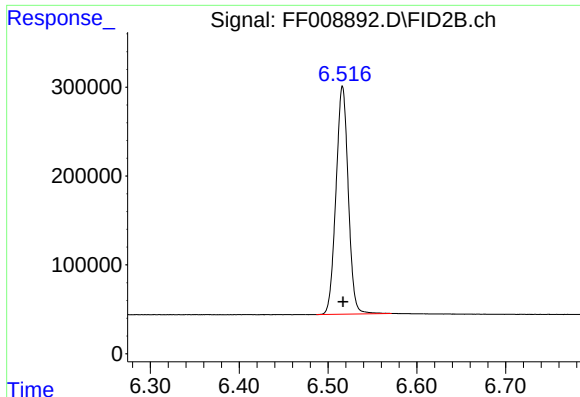

#3 N-DODECANE


R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 2461540
Conc: 18.55 ug/ml

Instrument :
FID_F
ClientSampleId :

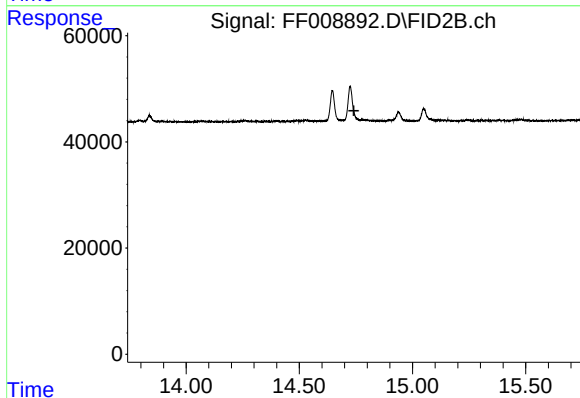


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.741 min
Response: 0
Conc: N.D.

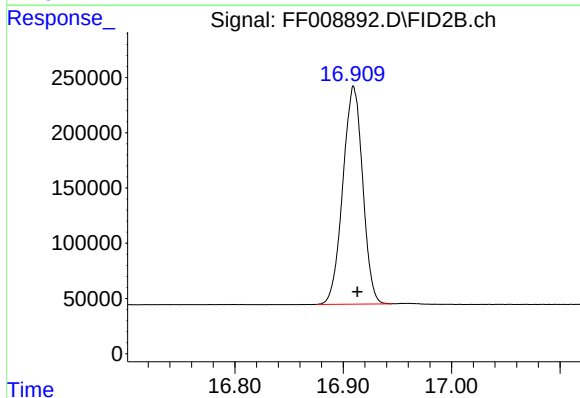


#12 N-OCTACOSANE

R.T.: 16.909 min
Delta R.T.: -0.004 min
Response: 2509357
Conc: 18.76 ug/ml

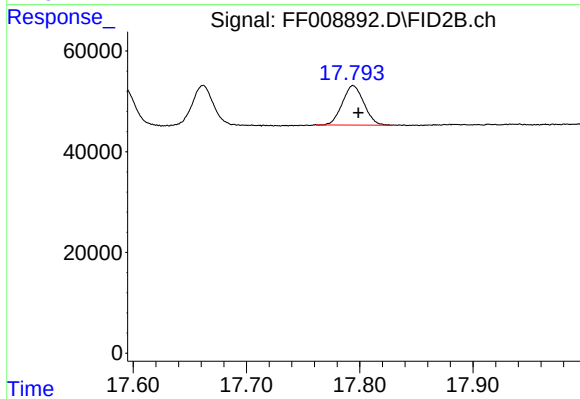

#13 N-TRIACONTANE


R.T.: 17.794 min
Delta R.T.: -0.005 min
Response: 103706
Conc: 0.79 ug/ml

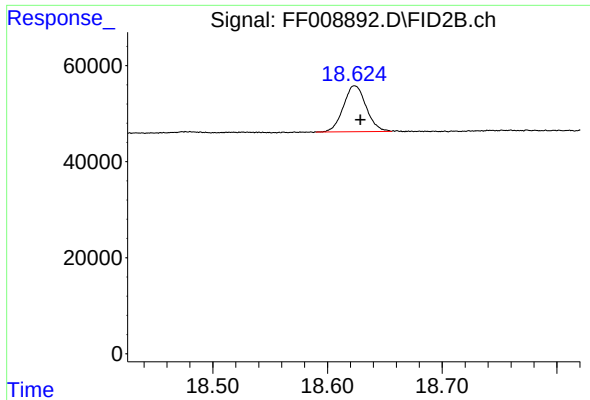

#14 N-DOTRIACONTANE

R.T.: 18.624 min
Delta R.T.: -0.005 min
Response: 131435
Conc: 1.06 ug/ml

Instrument :
FID_F
ClientSampleId :

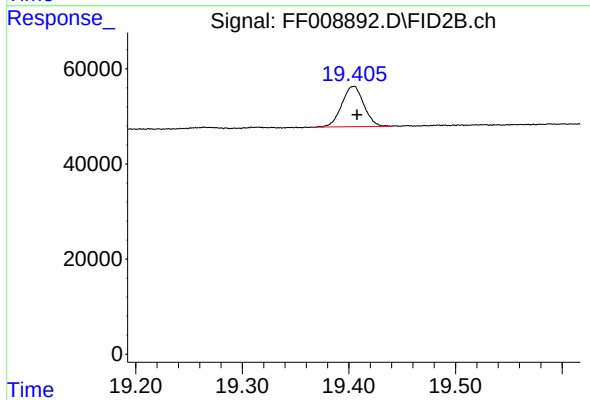

#15 N-TETRATRIACONTANE

R.T.: 19.406 min
Delta R.T.: -0.002 min
Response: 121713
Conc: 1.04 ug/ml