

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
 Data File : FF008895.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2021 15:46
 Operator : DD\AJ
 Sample : M3407-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 22:27:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	1935792	16.157 ug/ml
Target Compounds			
4) N-TETRADECANE	8.272	138893	1.035 ug/ml
6) N-OCTADECANE	11.353	90427	0.644 ug/ml
7) N-EICOSANE	12.717f	353388	2.525 ug/ml
10) N-TETRACOSANE	14.933	228916	1.654 ug/ml
11) N-HEXACOSANE	15.934	24956	0.183 ug/ml
14) N-DOTRIACONTANE	18.623	255979	2.069 ug/ml
15) N-TETRATRIACONTANE	19.448	265676	2.281 ug/ml
16) N-HEXATRIACONTANE	20.094f	115014	1.083 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
Data File : FF008895.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2021 15:46
Operator : DD\AJ
Sample : M3407-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 22:27:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

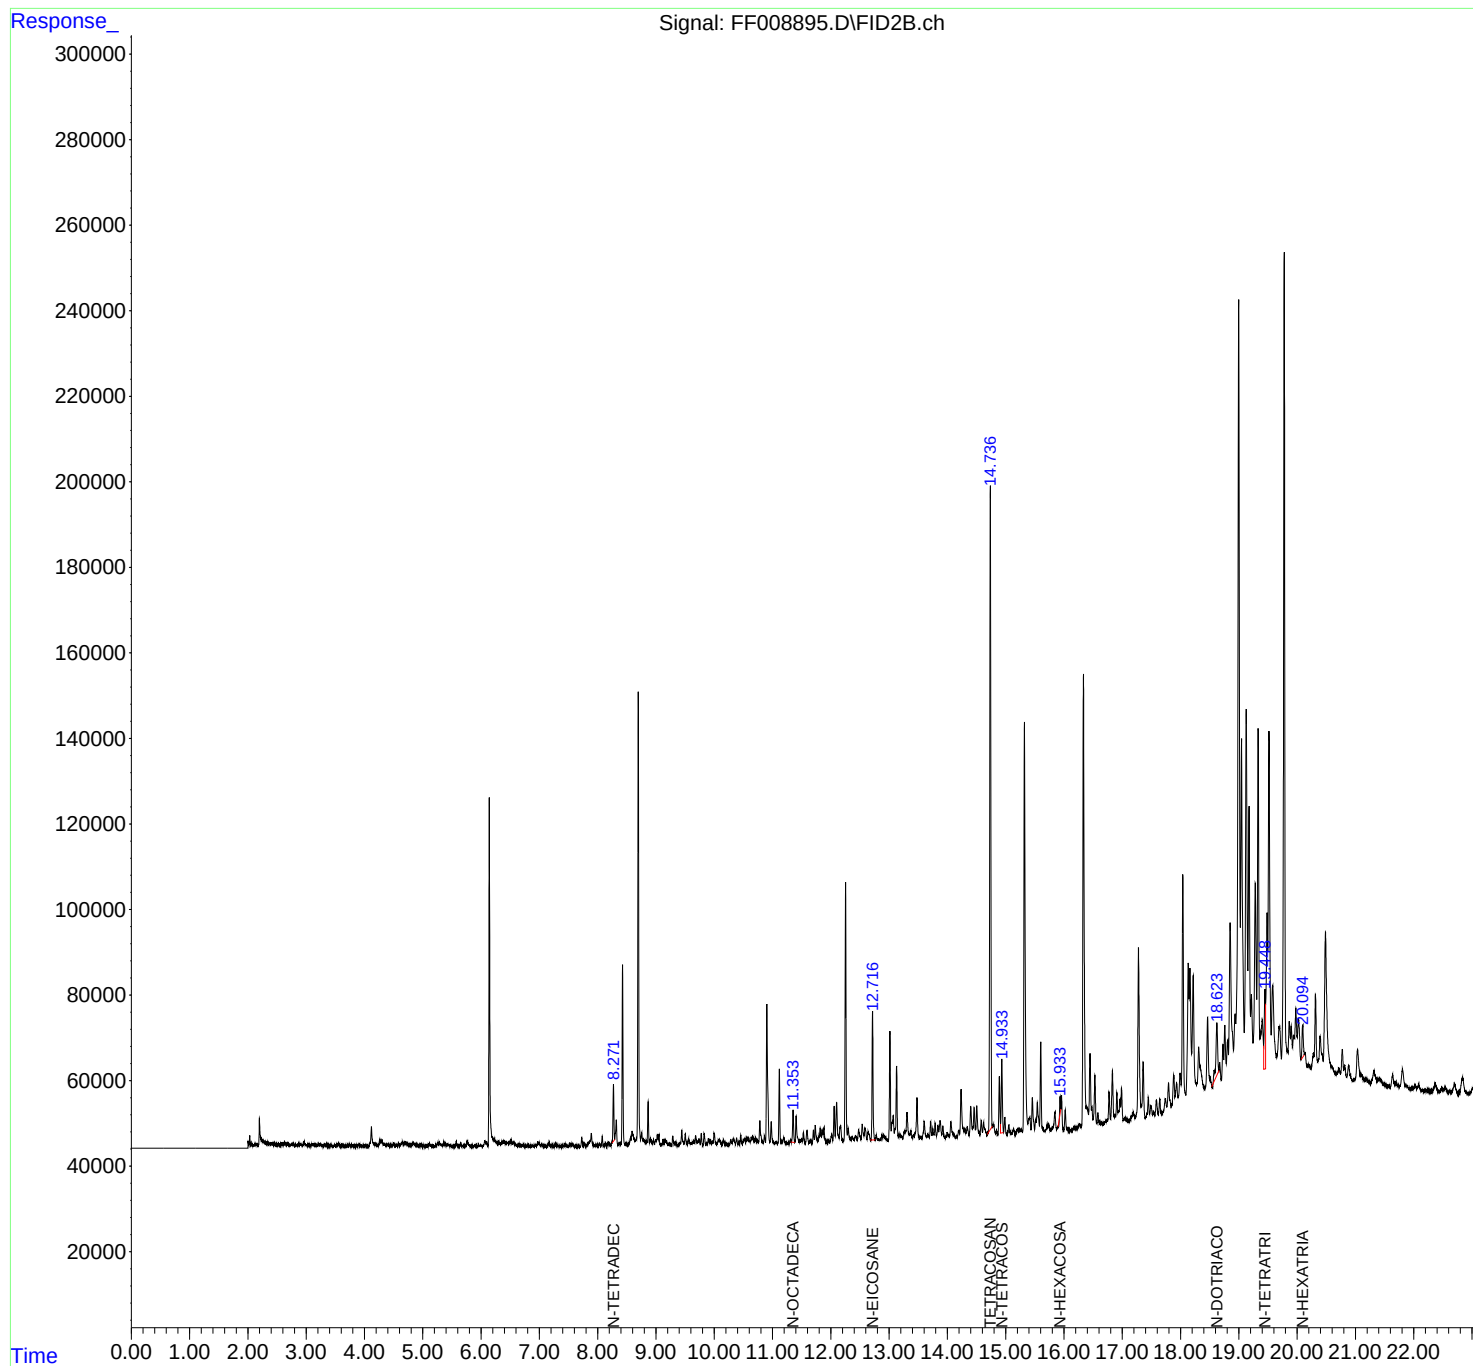


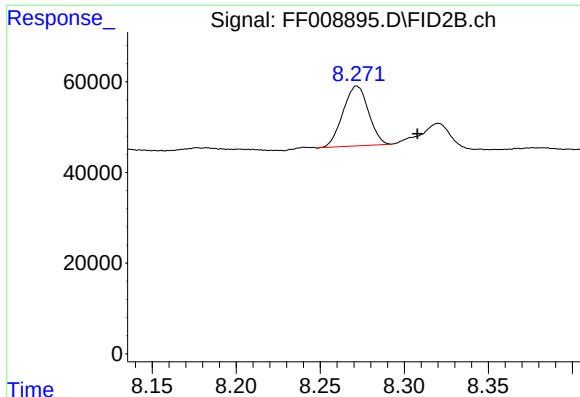

#4 N-TETRADECANE


R.T.: 8.272 min
Delta R.T.: -0.036 min
Response: 138893
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :

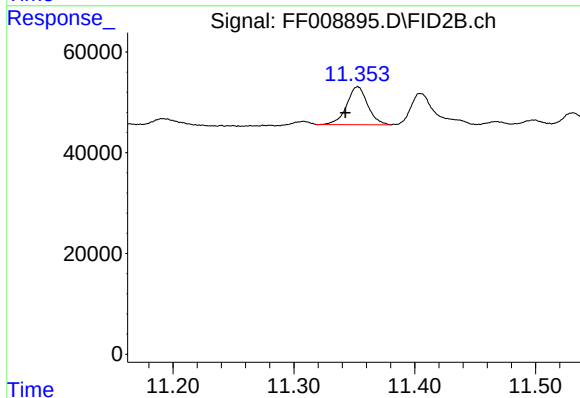


#6 N-OCTADECANE

R.T.: 11.353 min
Delta R.T.: 0.010 min
Response: 90427
Conc: 0.64 ug/ml

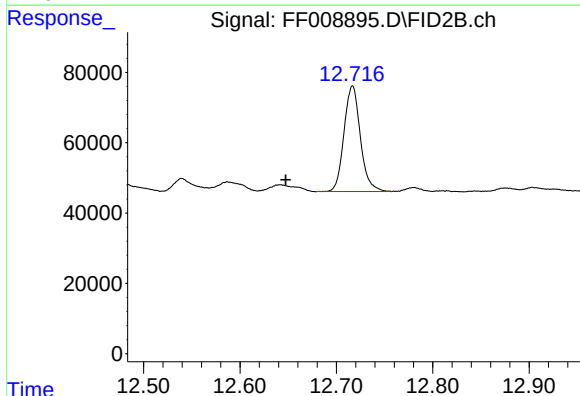


#7 N-EICOSANE

R.T.: 12.717 min
Delta R.T.: 0.069 min
Response: 353388
Conc: 2.52 ug/ml

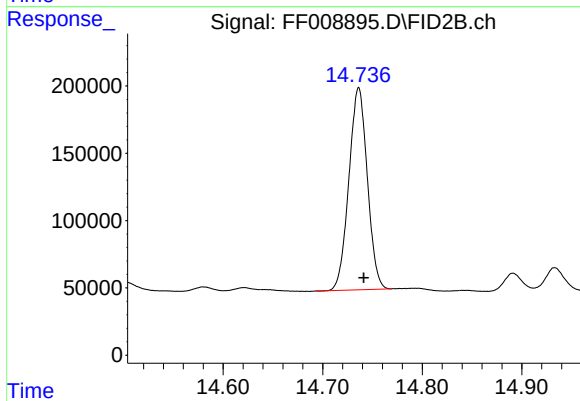

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.736 min
Delta R.T.: -0.005 min
Response: 1935792
Conc: 16.16 ug/ml

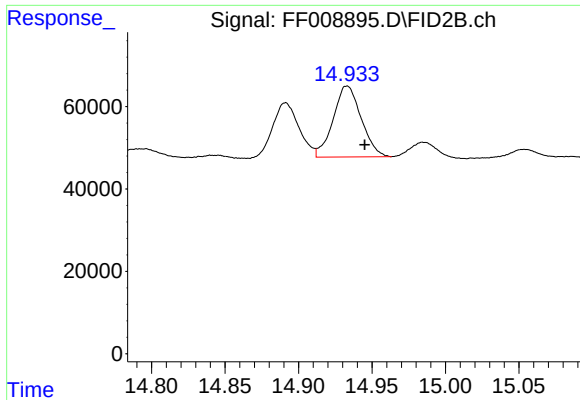

#10 N-TETRACOSANE


R.T.: 14.933 min
Delta R.T.: -0.012 min
Response: 228916
Conc: 1.65 ug/ml

Instrument :
FID_F
ClientSampleId :

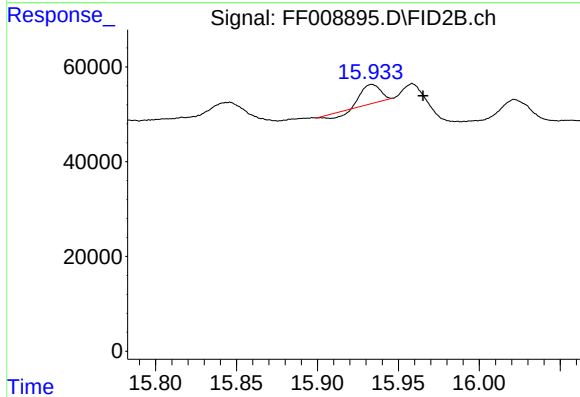


#11 N-HEXACOSANE

R.T.: 15.934 min
Delta R.T.: -0.032 min
Response: 24956
Conc: 0.18 ug/ml

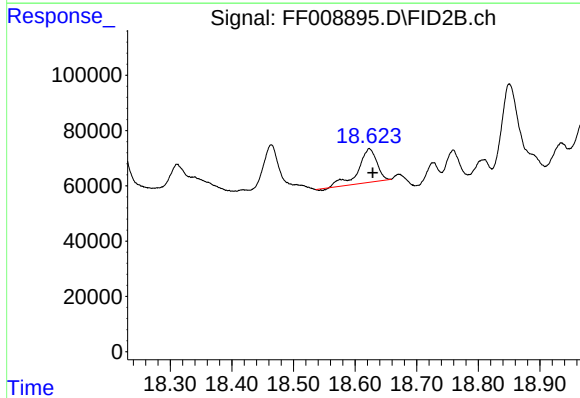


#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: -0.005 min
Response: 255979
Conc: 2.07 ug/ml

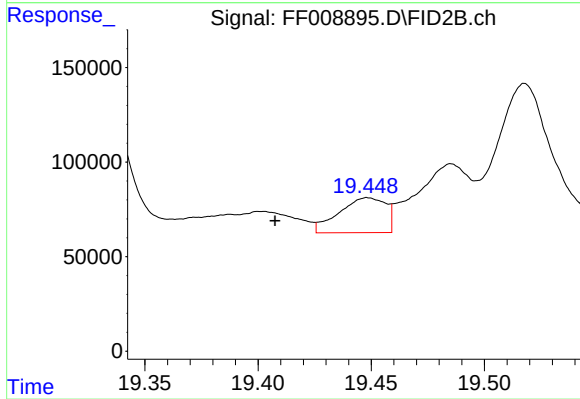

#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: 0.041 min
Response: 265676
Conc: 2.28 ug/ml

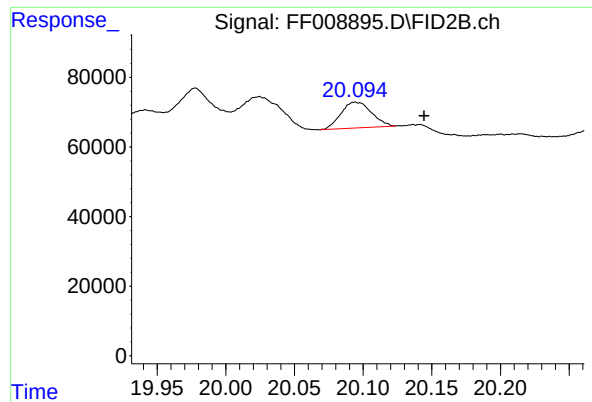

#16 N-HEXATRIACONTANE

R.T.: 20.094 min
Delta R.T.: -0.050 min
Response: 115014
Conc: 1.08 ug/ml

Instrument :
FID_F
ClientSampleId :