

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
 Data File : FF008900.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2021 18:26
 Operator : DD\AJ
 Sample : M3407-11
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 22:28:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.739	1461158	12.196 ug/ml
Target Compounds			
4) N-TETRADECANE	8.322	204388	1.523 ug/ml
6) N-OCTADECANE	11.358	139787	0.996 ug/ml
7) N-EICOSANE	12.665	176639	1.262 ug/ml
10) N-TETRACOSANE	14.937	445489	3.218 ug/ml
11) N-HEXACOSANE	15.963	128020	0.941 ug/ml
12) N-OCTACOSANE	16.913	69663	0.521 ug/ml
13) N-TRIACONTANE	17.797	451120	3.452 ug/ml
14) N-DOTRIACONTANE	18.628	970113	7.842 ug/ml
15) N-TETRATRIACONTANE	19.406	2029097	17.418 ug/ml
16) N-HEXATRIACONTANE	20.097	950995	8.951 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
Data File : FF008900.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2021 18:26
Operator : DD\AJ
Sample : M3407-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 22:28:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

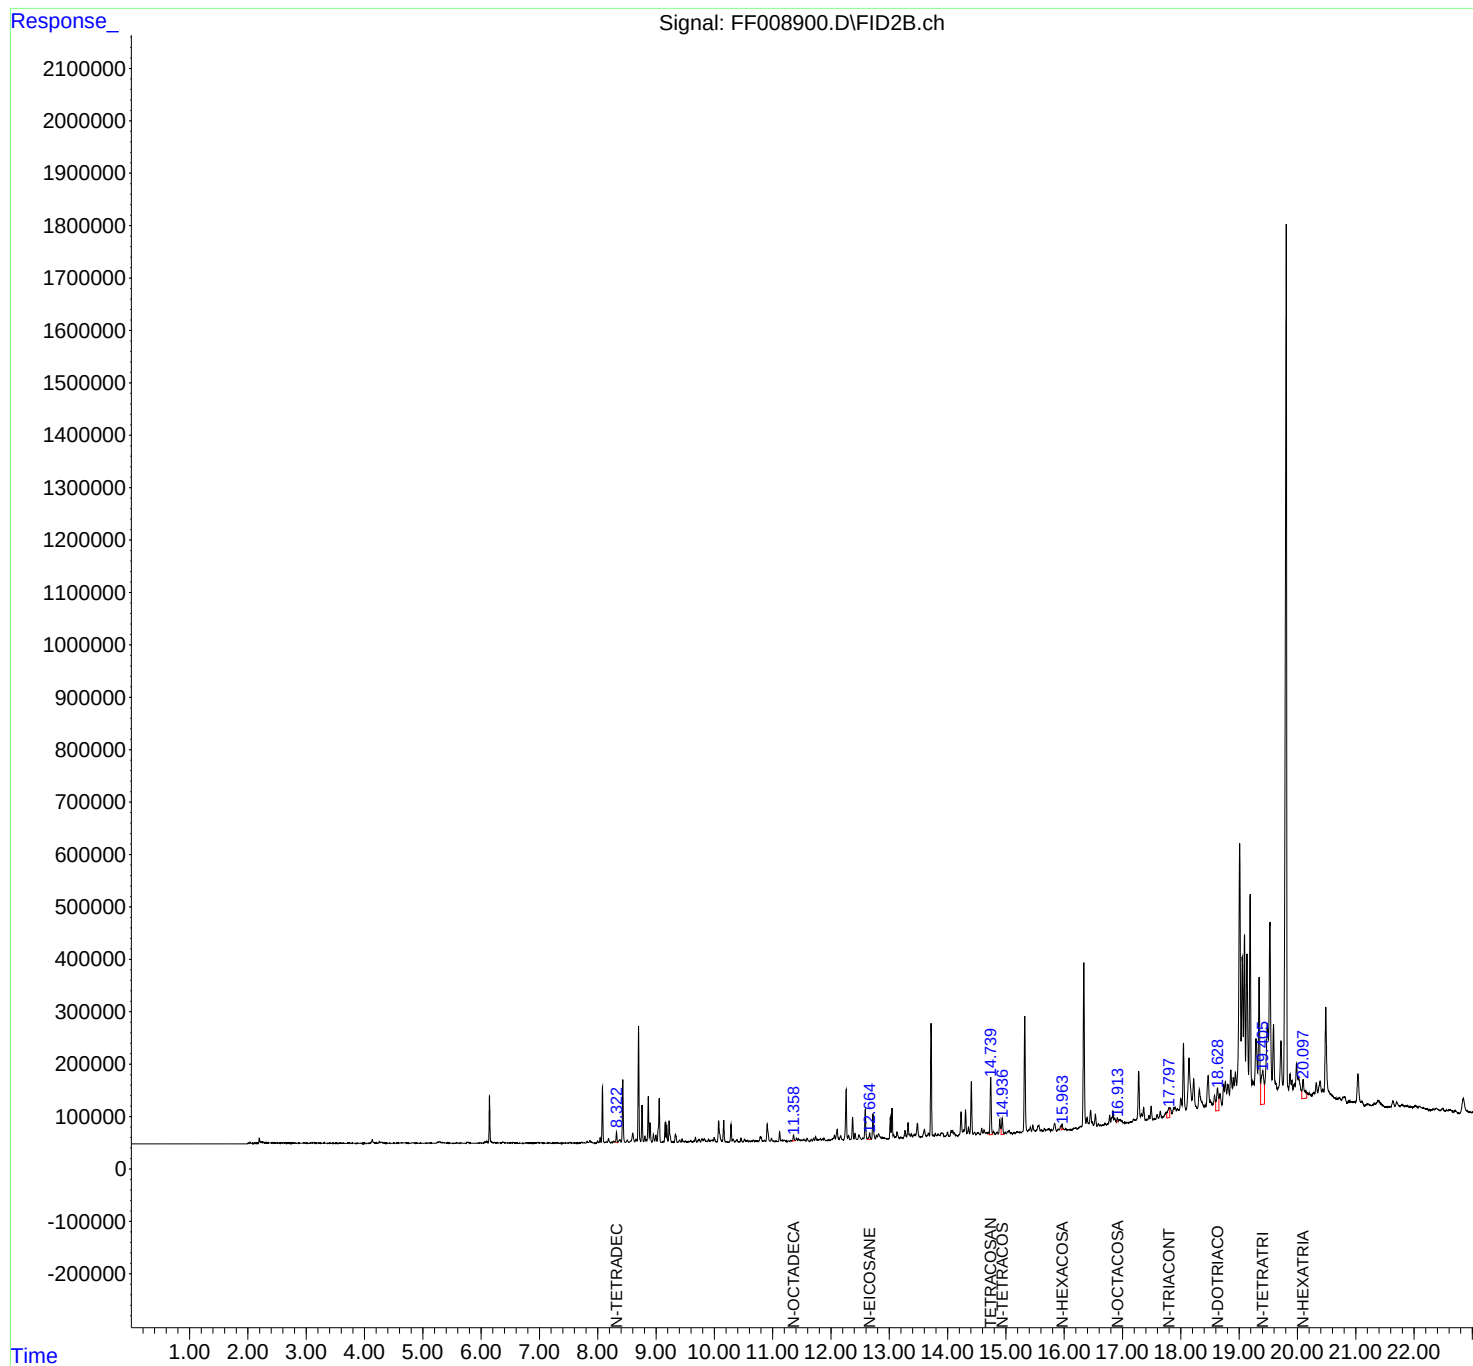


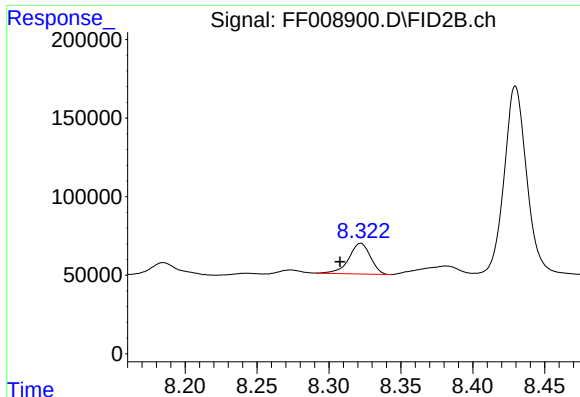

#4 N-TETRADECANE


R.T.: 8.322 min
Delta R.T.: 0.015 min
Response: 204388
Conc: 1.52 ug/ml

Instrument :
FID_F
ClientSampleId :

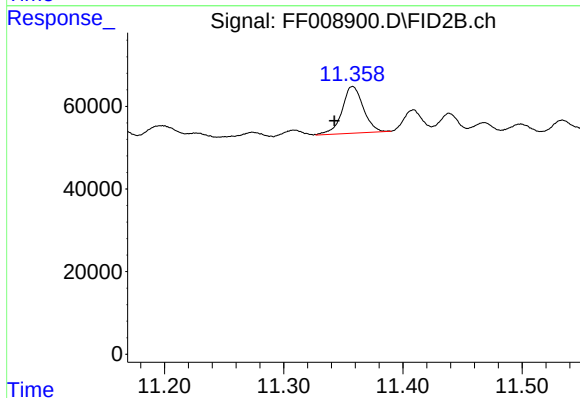


#6 N-OCTADECANE

R.T.: 11.358 min
Delta R.T.: 0.015 min
Response: 139787
Conc: 1.00 ug/ml

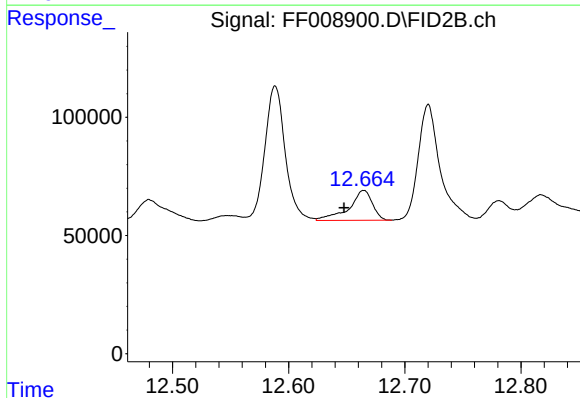


#7 N-EICOSANE

R.T.: 12.665 min
Delta R.T.: 0.017 min
Response: 176639
Conc: 1.26 ug/ml

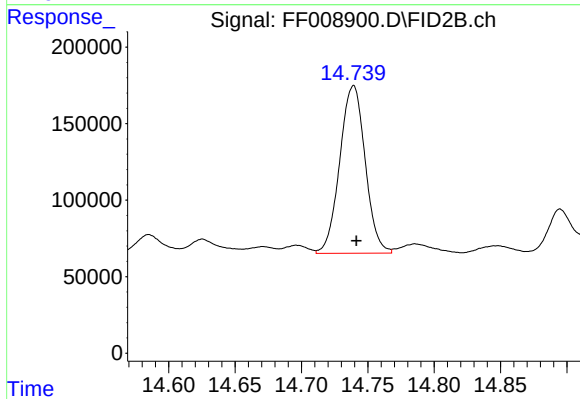

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.739 min
Delta R.T.: -0.002 min
Response: 1461158
Conc: 12.20 ug/ml

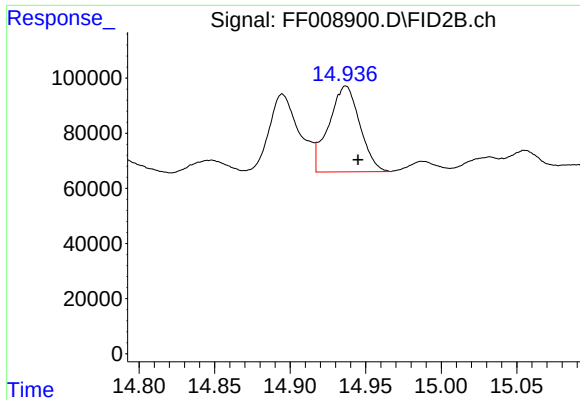

#10 N-TETRACOSANE


R.T.: 14.937 min
Delta R.T.: -0.008 min
Response: 445489
Conc: 3.22 ug/ml

Instrument :
FID_F
ClientSampleId :

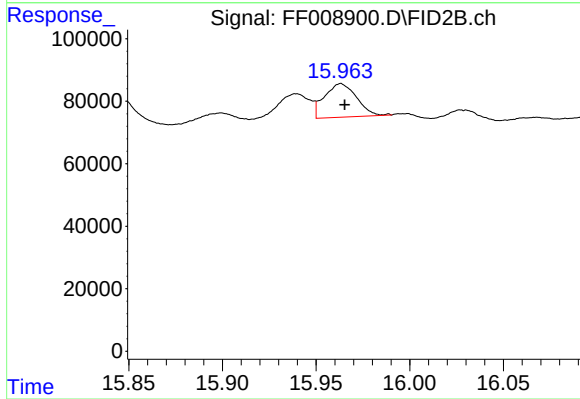


#11 N-HEXACOSANE

R.T.: 15.963 min
Delta R.T.: -0.002 min
Response: 128020
Conc: 0.94 ug/ml

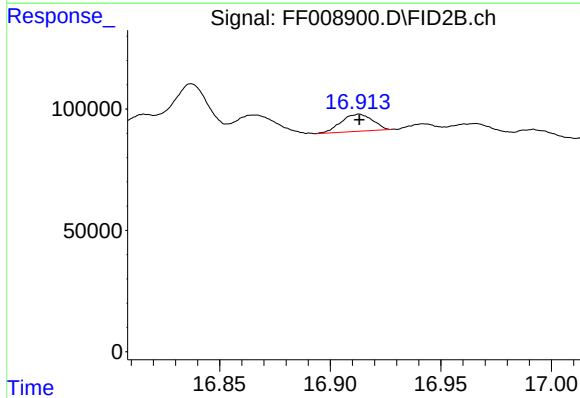


#12 N-OCTACOSANE

R.T.: 16.913 min
Delta R.T.: 0.000 min
Response: 69663
Conc: 0.52 ug/ml

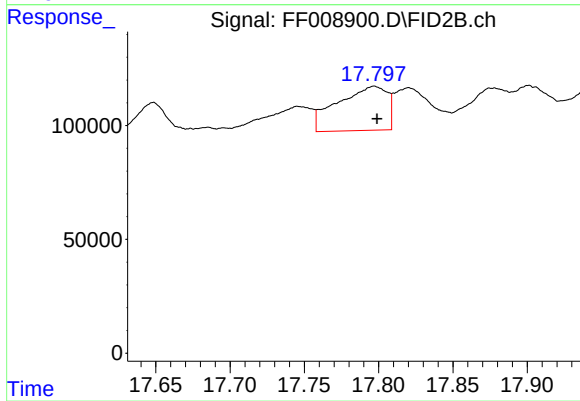

#13 N-TRIACONTANE


R.T.: 17.797 min
Delta R.T.: -0.002 min
Response: 451120
Conc: 3.45 ug/ml

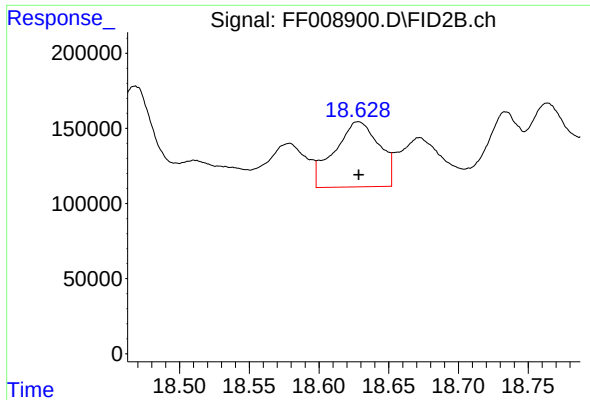

#14 N-DOTRIACONTANE


R.T.: 18.628 min
Delta R.T.: 0.000 min
Response: 970113
Conc: 7.84 ug/ml

Instrument :
FID_F
ClientSampleId :

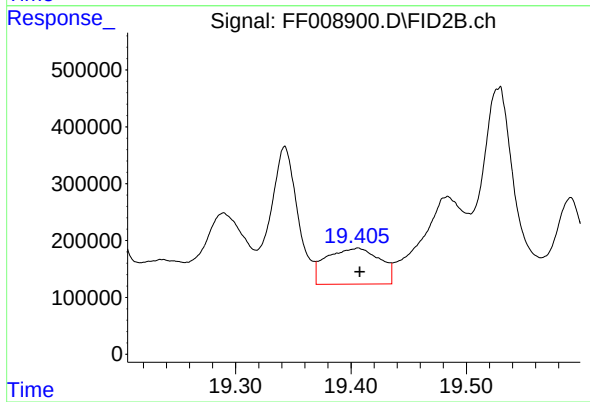

#15 N-TETRATRIACONTANE

R.T.: 19.406 min
Delta R.T.: -0.001 min
Response: 2029097
Conc: 17.42 ug/ml

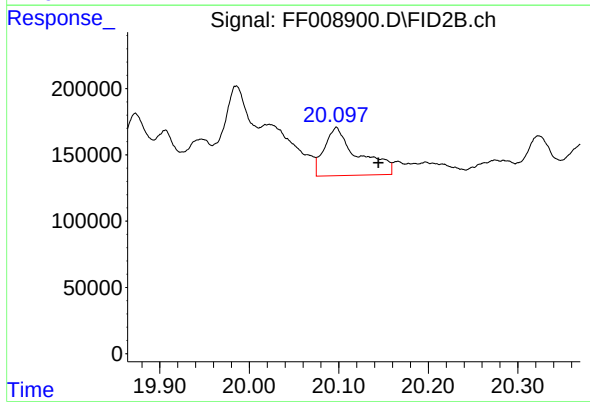

#16 N-HEXATRIACONTANE

R.T.: 20.097 min
Delta R.T.: -0.047 min
Response: 950995
Conc: 8.95 ug/ml