

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
 Data File : FF008910.D
 Signal(s) : FID2B.ch
 Acq On : 13 Aug 2021 23:45
 Operator : DD\AJ
 Sample : M3408-14
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 14 01:56:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	2378929	19.856 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.939	90874	0.656 ug/ml
11) N-HEXACOSANE	15.960	89674	0.659 ug/ml
14) N-DOTRIACONTANE	18.621	116930	0.945 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081321\
Data File : FF008910.D
Signal(s) : FID2B.ch
Acq On : 13 Aug 2021 23:45
Operator : DD\AJ
Sample : M3408-14
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 01:56:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

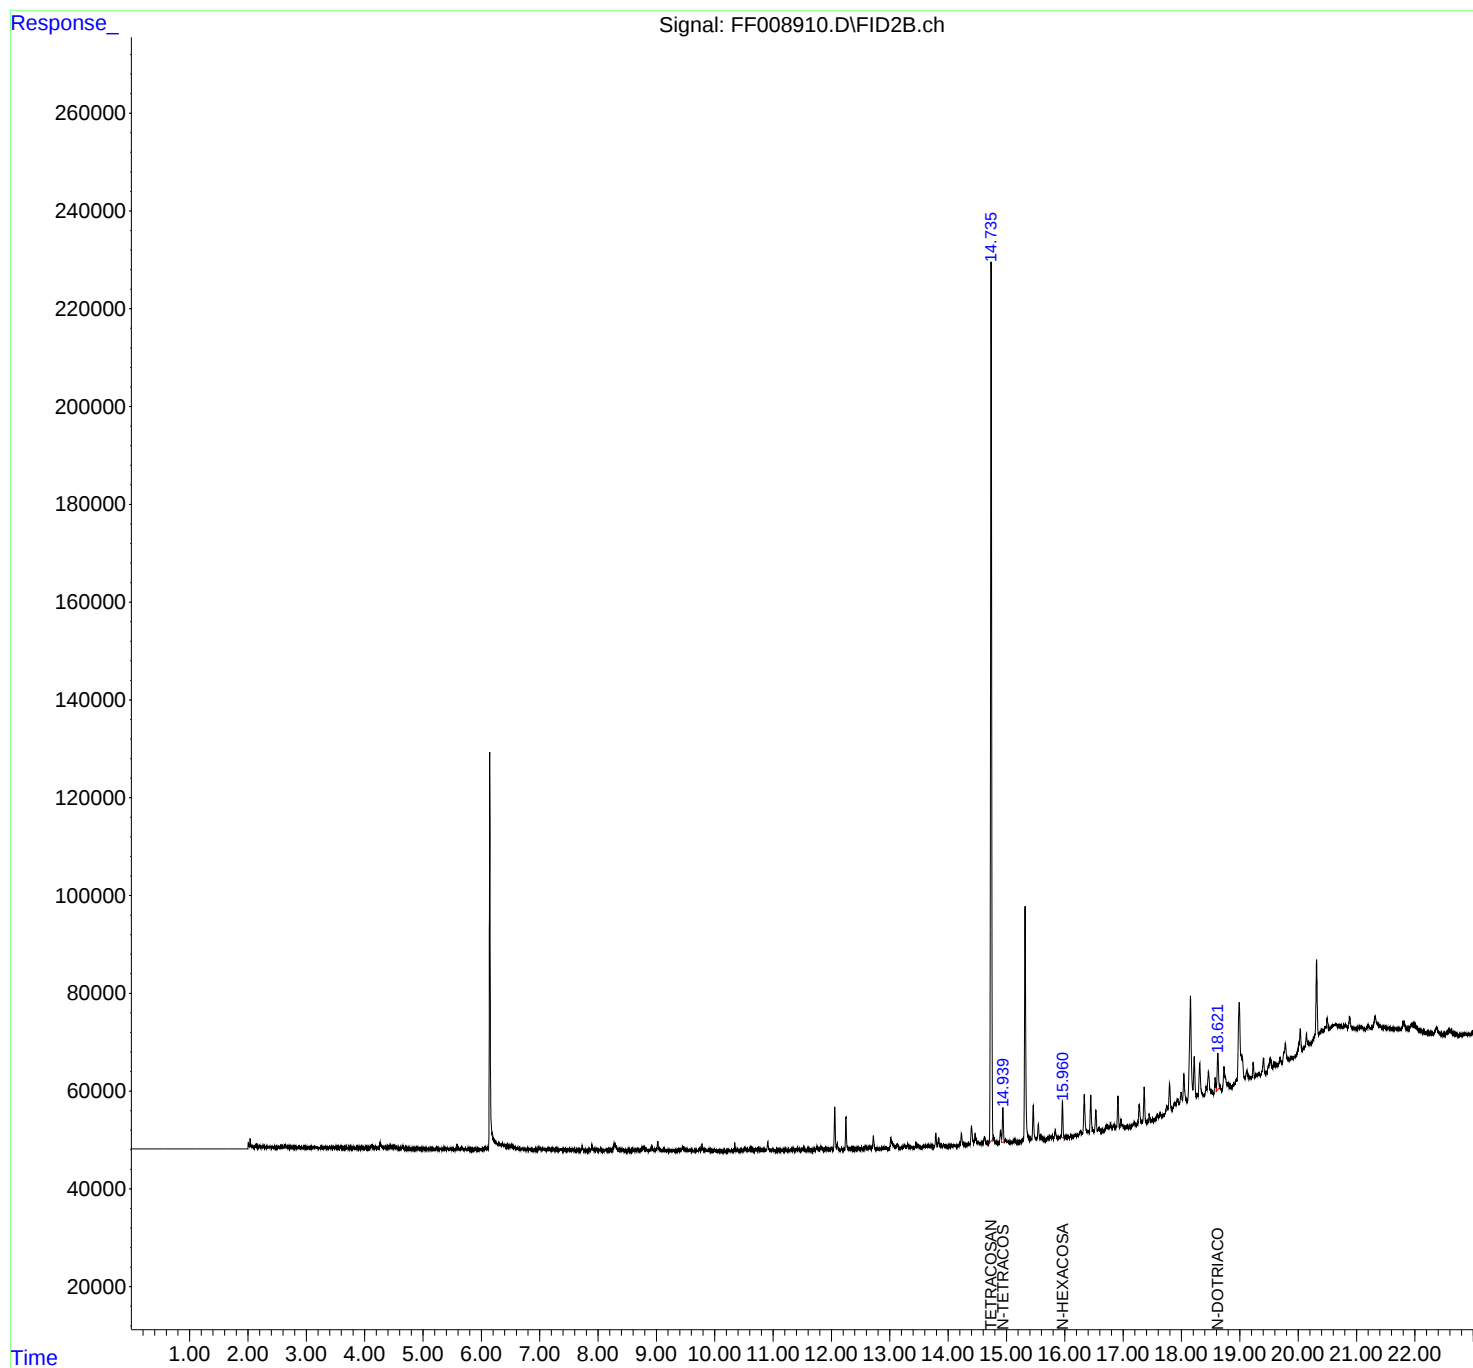


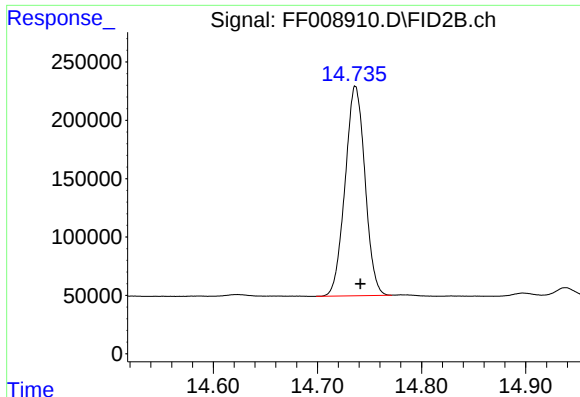

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.736 min
Delta R.T.: -0.005 min
Response: 2378929
Conc: 19.86 ug/ml

Instrument :
FID_F
ClientSampleId :

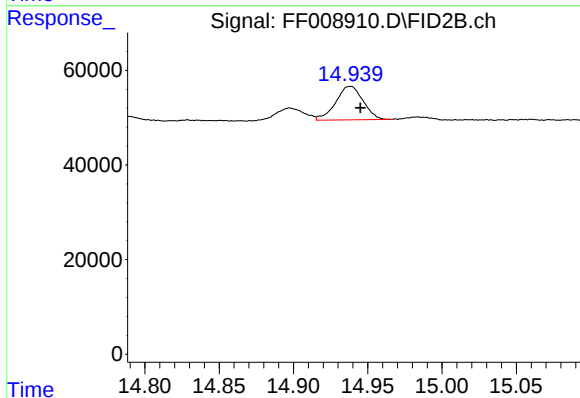


#10 N-TETRACOSANE

R.T.: 14.939 min
Delta R.T.: -0.006 min
Response: 90874
Conc: 0.66 ug/ml

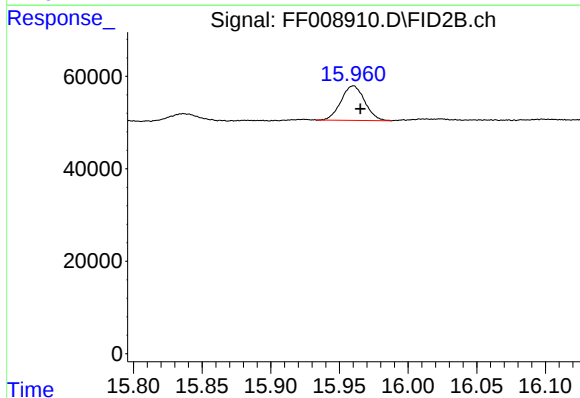

#11 N-HEXACOSANE

R.T.: 15.960 min
Delta R.T.: -0.005 min
Response: 89674
Conc: 0.66 ug/ml

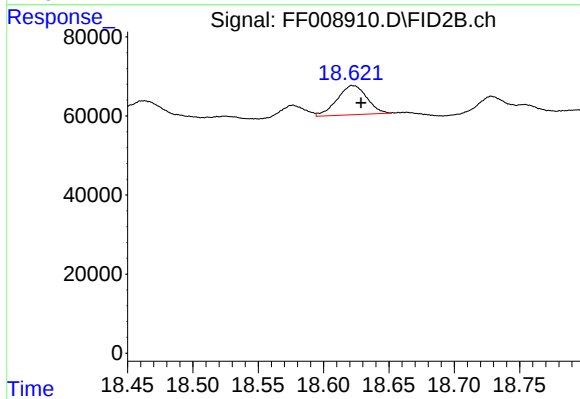

#14 N-DOTRIACONTANE

R.T.: 18.621 min
Delta R.T.: -0.007 min
Response: 116930
Conc: 0.95 ug/ml