

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081418\
Data File : FF001867.D
Signal(s) : FID2B.ch
Acq On : 14 Aug 2018 11:08
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 15 08:10:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.198	366735	2.461 ug/ml
8)	N-DOCOSANE	13.407	264153	1.808 ug/ml
10)	N-TETRACOSANE	14.478	17456204	122.369 ug/ml
11)	N-HEXACOSANE	15.528	172890	1.227 ug/ml
12)	N-OCTACOSANE	16.477	171659	1.224 ug/ml
13)	N-TRIACONTANE	17.363	191785	1.385 ug/ml
14)	N-DOTRIACONTANE	18.192	376309	2.884 ug/ml
15)	N-TETRATRIACONTANE	18.978	276763	2.290 ug/ml
16)	N-HEXATRIACONTANE	19.720	154336	1.387 ug/ml
17)	N-OCTATRIACONTANE	20.424	145054	1.456 ug/ml
18)	N-TETRACONTANE	21.207	193979	1.947 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081418\
Data File : FF001867.D
Signal(s) : FID2B.ch
Acq On : 14 Aug 2018 11:08
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 15 08:10:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

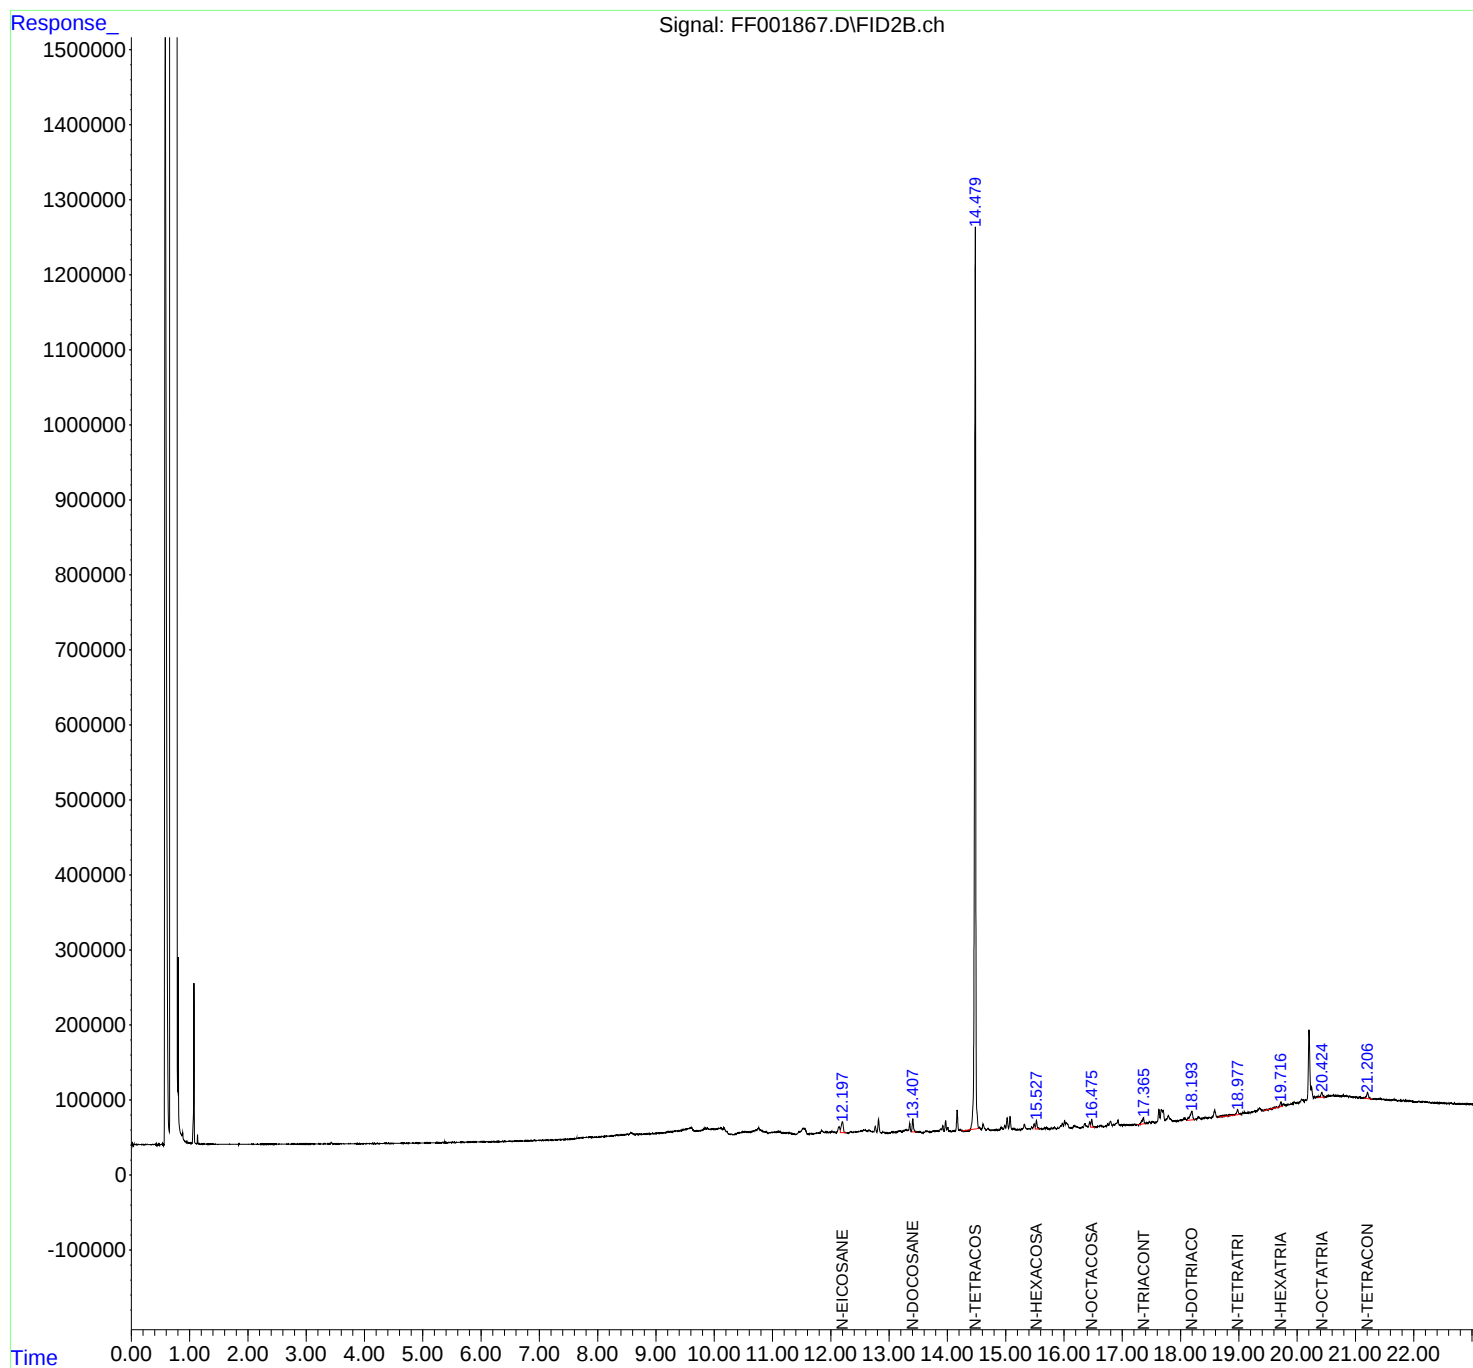

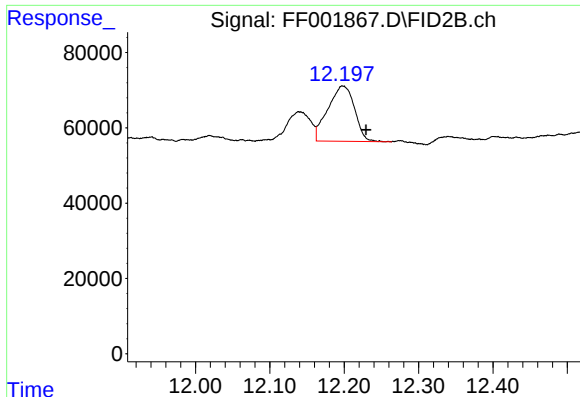


#7 N-EICOSANE

R.T.: 12.198 min
Delta R.T.: -0.032 min
Response: 366735
Conc: 2.46 ug/ml

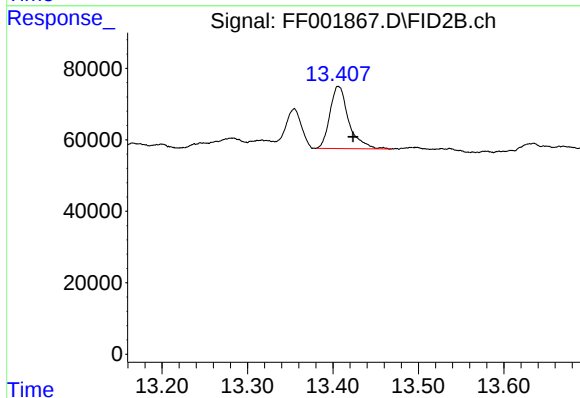


#8 N-DOCOSANE

R.T.: 13.407 min
Delta R.T.: -0.017 min
Response: 264153
Conc: 1.81 ug/ml

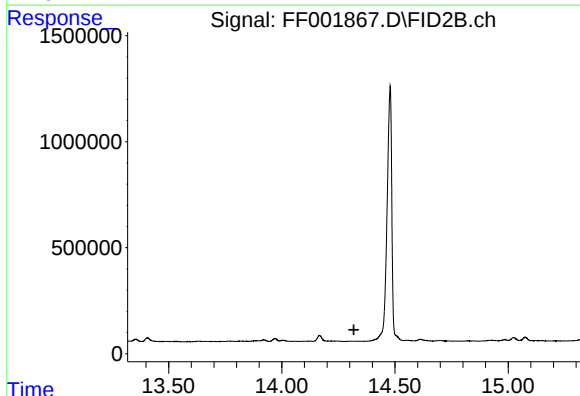


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.318 min
Response: 0
Conc: N.D.

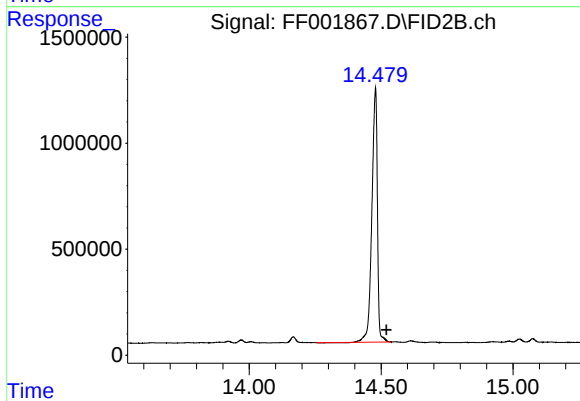


#10 N-TETRACOSANE

R.T.: 14.478 min
Delta R.T.: -0.043 min
Response: 17456204
Conc: 122.37 ug/ml

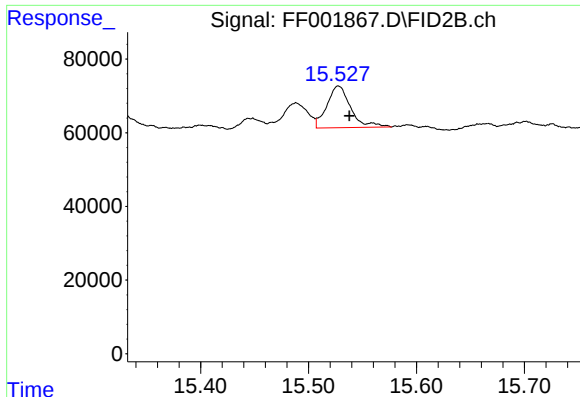


#11 N-HEXACOSANE

R.T.: 15.528 min
Delta R.T.: -0.010 min
Response: 172890
Conc: 1.23 ug/ml

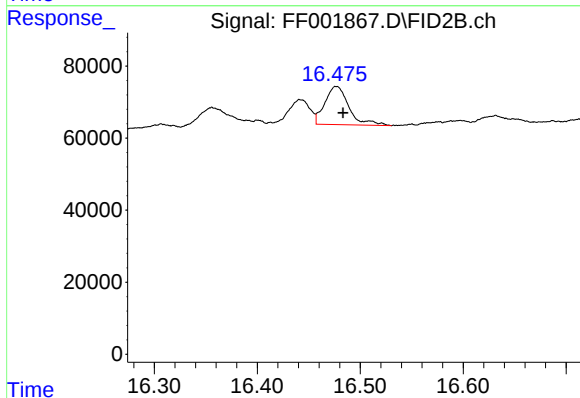


#12 N-OCTACOSANE

R.T.: 16.477 min
Delta R.T.: -0.006 min
Response: 171659
Conc: 1.22 ug/ml

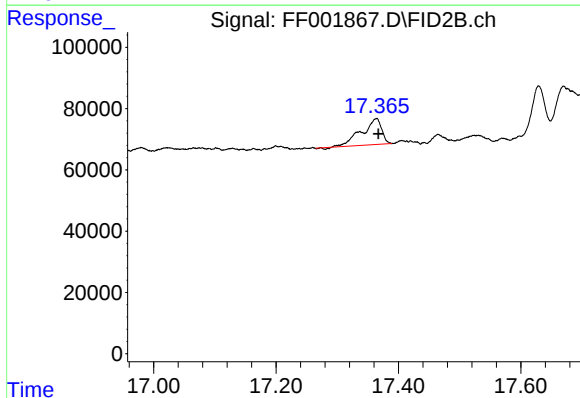


#13 N-TRIACONTANE

R.T.: 17.363 min
Delta R.T.: -0.004 min
Response: 191785
Conc: 1.39 ug/ml

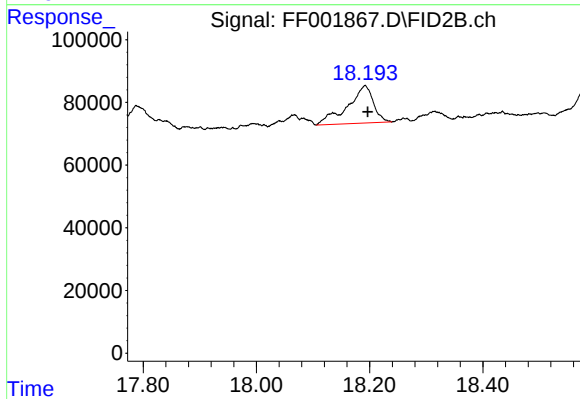


#14 N-DOTRIACONTANE

R.T.: 18.192 min
Delta R.T.: -0.005 min
Response: 376309
Conc: 2.88 ug/ml

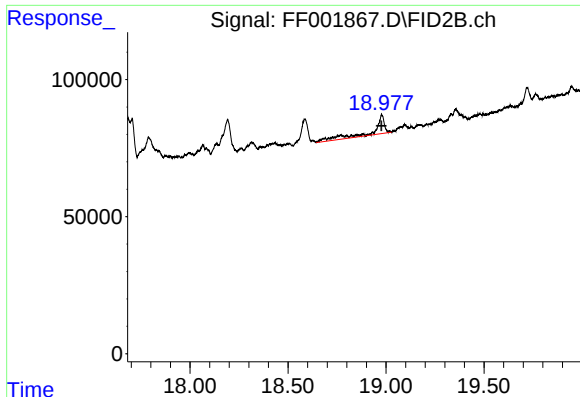


#15 N-TETRATRIACONTANE

R.T.: 18.978 min
Delta R.T.: 0.001 min
Response: 276763
Conc: 2.29 ug/ml

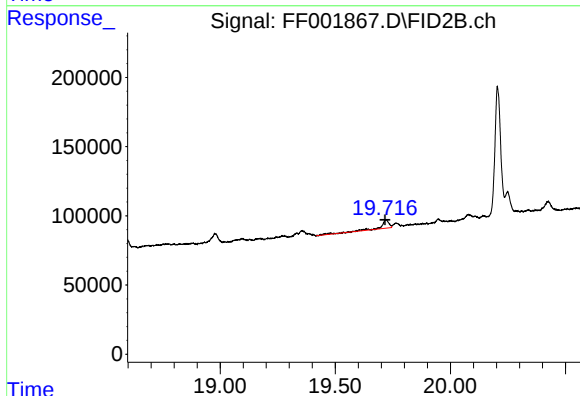


#16 N-HEXATRIACONTANE

R.T.: 19.720 min
Delta R.T.: 0.004 min
Response: 154336
Conc: 1.39 ug/ml

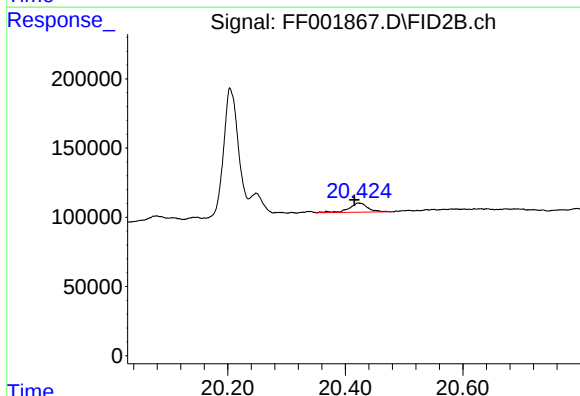

#17 N-OCTATRIACONTANE

R.T.: 20.424 min
Delta R.T.: 0.008 min
Response: 145054
Conc: 1.46 ug/ml

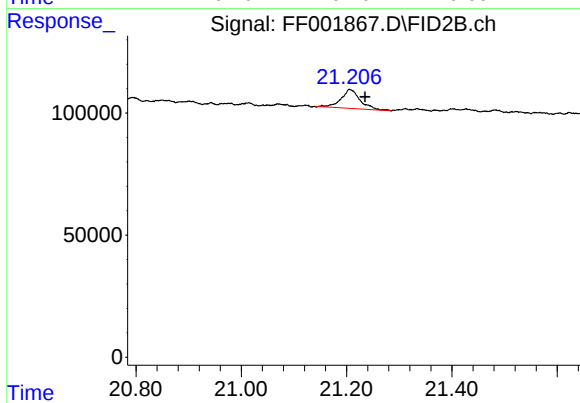

#18 N-TETRACONTANE

R.T.: 21.207 min
Delta R.T.: -0.028 min
Response: 193979
Conc: 1.95 ug/ml