

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081418\
Data File : FF001872.D
Signal(s) : FID2B.ch
Acq On : 14 Aug 2018 16:52
Operator : AJ\SJ
Sample : PB112058BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 15 08:12:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units


System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.312	2299908	18.210 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.475	232823	1.632 ug/ml
16) N-HEXATRIACONTANE	19.722	94459	0.849 ug/ml


(f)=RT Delta > 1/2 Window

(m)=manual int.

Integration File: autoint1.e
Quant Time: Aug 15 08:12:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

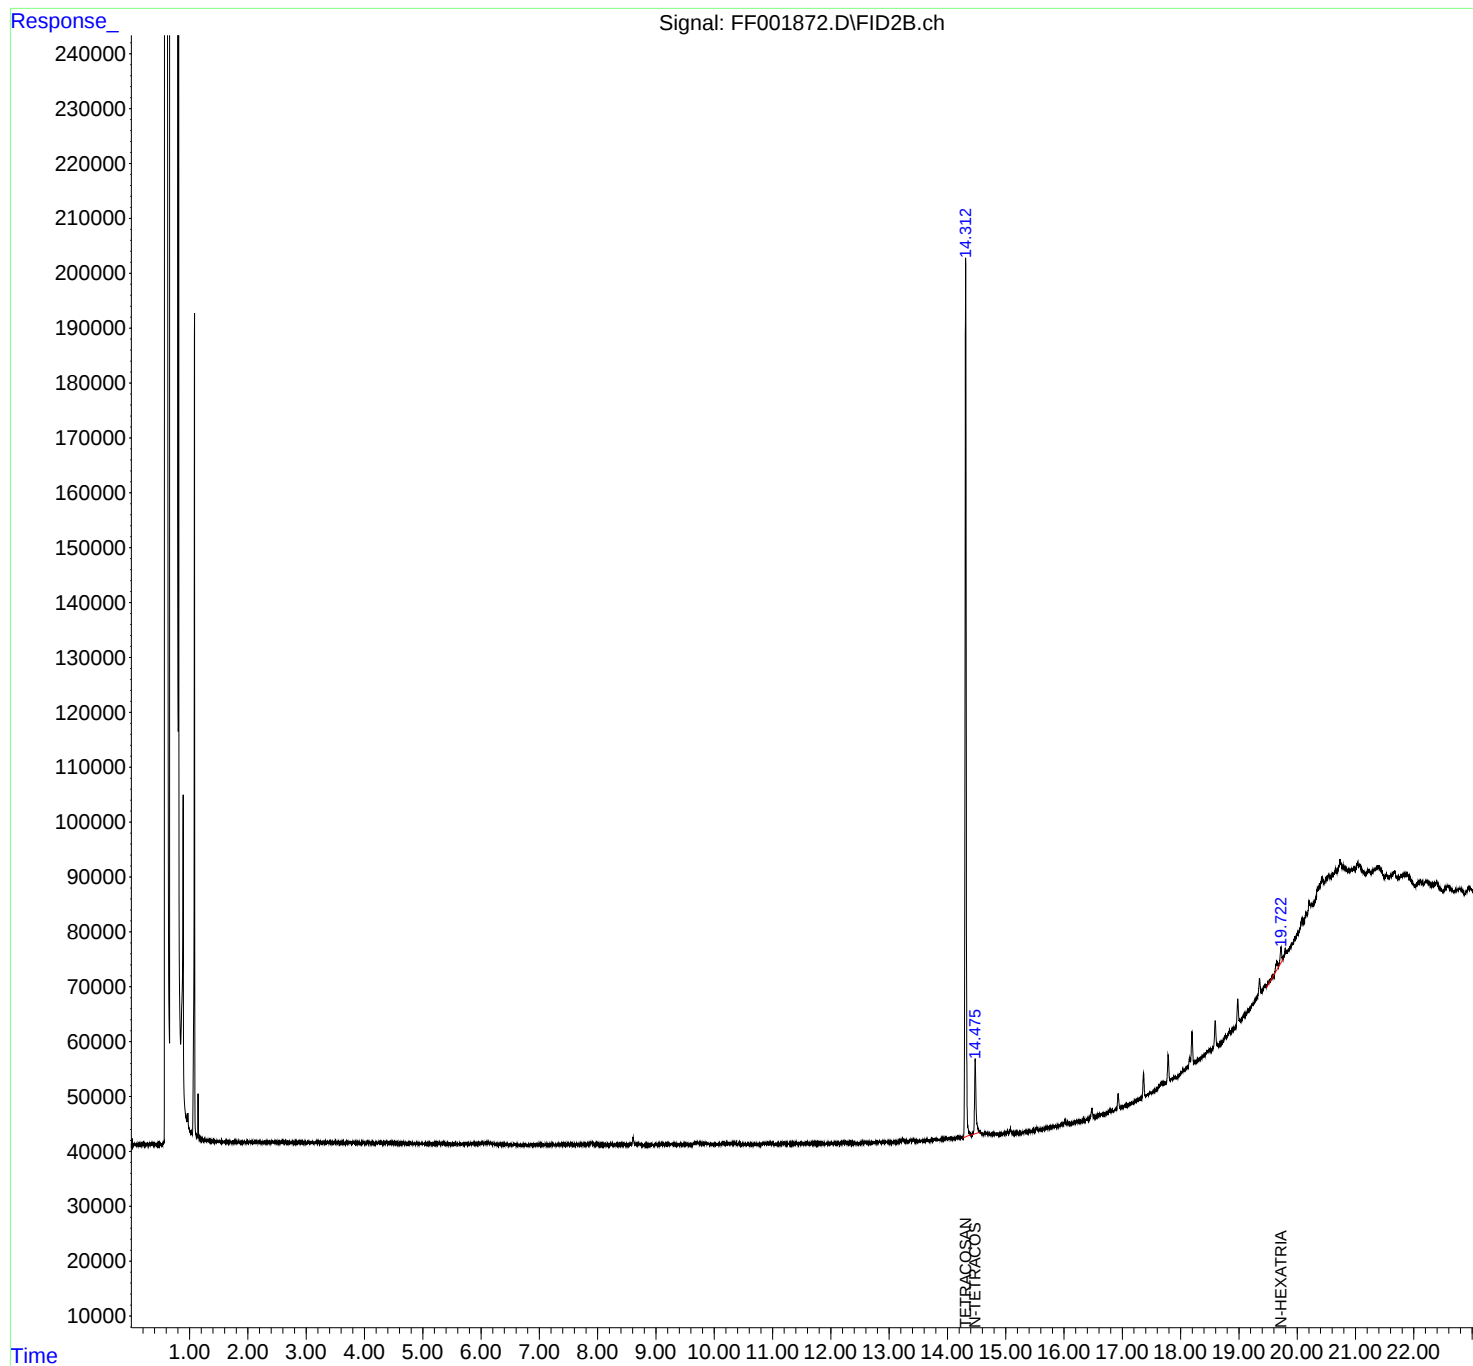

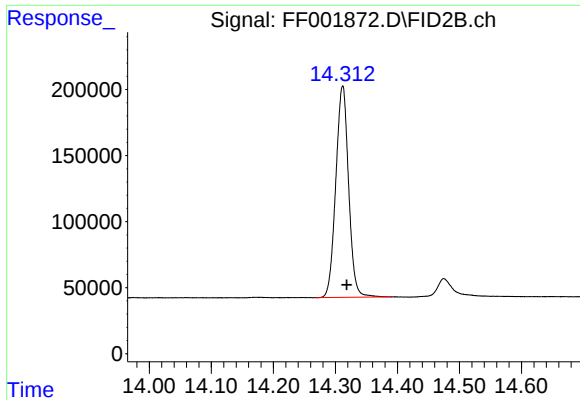


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.312 min
Delta R.T.: -0.007 min
Response: 2299908
Conc: 18.21 ug/ml

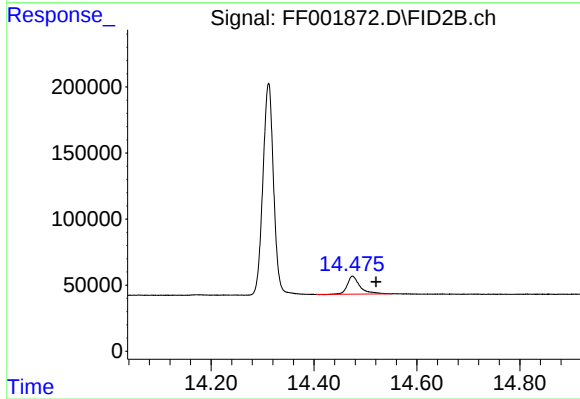

#10 N-TETRACOSANE

R.T.: 14.475 min
Delta R.T.: -0.046 min
Response: 232823
Conc: 1.63 ug/ml

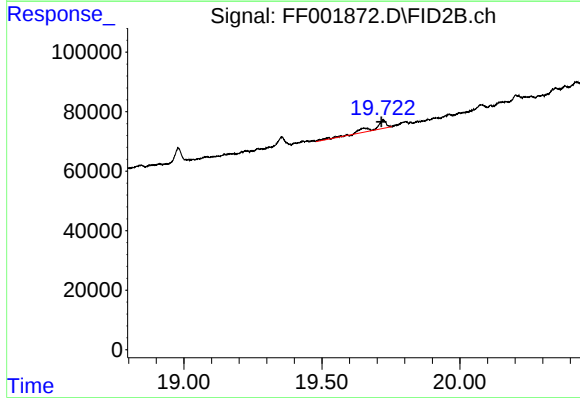

#16 N-HEXATRIACONTANE

R.T.: 19.722 min
Delta R.T.: 0.006 min
Response: 94459
Conc: 0.85 ug/ml