

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081522\
 Data File : FF011250.D
 Signal(s) : FID2B.ch
 Acq On : 15 Aug 2022 13:29
 Operator : YP\AJ
 Sample : N4189-03MS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB19MS

Integration File: Sample.e
 Quant Time: Aug 15 14:09:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
 Quant Title :
 QLast Update : Thu Jul 28 14:46:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.798	1445812	13.302 ug/ml
Target Compounds			
2) N-DECANE	4.359	1832901	14.714 ug/ml
3) N-DODECANE	6.528	1866930	14.831 ug/ml
4) N-TETRADECANE	8.352	1851118	14.744 ug/ml
5) N-HEXADECANE	9.956	1765590	13.802 ug/ml
6) N-OCTADECANE	11.395	1942650	15.083 ug/ml
7) N-EICOSANE	12.703	1957265	15.310 ug/ml
8) N-DOCOSANE	13.899	1904197	15.266 ug/ml
10) N-TETRACOSANE	15.000	1904069	15.305 ug/ml
11) N-HEXACOSANE	16.020	1856455	15.172 ug/ml
12) N-OCTACOSANE	16.968	1844245	15.278 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081522\
Data File : FF011250.D
Signal(s) : FID2B.ch
Acq On : 15 Aug 2022 13:29
Operator : YP\AJ
Sample : N4189-03MS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB19MS

Integration File: Sample.e
Quant Time: Aug 15 14:09:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

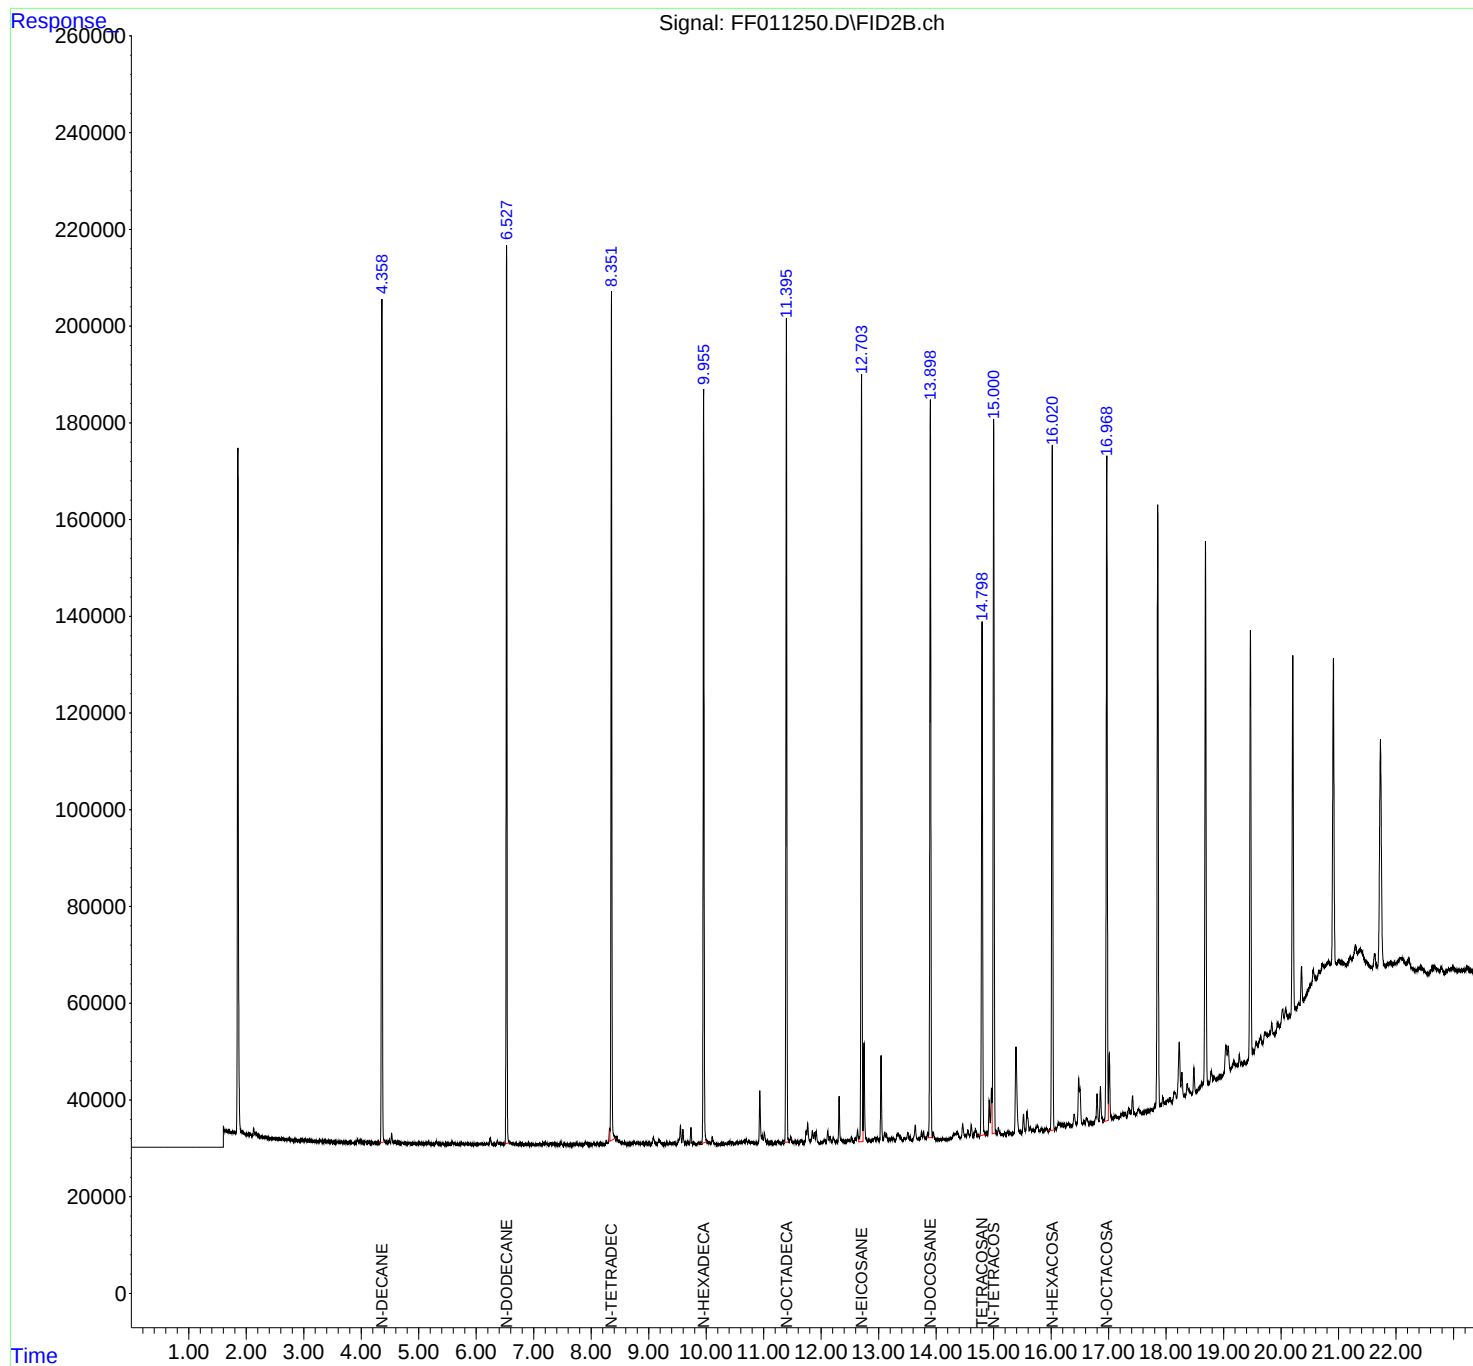


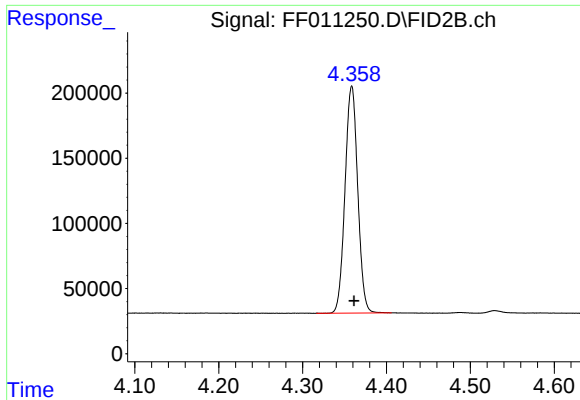

#2 N-DECANE


R.T.: 4.359 min
Delta R.T.: -0.003 min
Response: 1832901
Conc: 14.71 ug/ml

Instrument :
FID_F
ClientSampleId :
SB19MS

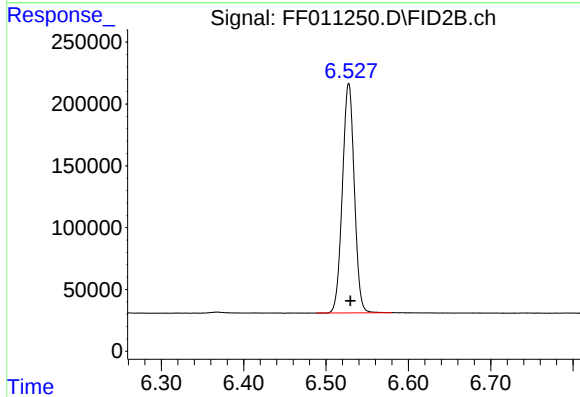


#3 N-DODECANE

R.T.: 6.528 min
Delta R.T.: -0.002 min
Response: 1866930
Conc: 14.83 ug/ml

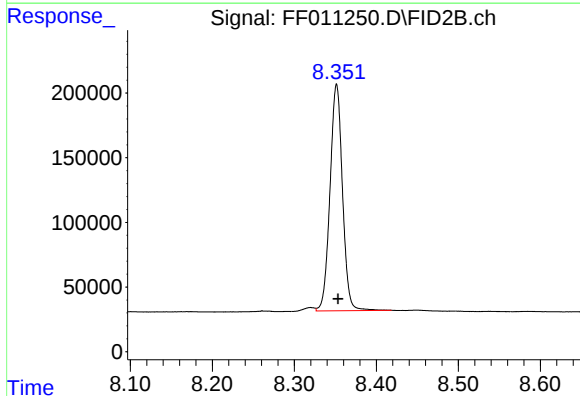


#4 N-TETRADECANE

R.T.: 8.352 min
Delta R.T.: -0.002 min
Response: 1851118
Conc: 14.74 ug/ml

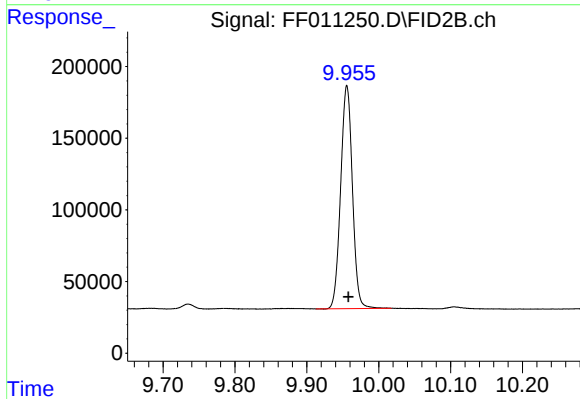

#5 N-HEXADECANE


R.T.: 9.956 min
Delta R.T.: -0.002 min
Response: 1765590
Conc: 13.80 ug/ml

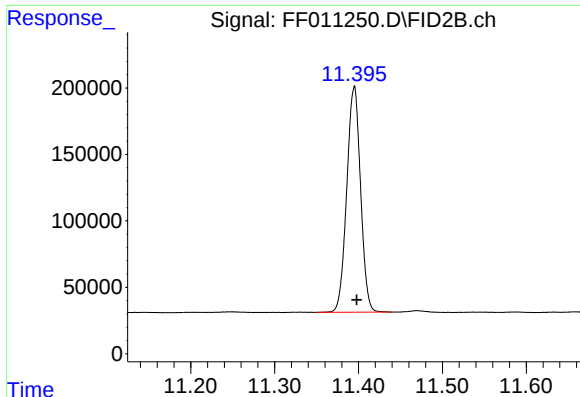

#6 N-OCTADECANE


R.T.: 11.395 min
Delta R.T.: -0.003 min
Response: 1942650
Conc: 15.08 ug/ml

Instrument :
FID_F
ClientSampleId :
SB19MS

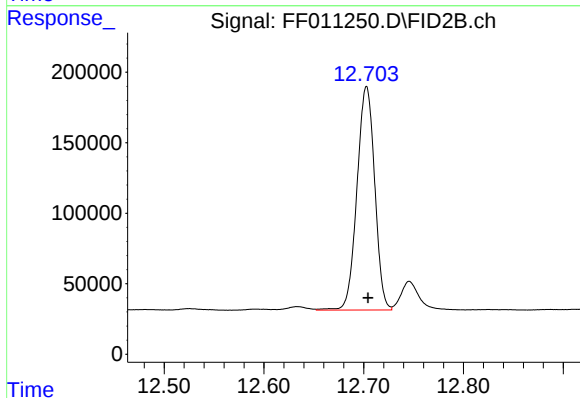


#7 N-EICOSANE

R.T.: 12.703 min
Delta R.T.: -0.001 min
Response: 1957265
Conc: 15.31 ug/ml

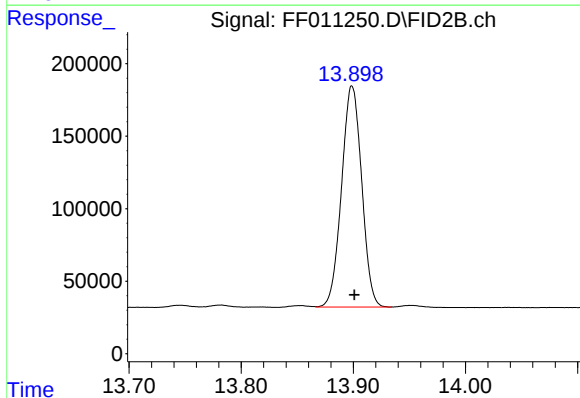


#8 N-DOCOSANE

R.T.: 13.899 min
Delta R.T.: -0.002 min
Response: 1904197
Conc: 15.27 ug/ml

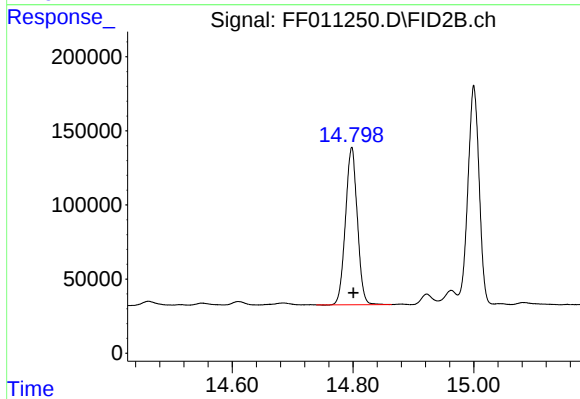

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.798 min
Delta R.T.: -0.003 min
Response: 1445812
Conc: 13.30 ug/ml

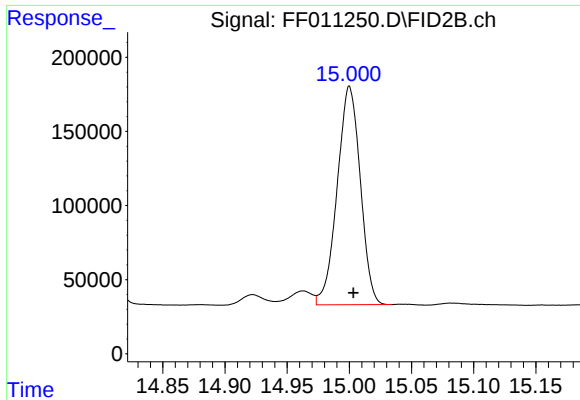

#10 N-TETRACOSANE


R.T.: 15.000 min
Delta R.T.: -0.003 min
Response: 1904069
Conc: 15.31 ug/ml

Instrument :
FID_F
ClientSampleId :
SB19MS

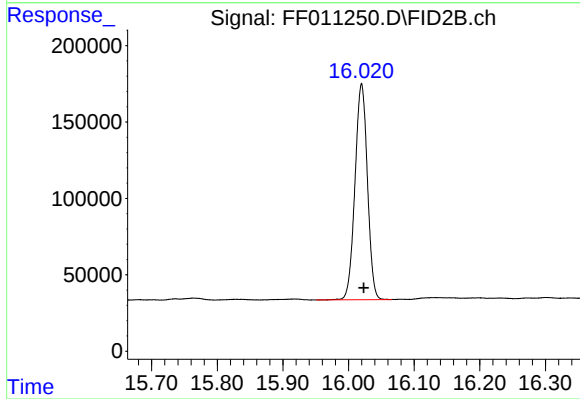

#11 N-HEXACOSANE

R.T.: 16.020 min
Delta R.T.: -0.003 min
Response: 1856455
Conc: 15.17 ug/ml

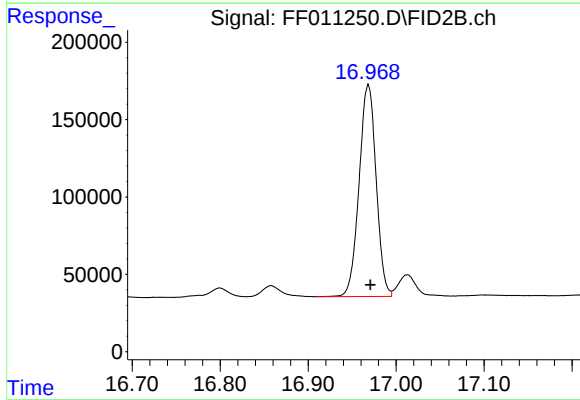

#12 N-OCTACOSANE

R.T.: 16.968 min
Delta R.T.: -0.002 min
Response: 1844245
Conc: 15.28 ug/ml