

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008917.D
Signal(s) : FID2B.ch
Acq On : 16 Aug 2021 11:21
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 17 08:33:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) N-HEXACOSANE	15.971	90422	0.664 ug/ml
12) N-OCTACOSANE	16.920	401769	3.003 ug/ml
13) N-TRIACONTANE	17.808	744686	5.698 ug/ml
14) N-DOTRIACONTANE	18.638	471962	3.815 ug/ml
15) N-TETRATRIACONTANE	19.417	177363	1.522 ug/ml
16) N-HEXATRIACONTANE	20.155	134028	1.262 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008917.D
Signal(s) : FID2B.ch
Acq On : 16 Aug 2021 11:21
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 17 08:33:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

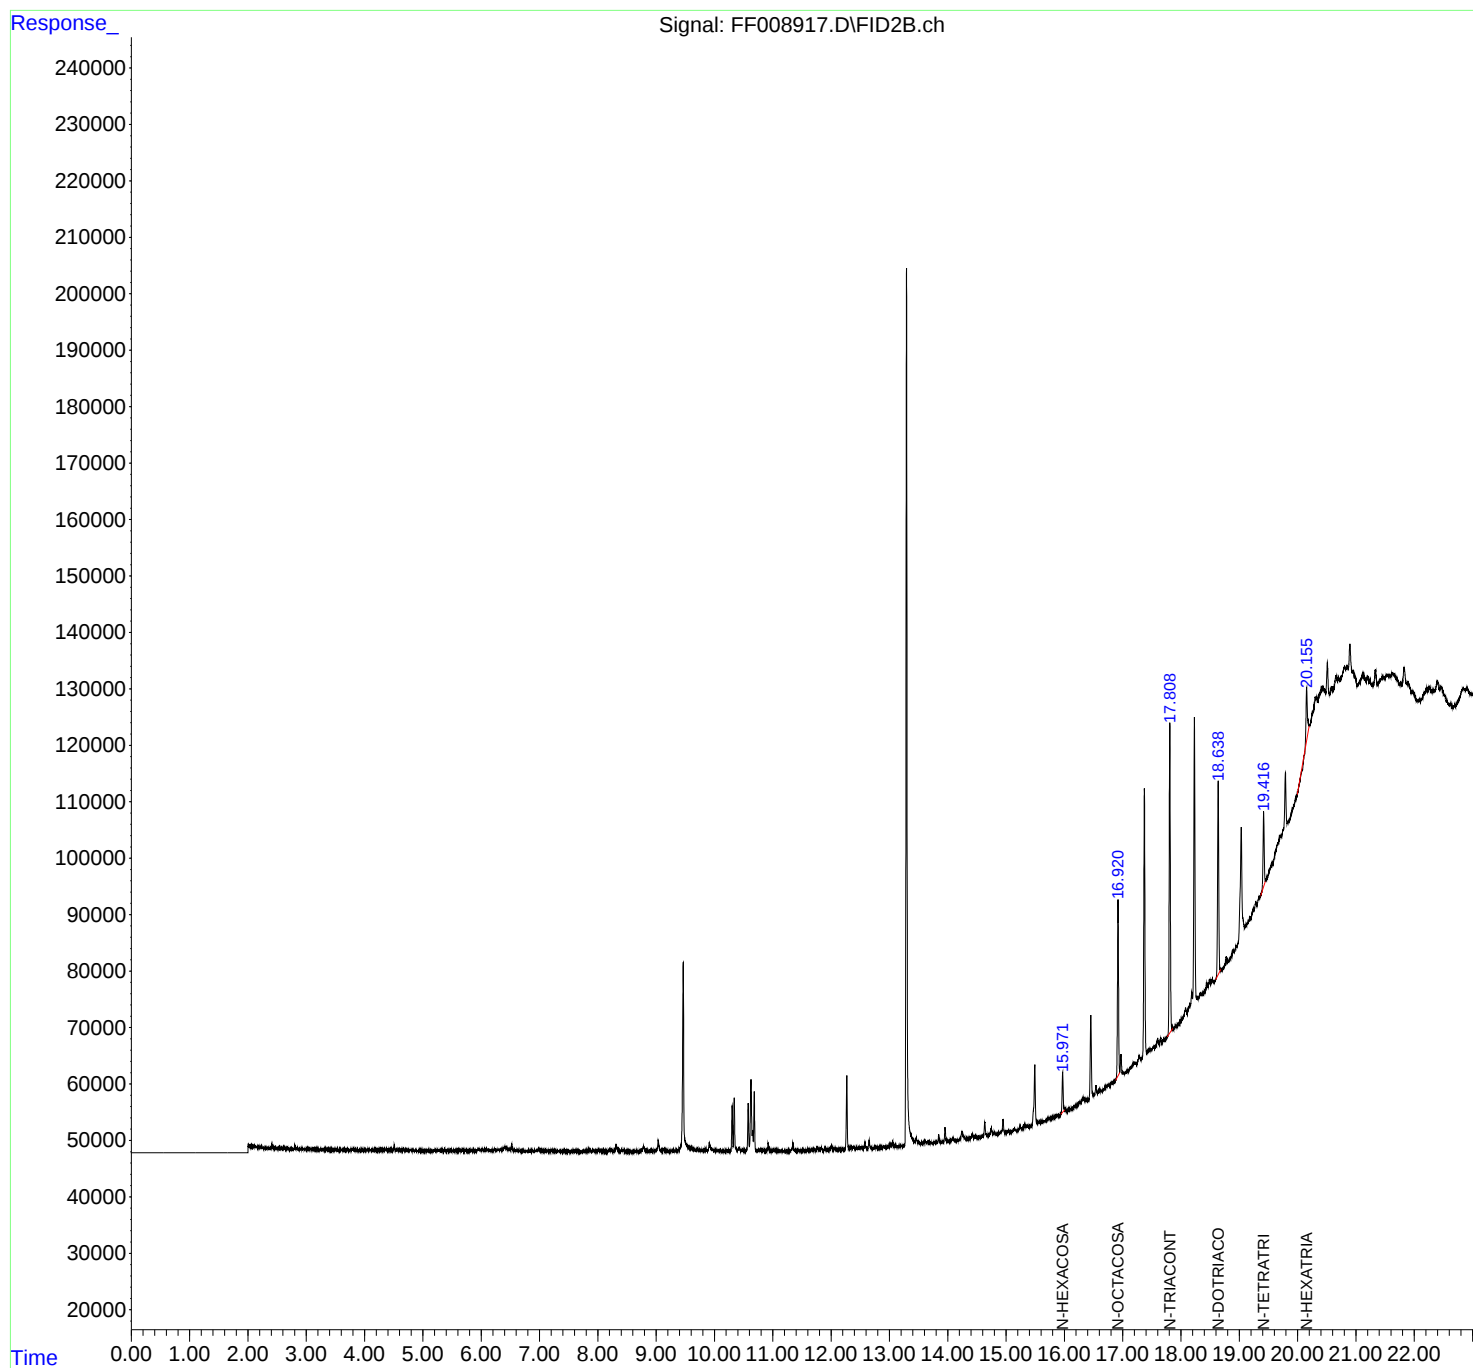


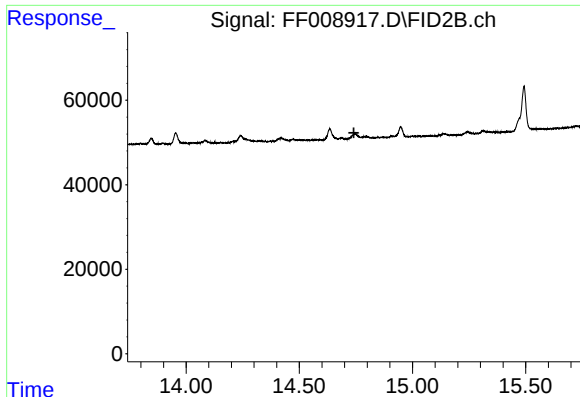

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.741 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

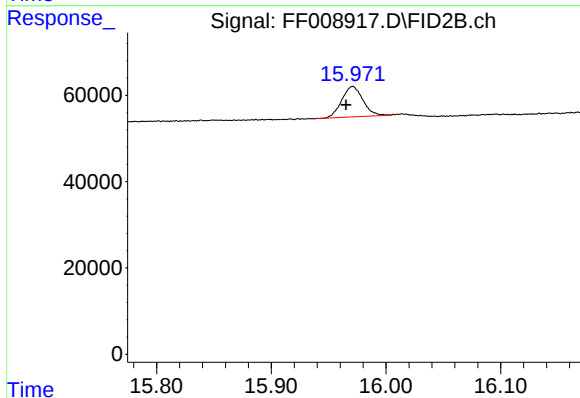


#11 N-HEXACOSANE

R.T.: 15.971 min
Delta R.T.: 0.006 min
Response: 90422
Conc: 0.66 ug/ml

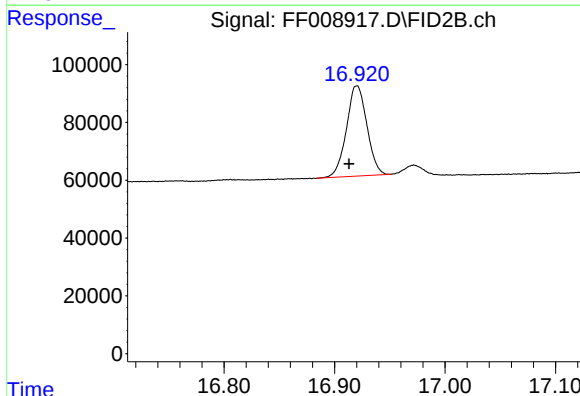


#12 N-OCTACOSANE

R.T.: 16.920 min
Delta R.T.: 0.007 min
Response: 401769
Conc: 3.00 ug/ml

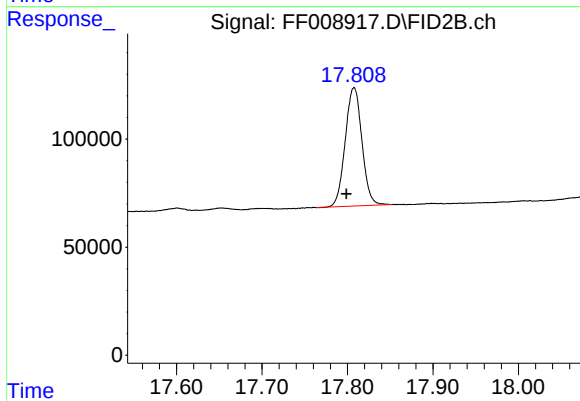

#13 N-TRIACONTANE


R.T.: 17.808 min
Delta R.T.: 0.009 min
Response: 744686
Conc: 5.70 ug/ml

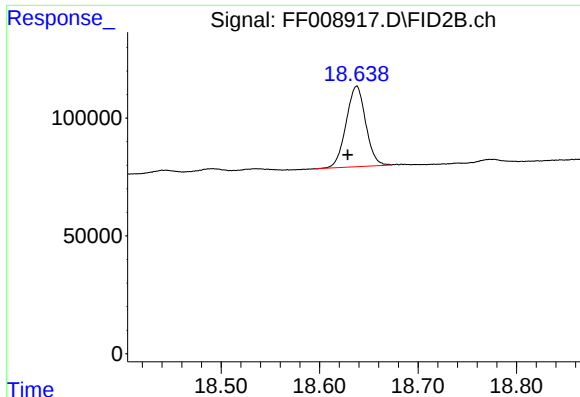

#14 N-DOTRIACONTANE


R.T.: 18.638 min
Delta R.T.: 0.009 min
Response: 471962
Conc: 3.81 ug/ml

Instrument :
FID_F
ClientSampleId :

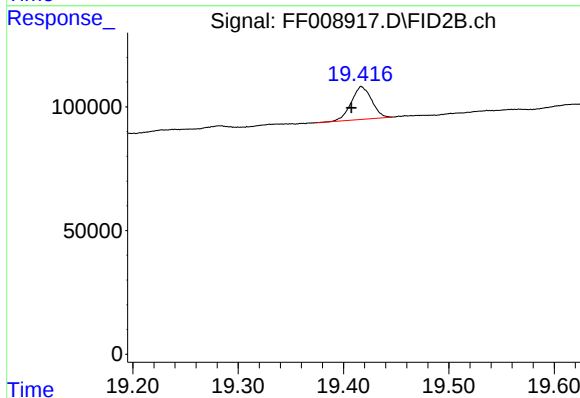

#15 N-TETRATRIACONTANE

R.T.: 19.417 min
Delta R.T.: 0.010 min
Response: 177363
Conc: 1.52 ug/ml

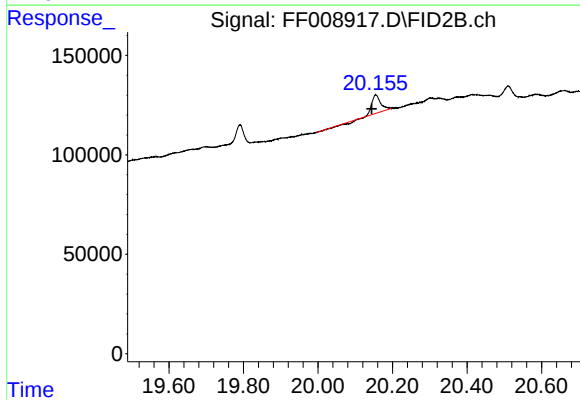

#16 N-HEXATRIACONTANE

R.T.: 20.155 min
Delta R.T.: 0.010 min
Response: 134028
Conc: 1.26 ug/ml