

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
 Data File : FF008923.D
 Signal(s) : FID2B.ch
 Acq On : 16 Aug 2021 19:56
 Operator : DD\AJ
 Sample : M3424-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 17 08:35:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.740	1930656	16.115 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.277	252710	1.883 ug/ml
10)	N-TETRACOSANE	14.943	99693	0.720 ug/ml
14)	N-DOTRIACONTANE	18.630	134122	1.084 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008923.D
Signal(s) : FID2B.ch
Acq On : 16 Aug 2021 19:56
Operator : DD\AJ
Sample : M3424-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 17 08:35:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

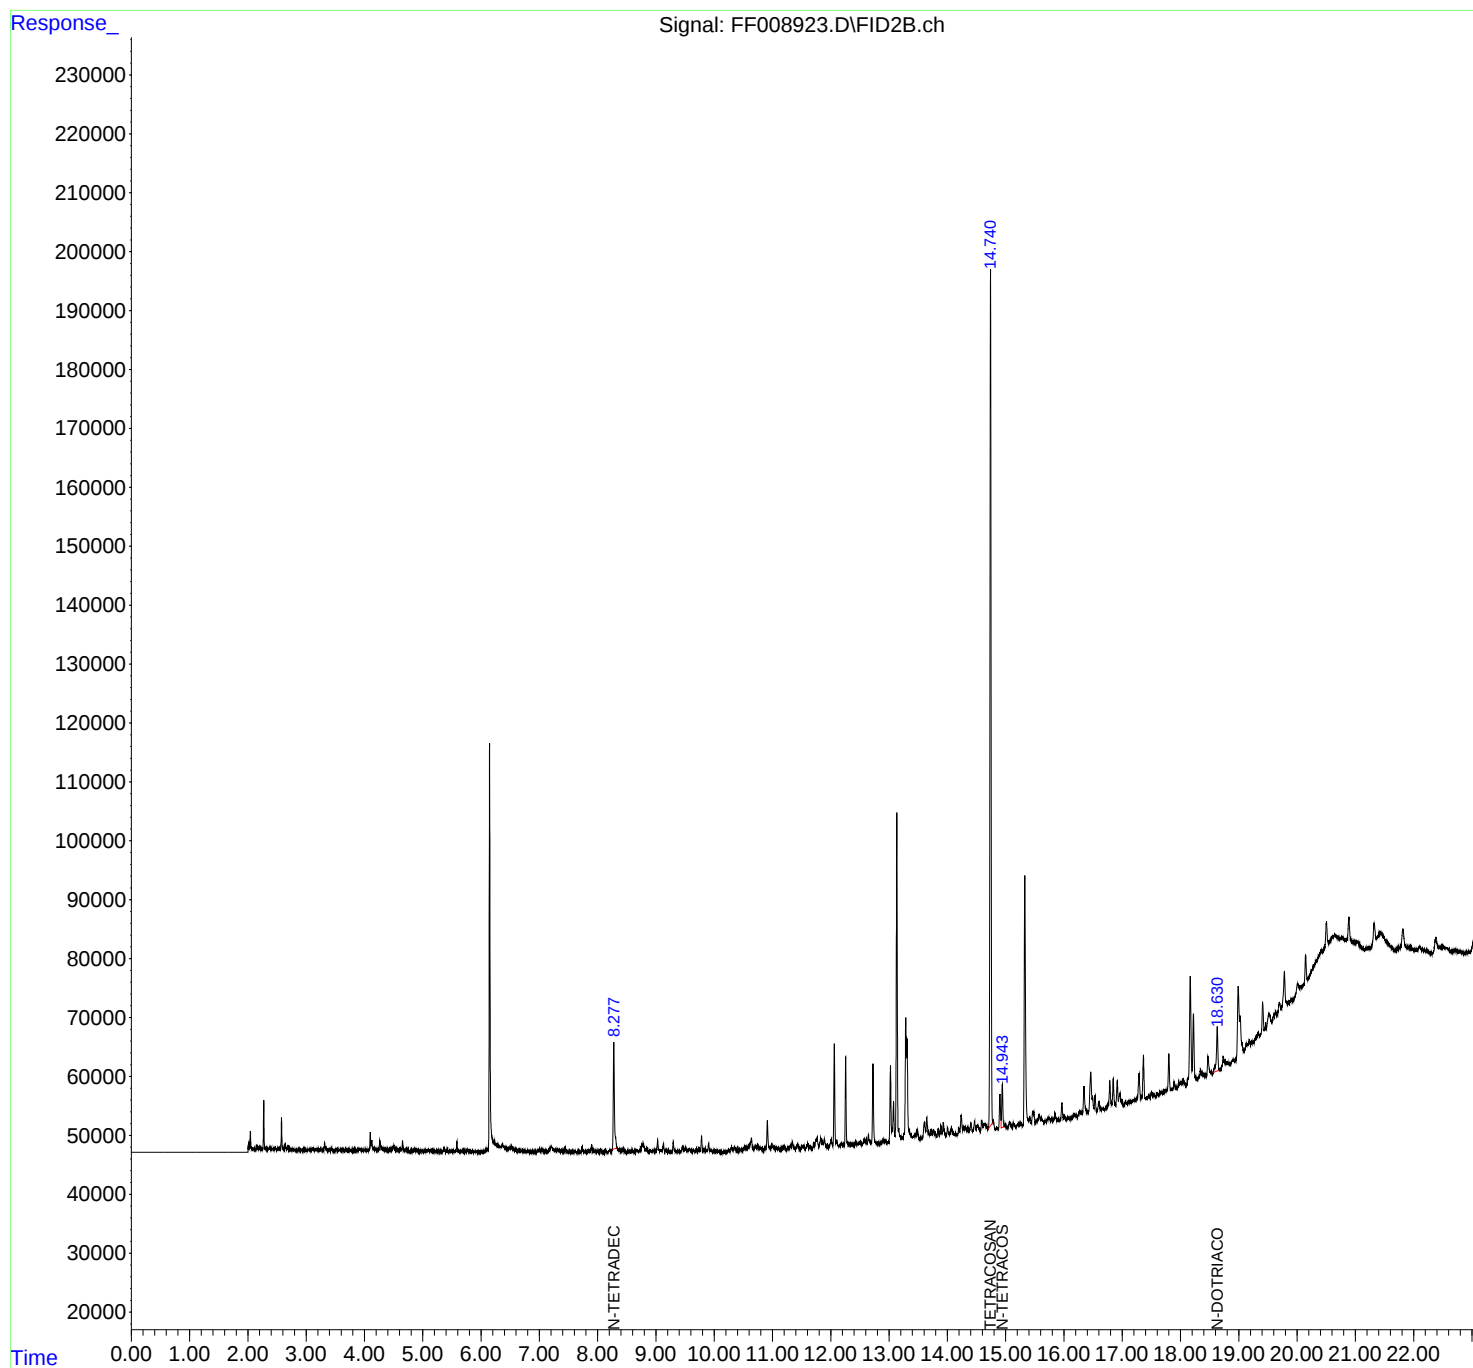


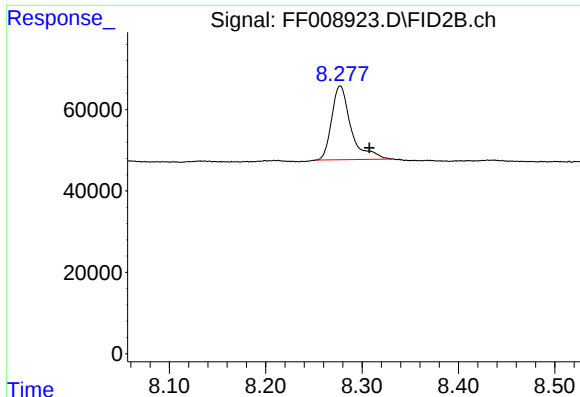

#4 N-TETRADECANE


R.T.: 8.277 min
Delta R.T.: -0.030 min
Response: 252710
Conc: 1.88 ug/ml

Instrument :
FID_F
ClientSampleId :

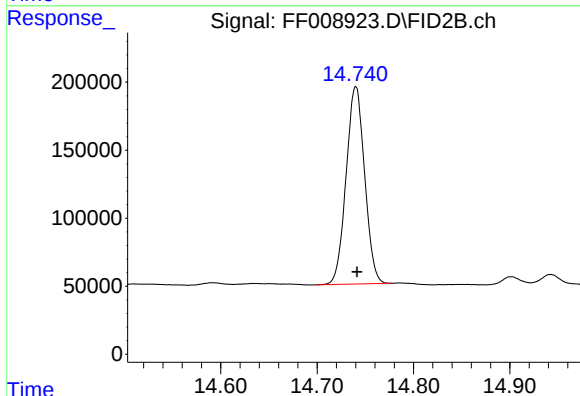


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: -0.001 min
Response: 1930656
Conc: 16.11 ug/ml

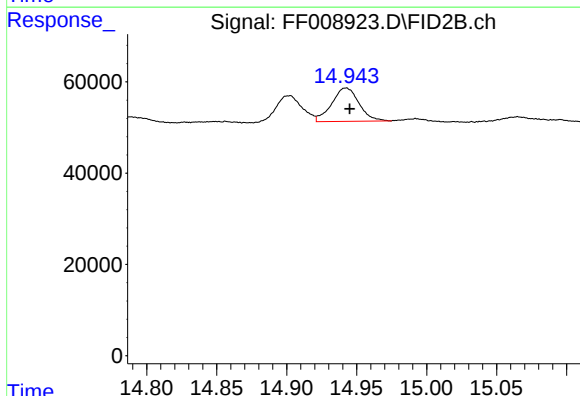

#10 N-TETRACOSANE

R.T.: 14.943 min
Delta R.T.: -0.003 min
Response: 99693
Conc: 0.72 ug/ml

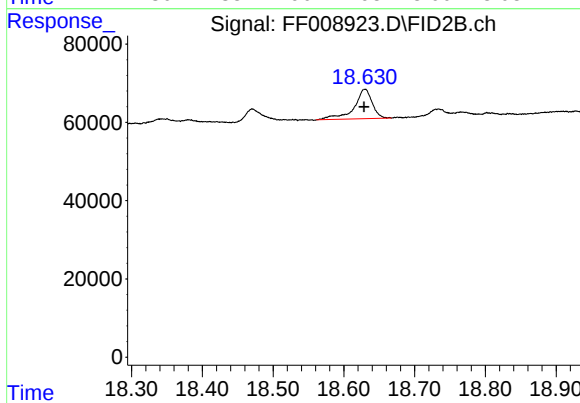

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.001 min
Response: 134122
Conc: 1.08 ug/ml