

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008927.D
Signal(s) : FID2B.ch
Acq On : 16 Aug 2021 22:02
Operator : DD\AJ
Sample : M3424-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 17 08:36:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	2179078	18.188 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.944	94154	0.680 ug/ml
14) N-DOTRIACONTANE	18.628	120276	0.972 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008927.D
Signal(s) : FID2B.ch
Acq On : 16 Aug 2021 22:02
Operator : DD\AJ
Sample : M3424-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 17 08:36:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

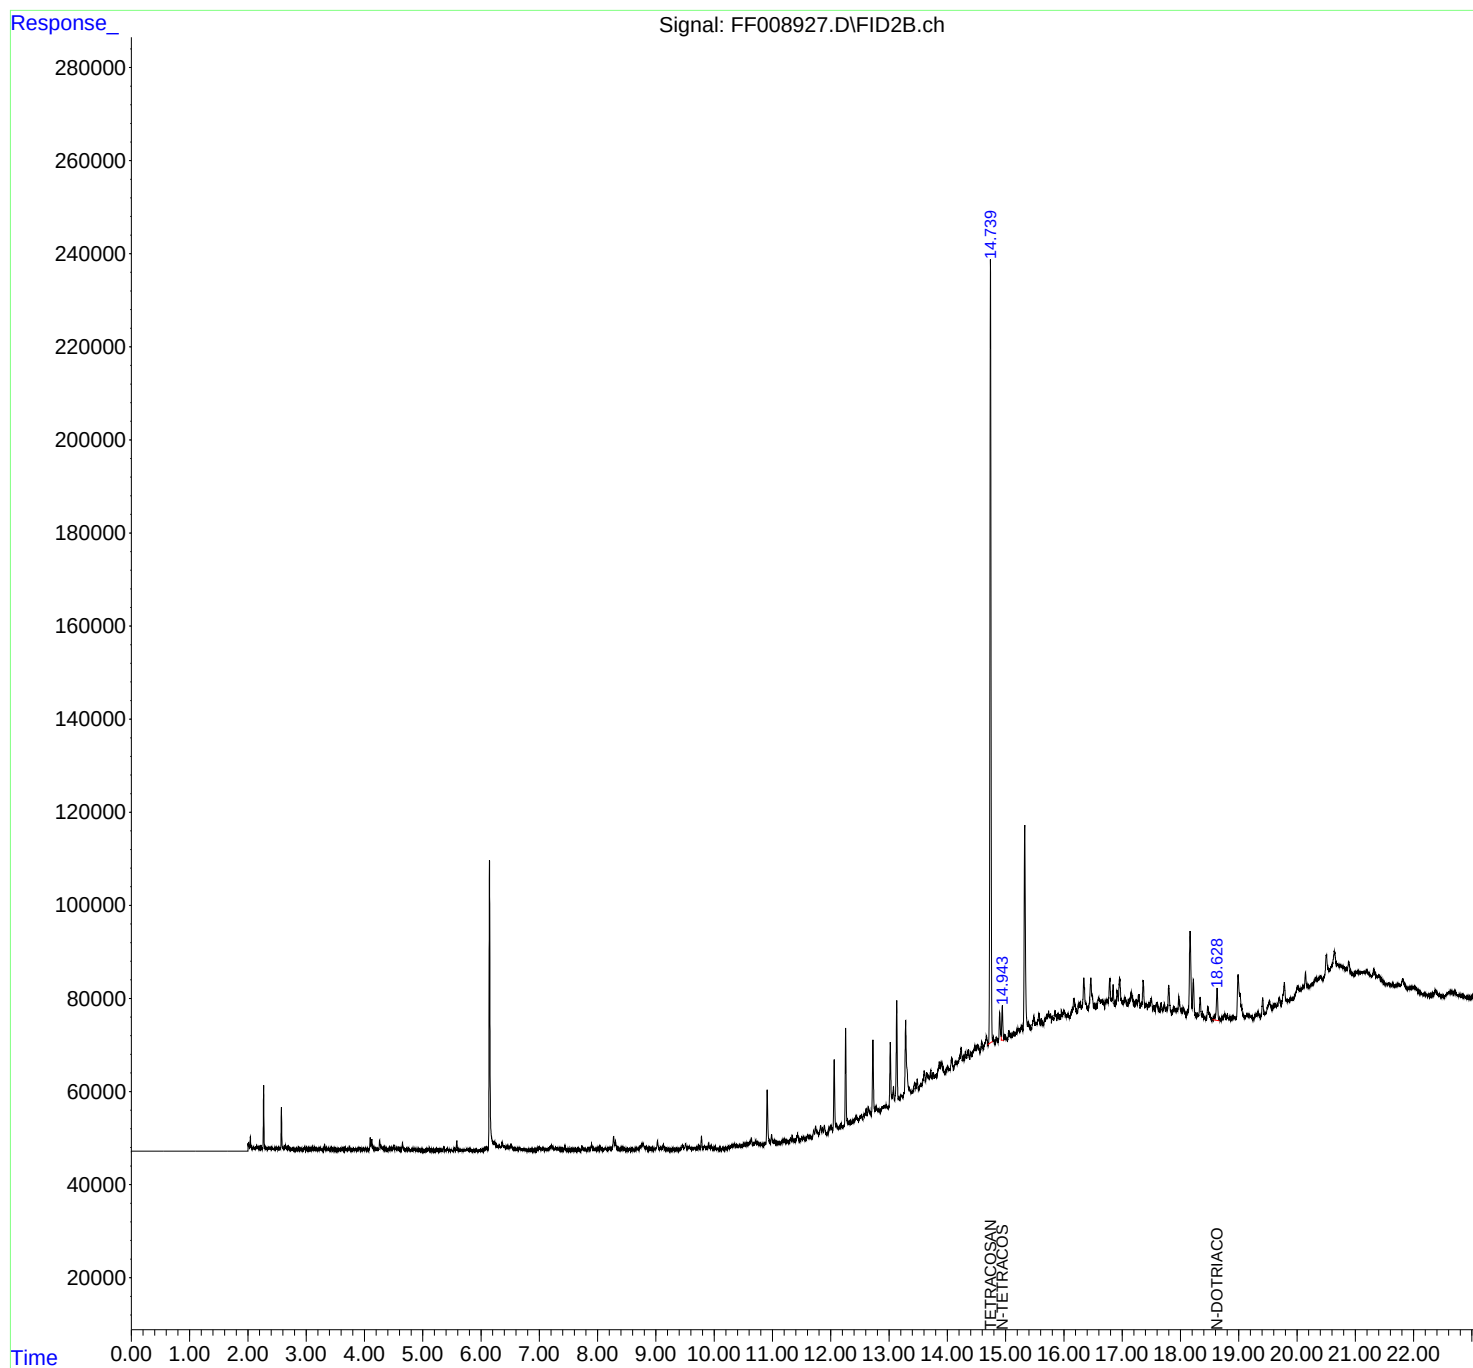


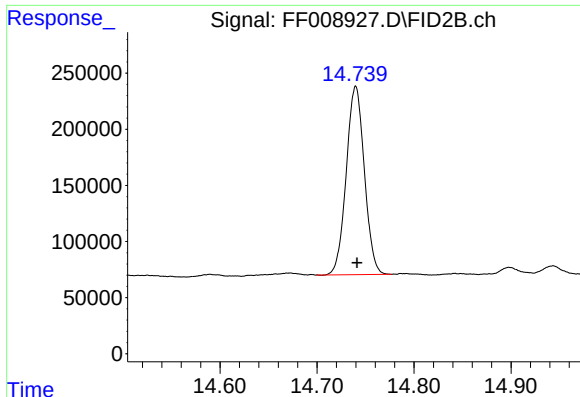

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.740 min
Delta R.T.: -0.001 min
Response: 2179078
Conc: 18.19 ug/ml

Instrument :
FID_F
ClientSampleId :

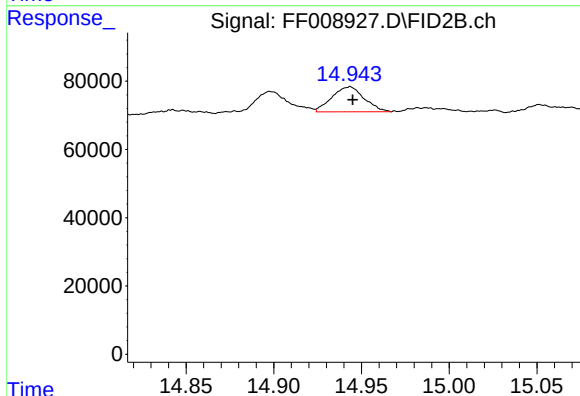

#10 N-TETRACOSANE

R.T.: 14.944 min
Delta R.T.: -0.001 min
Response: 94154
Conc: 0.68 ug/ml

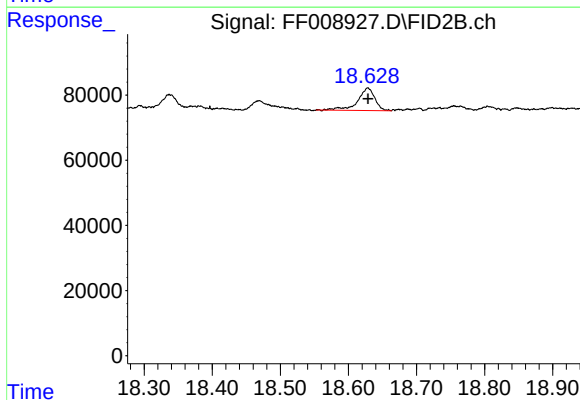

#14 N-DOTRIACONTANE

R.T.: 18.628 min
Delta R.T.: 0.000 min
Response: 120276
Conc: 0.97 ug/ml