

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
 Data File : FF008931.D
 Signal(s) : FID2B.ch
 Acq On : 17 Aug 2021 00:07
 Operator : DD\AJ
 Sample : M3425-05
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 17 08:37:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
 Quant Title :
 QLast Update : Thu Jul 22 01:38:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	1710146	14.274 ug/ml
Target Compounds			
8) N-DOCOSANE	13.901f	73133	0.528 ug/ml
10) N-TETRACOSANE	14.942	114726	0.829 ug/ml
14) N-DOTRIACONTANE	18.626	153936	1.244 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008931.D
Signal(s) : FID2B.ch
Acq On : 17 Aug 2021 00:07
Operator : DD\AJ
Sample : M3425-05
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 17 08:37:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

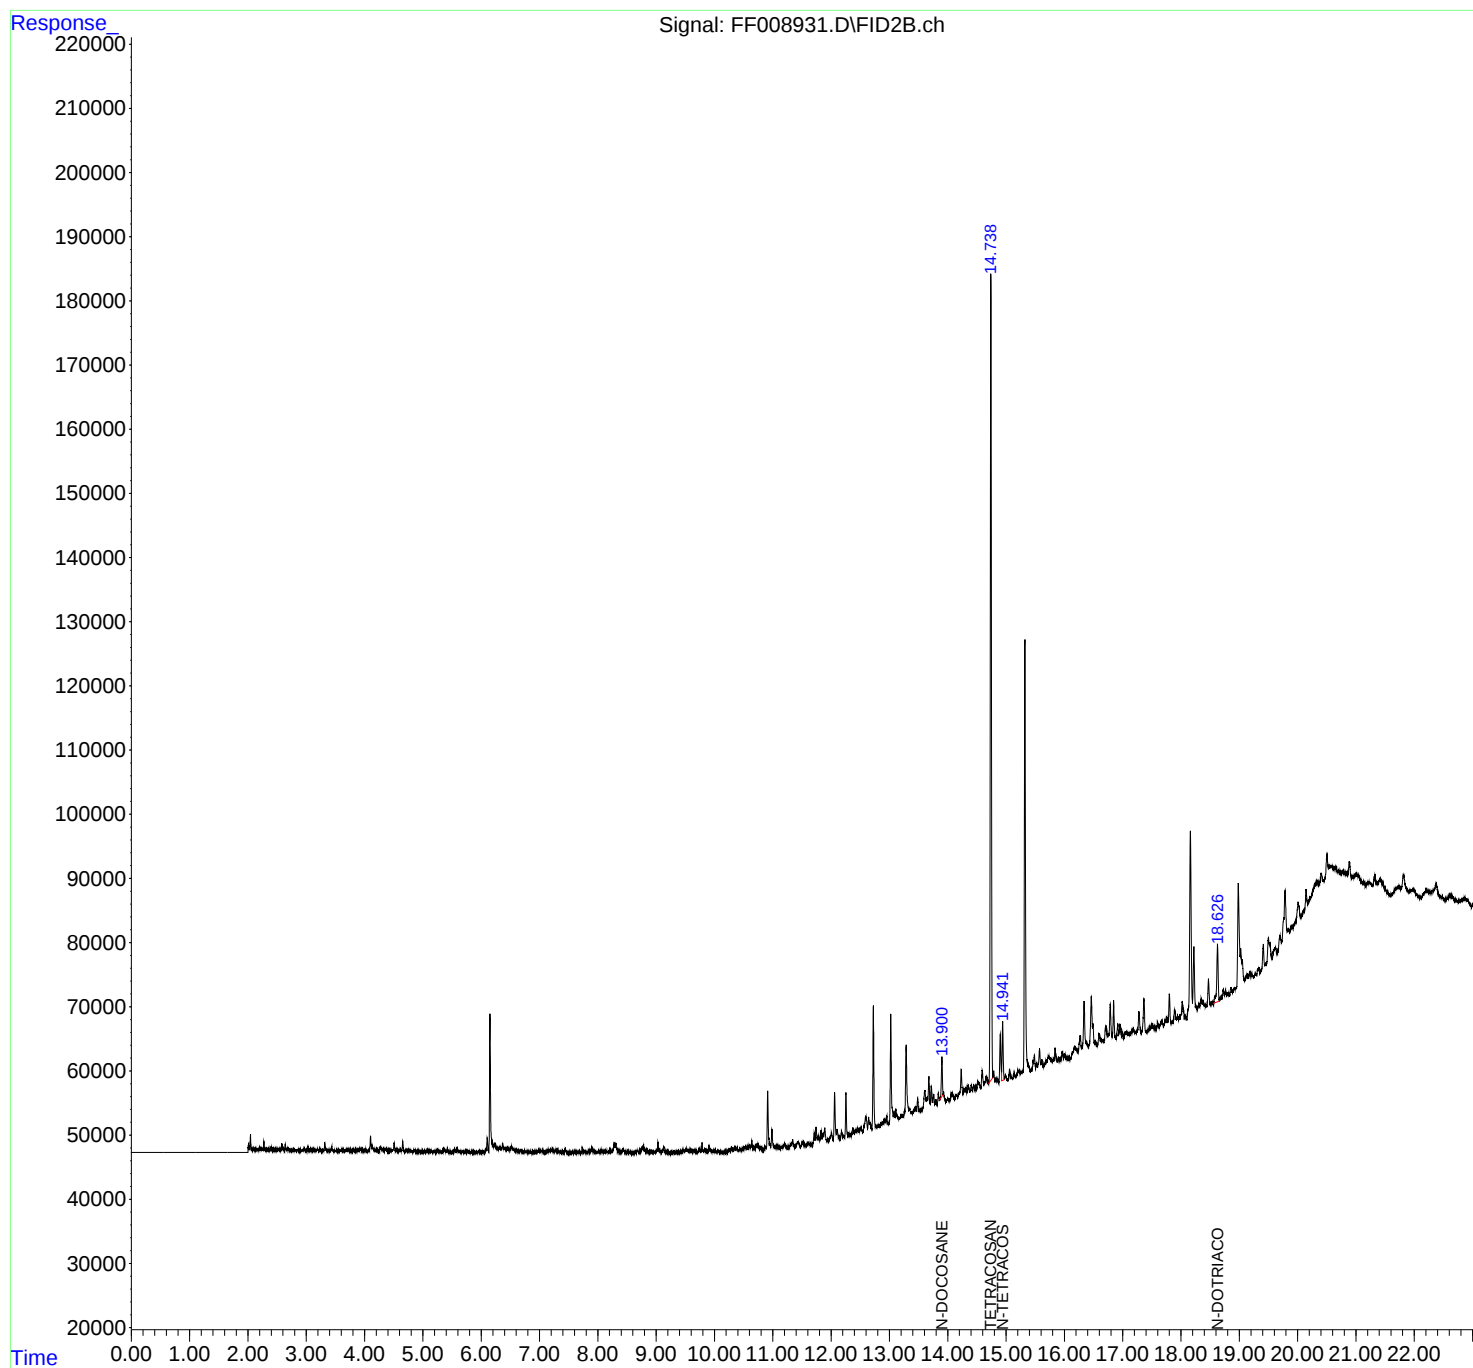


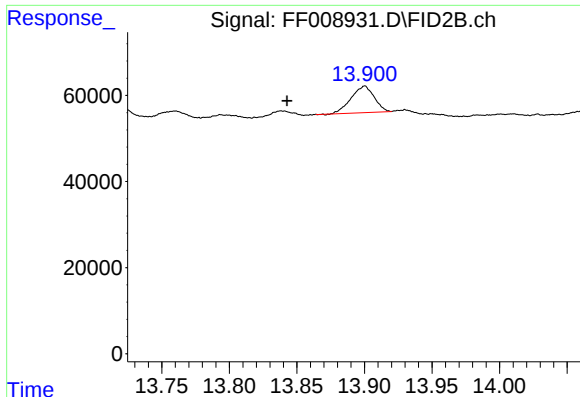

#8 N-DOCOSANE


R.T.: 13.901 min
Delta R.T.: 0.058 min
Response: 73133
Conc: 0.53 ug/ml

Instrument :
FID_F
ClientSampleId :

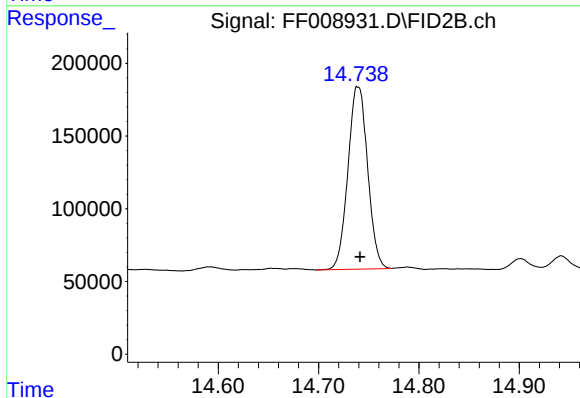


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.003 min
Response: 1710146
Conc: 14.27 ug/ml

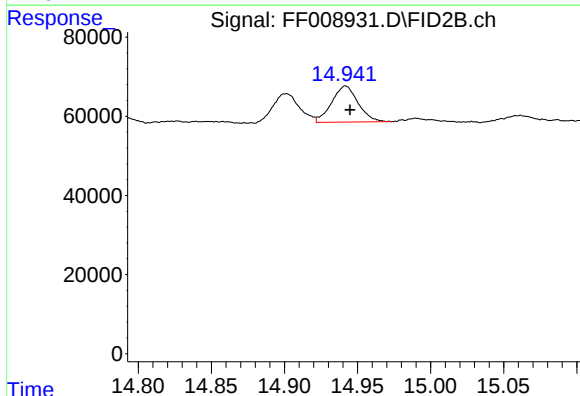

#10 N-TETRACOSANE

R.T.: 14.942 min
Delta R.T.: -0.003 min
Response: 114726
Conc: 0.83 ug/ml

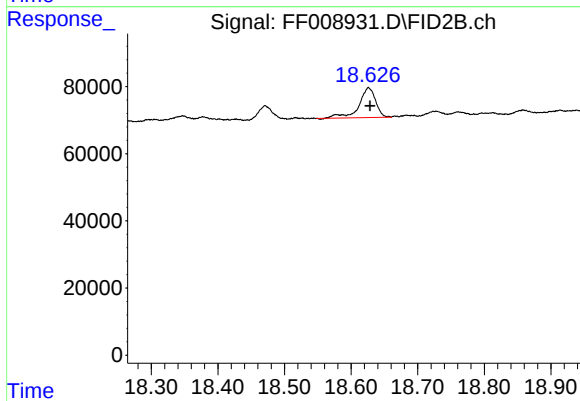

#14 N-DOTRIACONTANE

R.T.: 18.626 min
Delta R.T.: -0.003 min
Response: 153936
Conc: 1.24 ug/ml