

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008920.D
Signal(s) : FID2B.ch
Acq On : 16 Aug 2021 18:22
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 17 14:26:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.521	3481166	26.237 ug/ml
12) N-OCTACOSANE	16.917	3255001	24.332 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081621\
Data File : FF008920.D
Signal(s) : FID2B.ch
Acq On : 16 Aug 2021 18:22
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 17 14:26:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072121.M
Quant Title :
QLast Update : Thu Jul 22 01:38:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

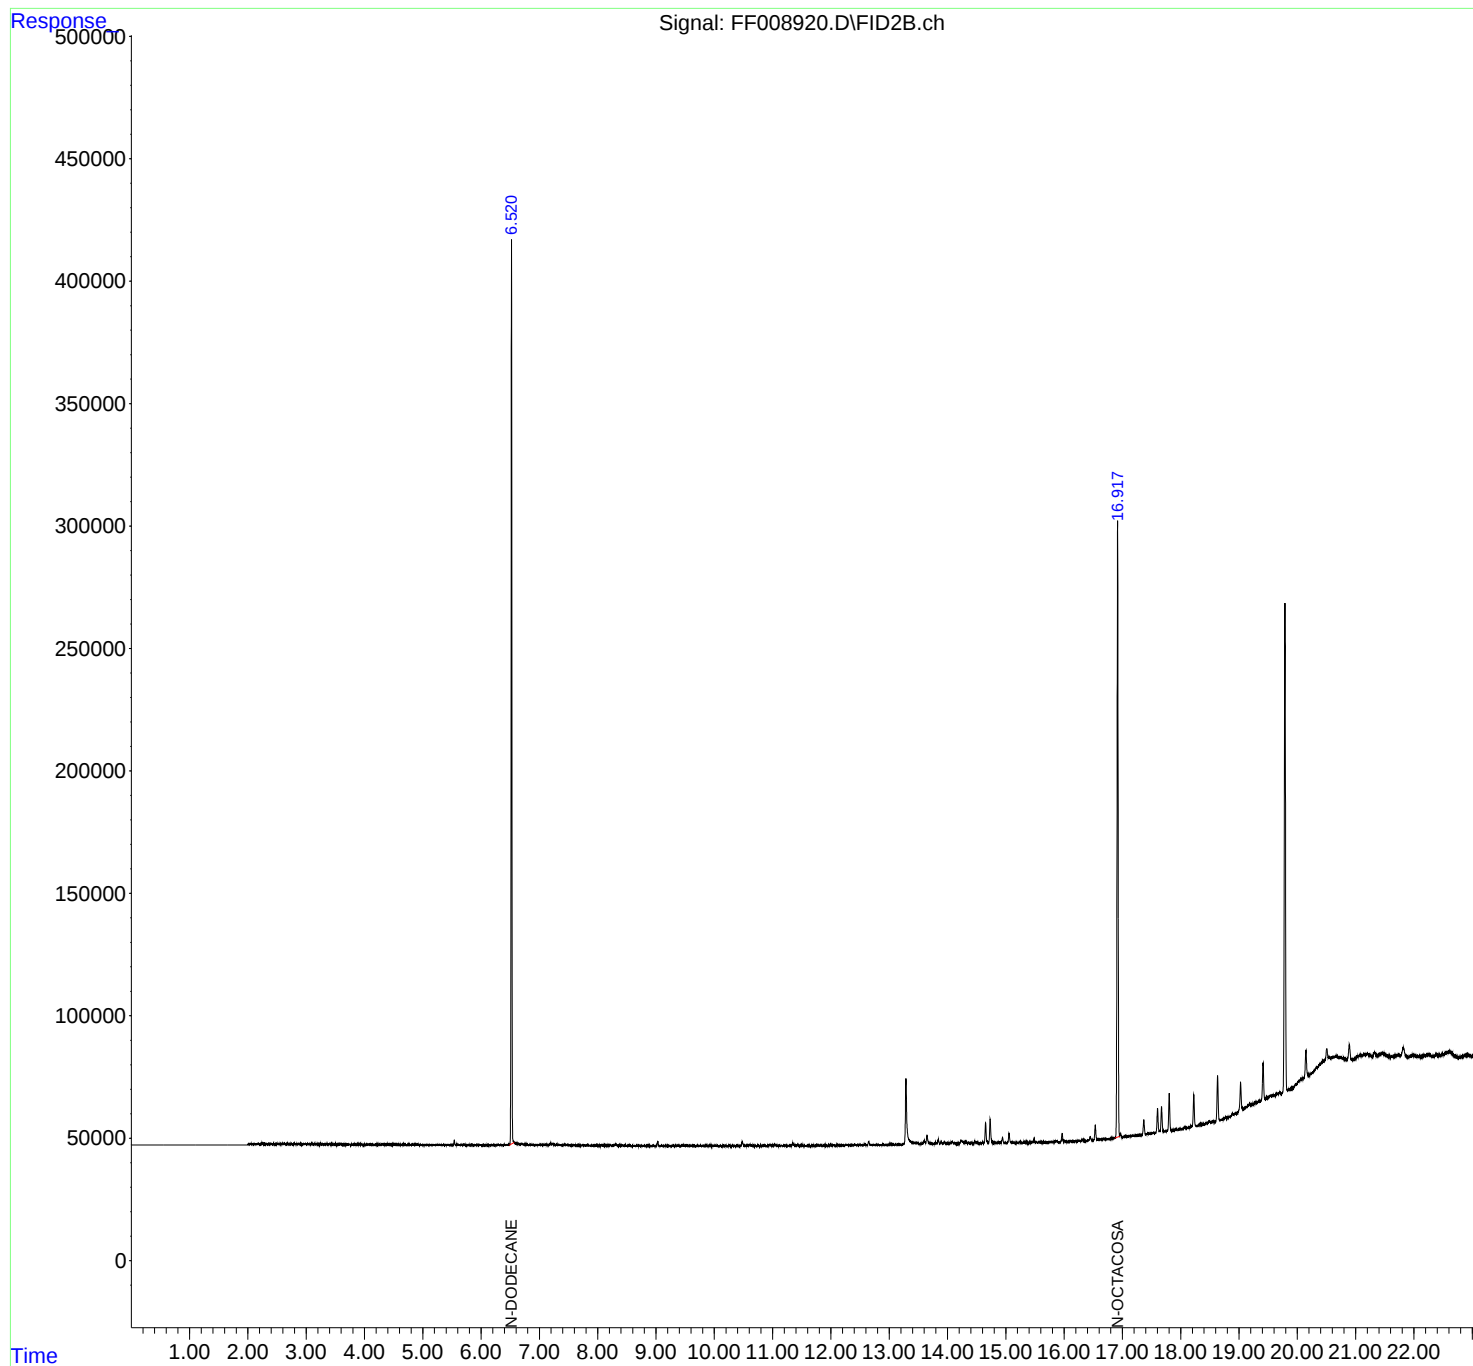


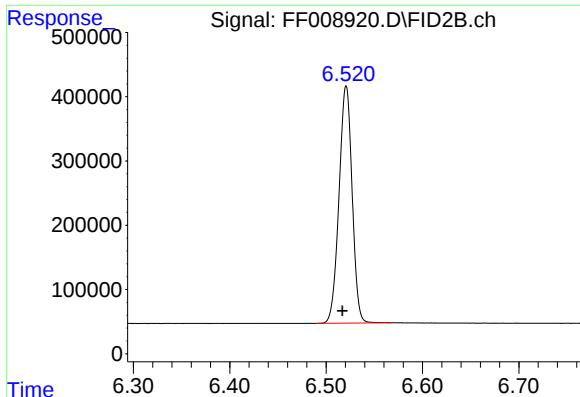

#3 N-DODECANE


R.T.: 6.521 min
Delta R.T.: 0.004 min
Response: 3481166
Conc: 26.24 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

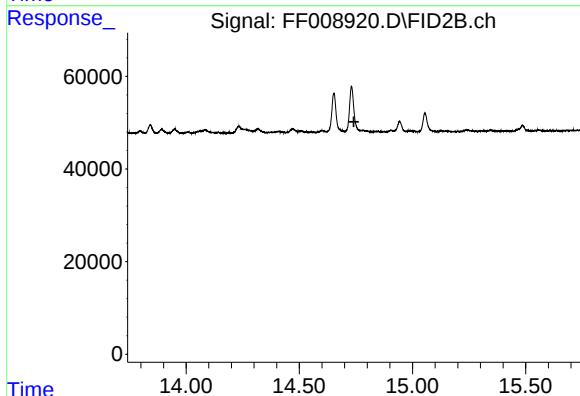

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.741 min
Response: 0
Conc: N.D.

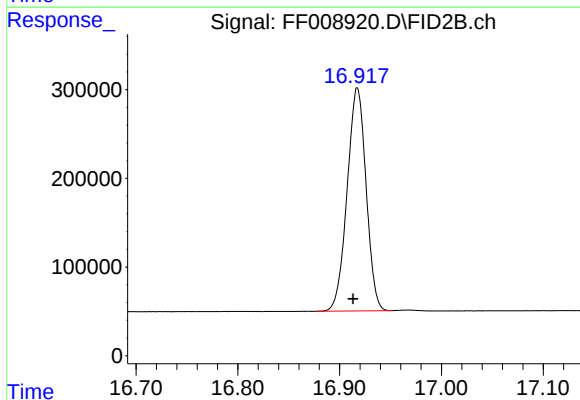

#12 N-OCTACOSANE

R.T.: 16.917 min
Delta R.T.: 0.004 min
Response: 3255001
Conc: 24.33 ug/ml