

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081823AL\
Data File : FF013199.D
Signal(s) : FID2B.ch
Acq On : 18 Aug 2023 09:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 23:53:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.034	29506	0.270 ug/ml
18) T	n-Dotriacontane (C32)	18.866	49726	0.440 ug/ml
19) T	n-Tetratriacontane (C34)	19.649	36035	0.339 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081823AL\
Data File : FF013199.D
Signal(s) : FID2B.ch
Acq On : 18 Aug 2023 09:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 23:53:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

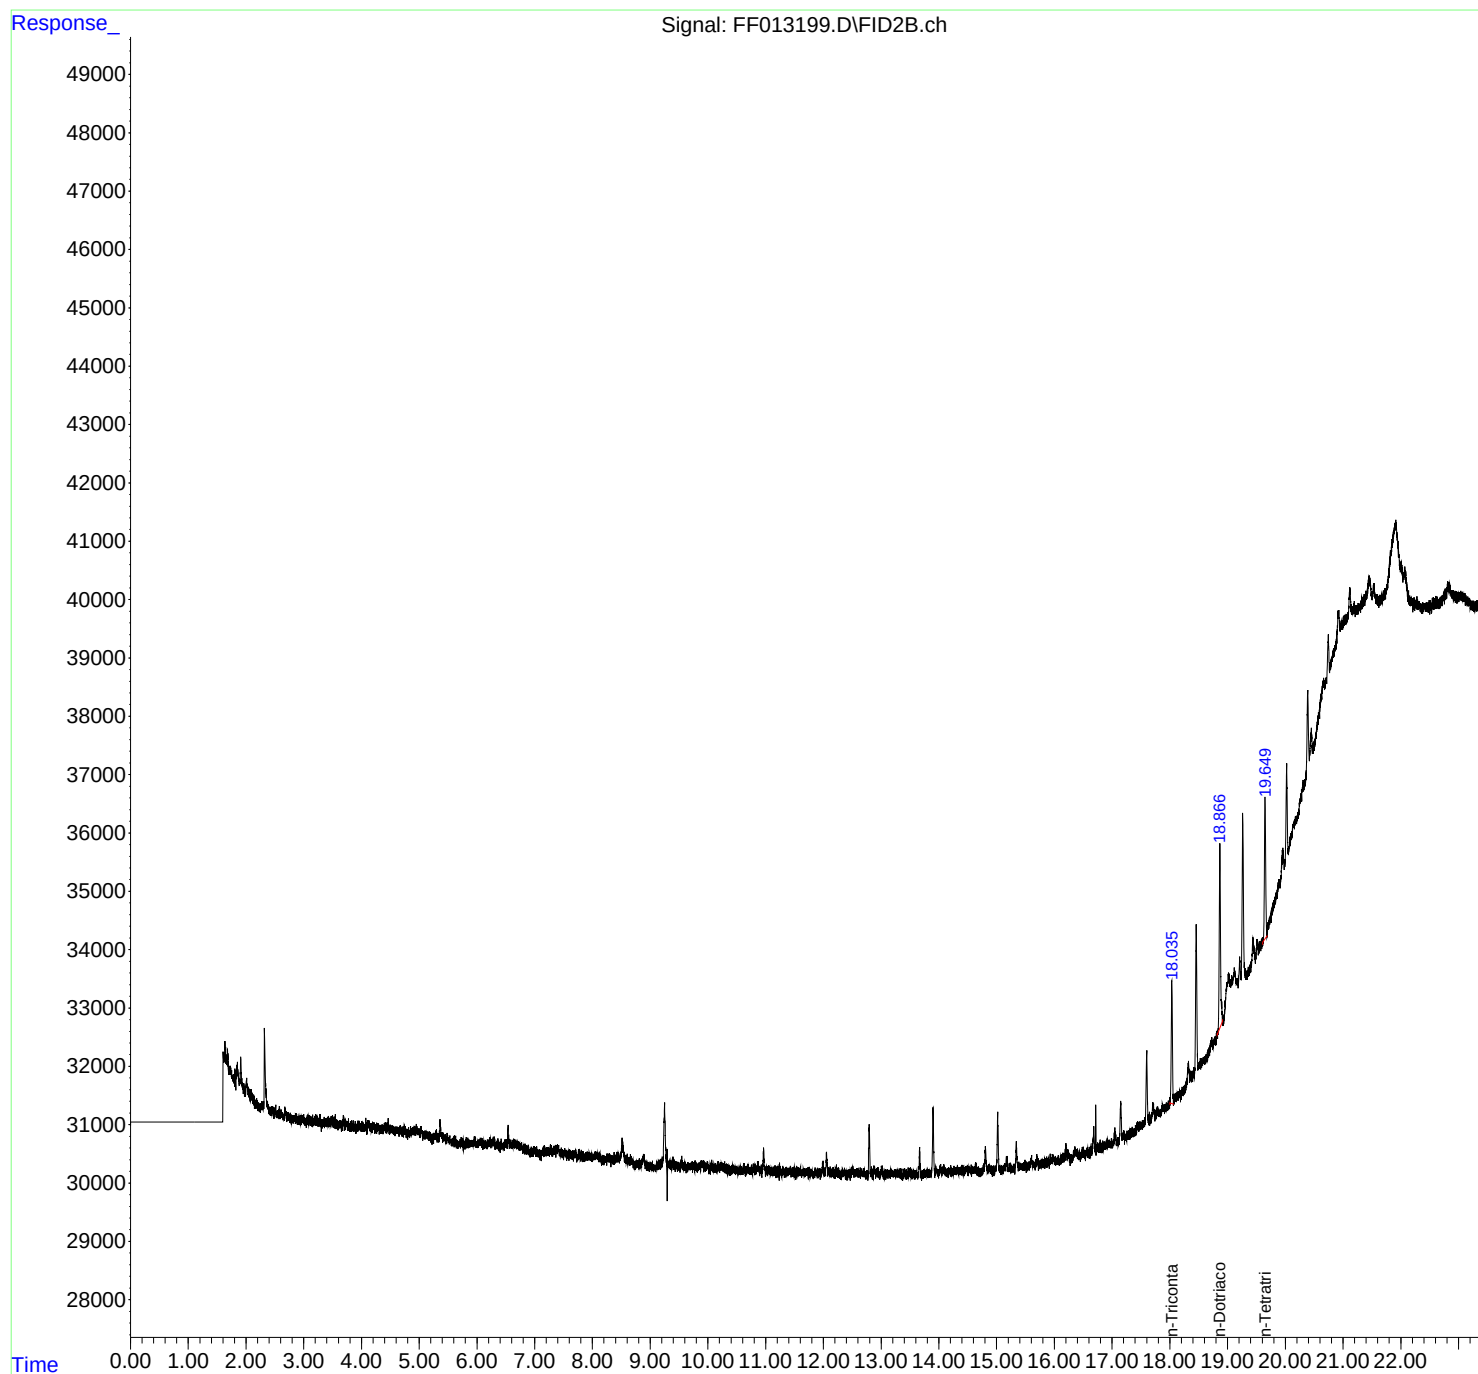


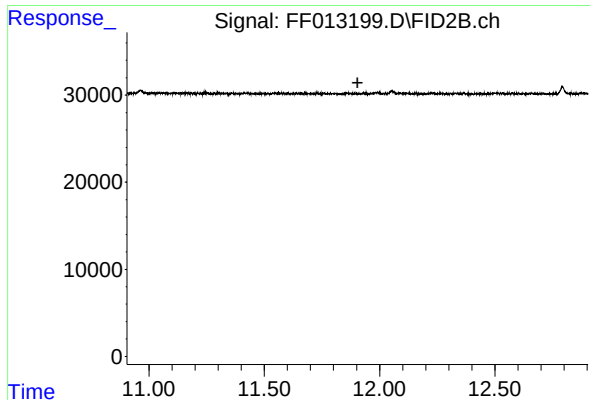

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.904 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

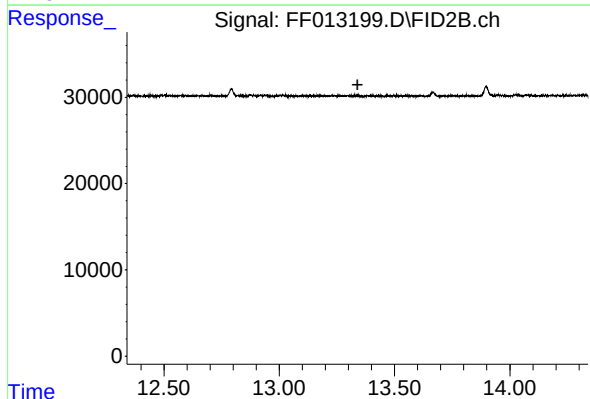


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.339 min
Response: 0
Conc: N.D.

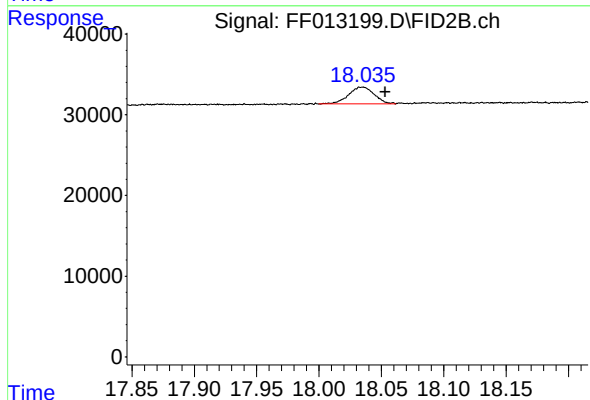


#17 n-Tricontane (C30)

R.T.: 18.034 min
Delta R.T.: -0.019 min
Response: 29506
Conc: 0.27 ug/ml

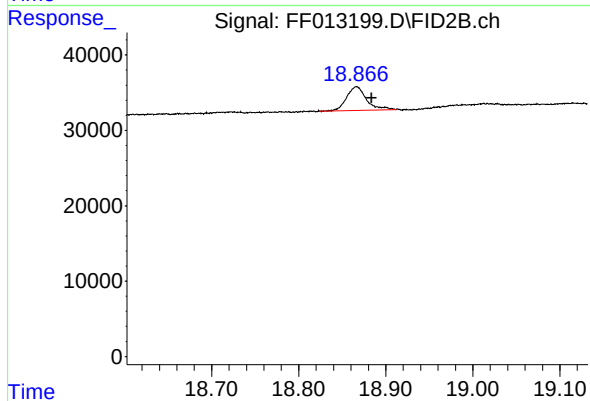

#18 n-Dotriacontane (C32)

R.T.: 18.866 min
Delta R.T.: -0.017 min
Response: 49726
Conc: 0.44 ug/ml

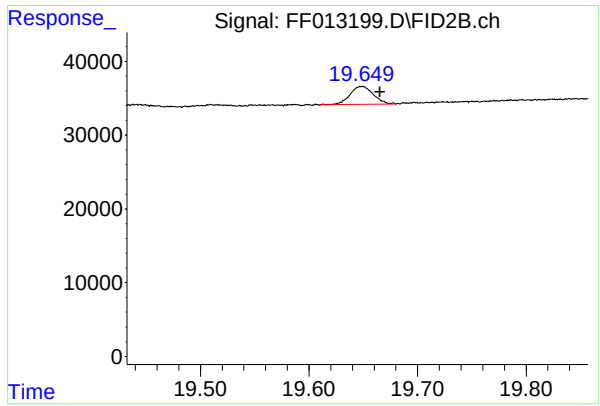

#19 n-Tetratriacontane (C34)

R.T.: 19.649 min
Delta R.T.: -0.017 min
Response: 36035
Conc: 0.34 ug/ml

Instrument :

FID_F

ClientSampleId :