

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081922\
Data File : FF011269.D
Signal(s) : FID2B.ch
Acq On : 19 Aug 2022 13:41
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 19 19:00:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.522	2254754	17.912 ug/ml
12)	N-OCTACOSANE	16.965	2125120	17.604 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF081922\
Data File : FF011269.D
Signal(s) : FID2B.ch
Acq On : 19 Aug 2022 13:41
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 19 19:00:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

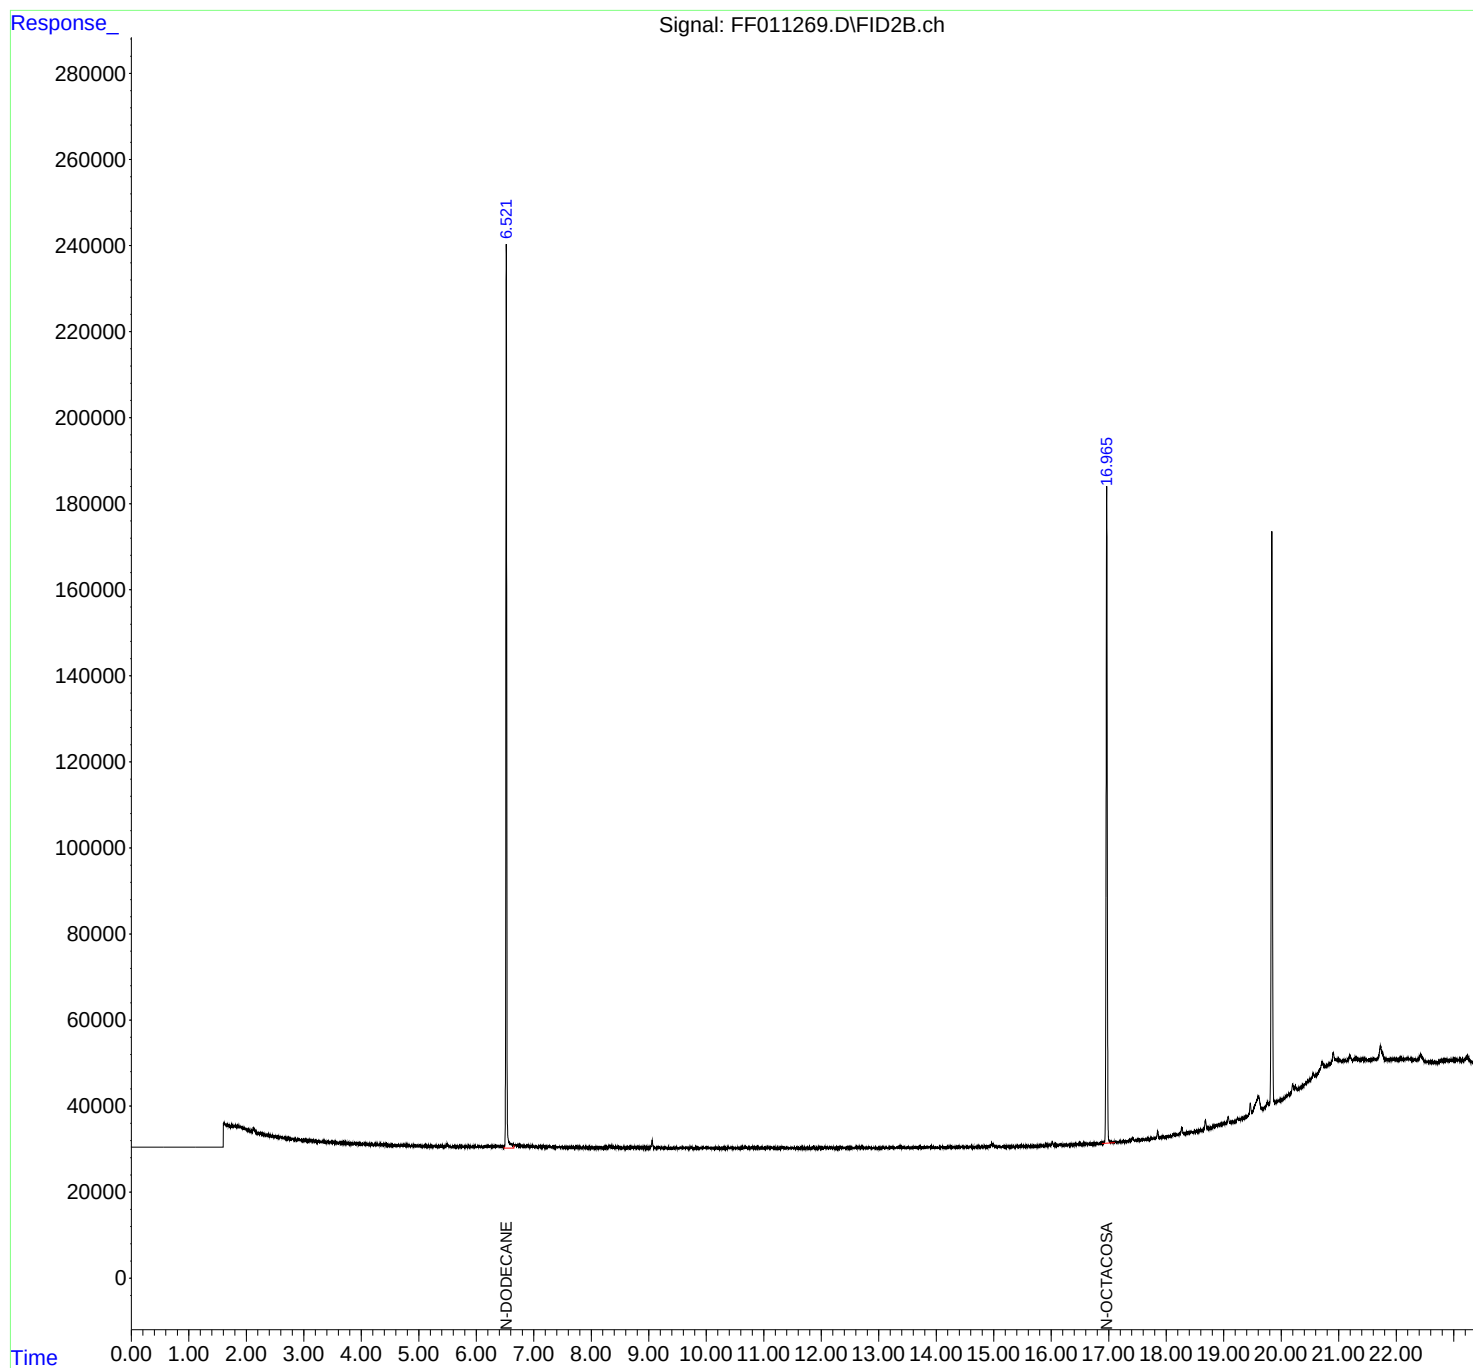


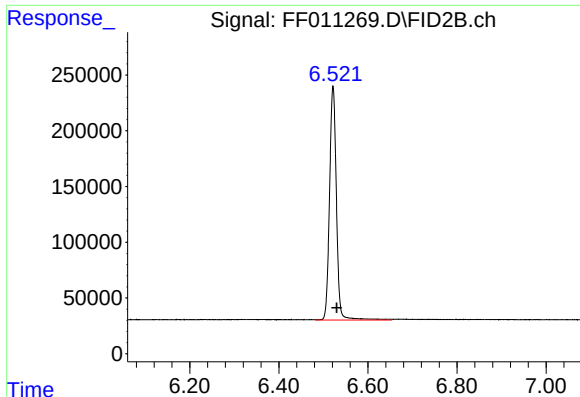

#3 N-DODECANE


R.T.: 6.522 min
Delta R.T.: -0.008 min
Response: 2254754
Conc: 17.91 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

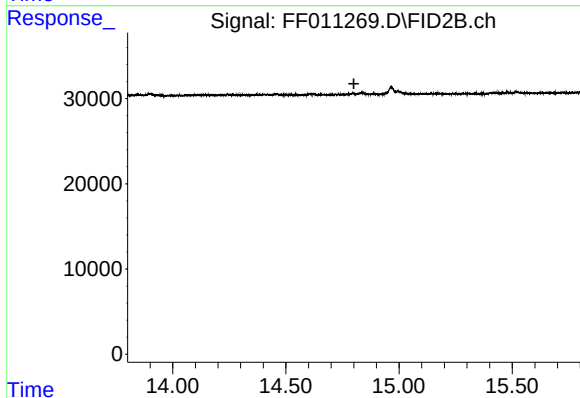

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.801 min
Response: 0
Conc: N.D.

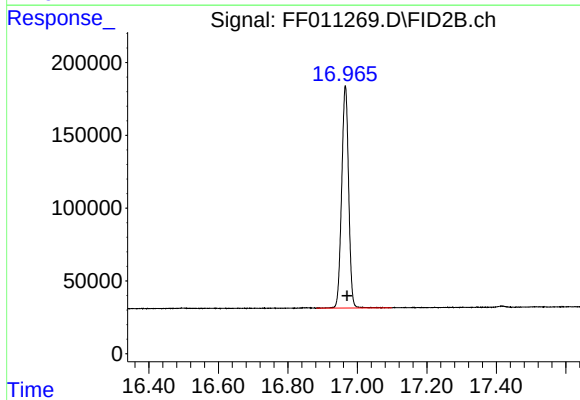

#12 N-OCTACOSANE

R.T.: 16.965 min
Delta R.T.: -0.006 min
Response: 2125120
Conc: 17.60 ug/ml