

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001877.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 10:38
 Operator : AJ\SJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:19:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.301	70324	0.557 ug/ml
Target Compounds			
3) N-DODECANE	6.092	130772	0.877 ug/ml
4) N-TETRADECANE	7.861	227441	1.509 ug/ml
5) N-HEXADECANE	9.524	112806	0.754 ug/ml
7) N-EICOSANE	12.183	372028	2.496 ug/ml
8) N-DOCOSANE	13.396	268138	1.836 ug/ml
10) N-TETRACOSANE	14.508	429037	3.008 ug/ml
11) N-HEXACOSANE	15.526	243363	1.728 ug/ml
12) N-OCTACOSANE	16.472	375773	2.680 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001877.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 10:38
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:19:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

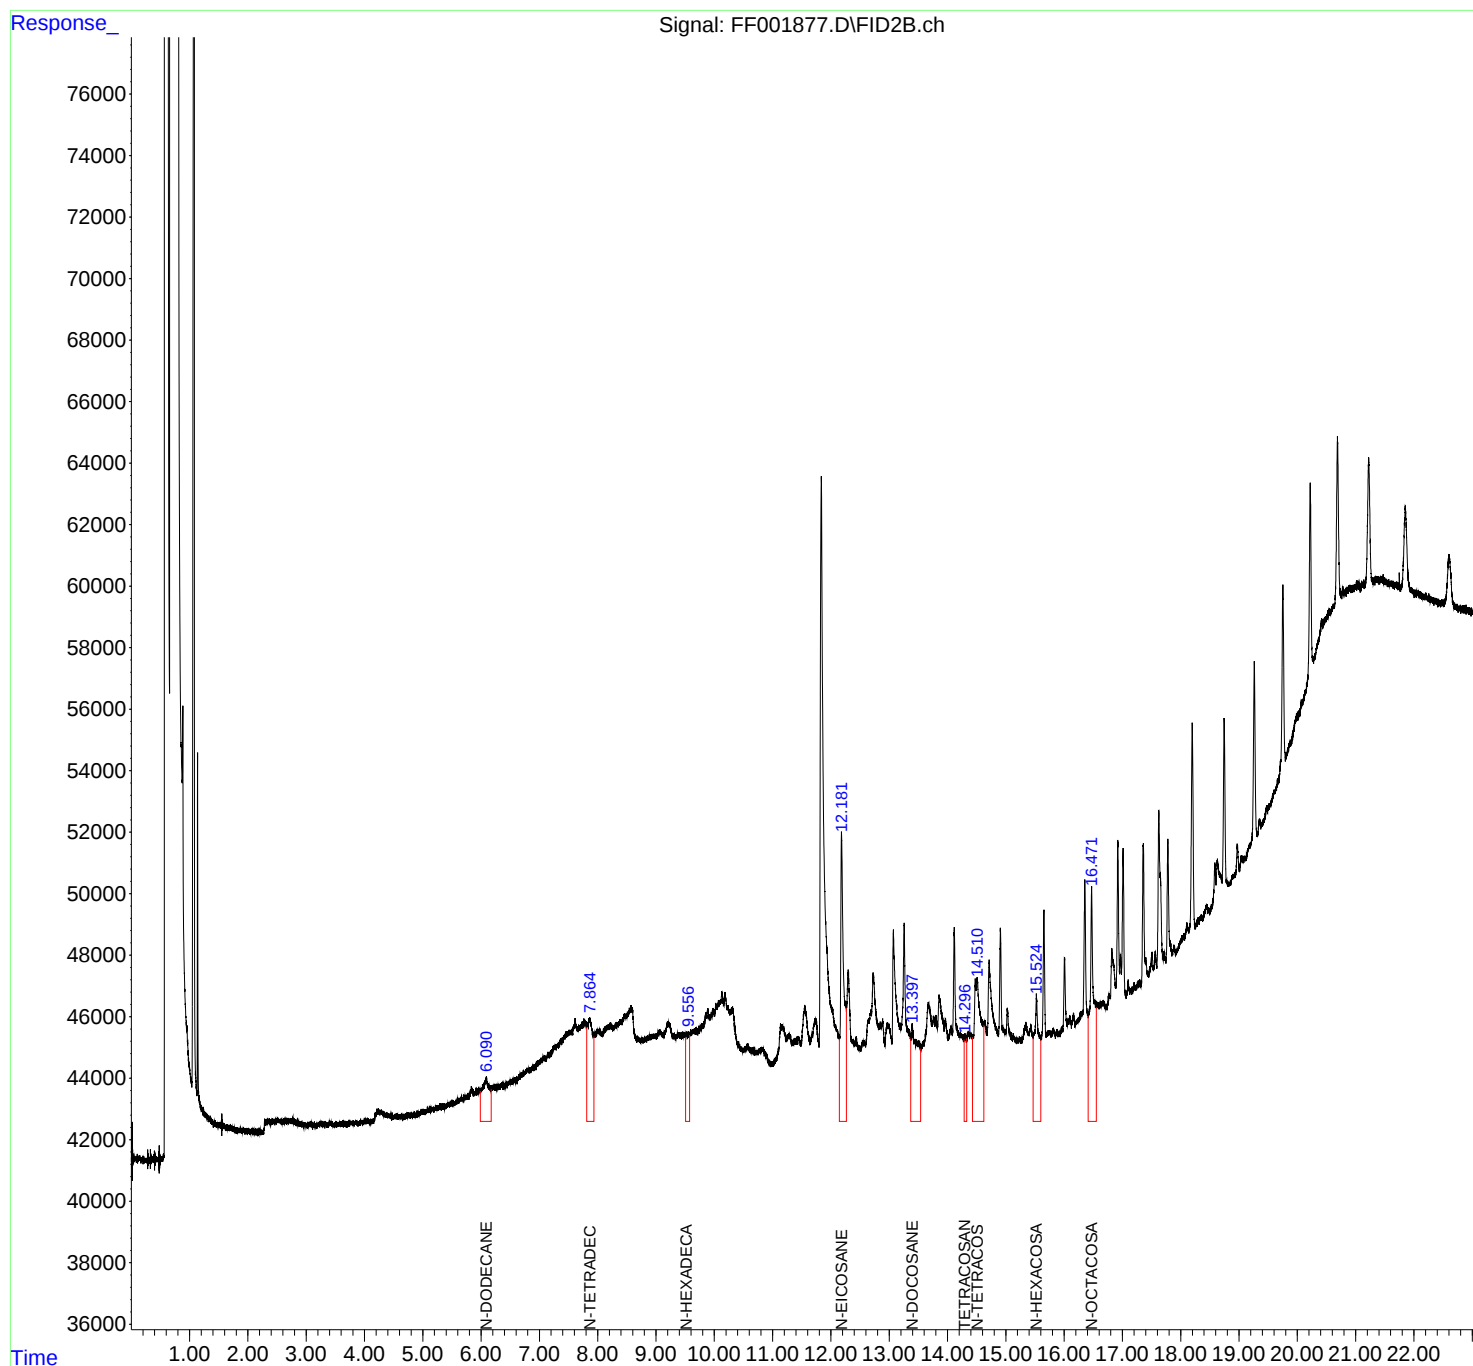


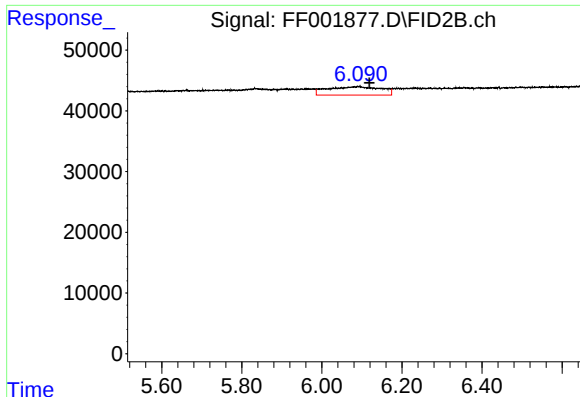

#3 N-DODECANE


R.T.: 6.092 min
Delta R.T.: -0.027 min
Response: 130772
Conc: 0.88 ug/ml

Instrument :
FID_F
ClientSampleId :

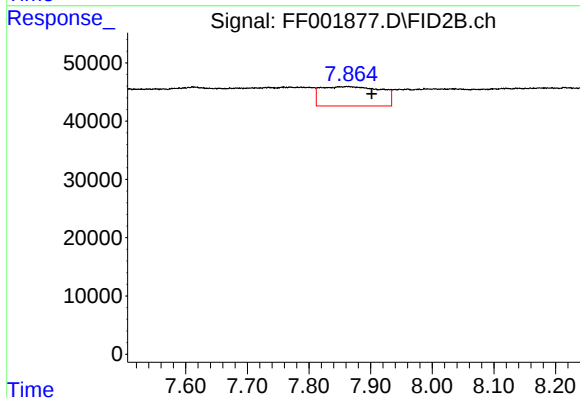


#4 N-TETRADECANE

R.T.: 7.861 min
Delta R.T.: -0.040 min
Response: 227441
Conc: 1.51 ug/ml

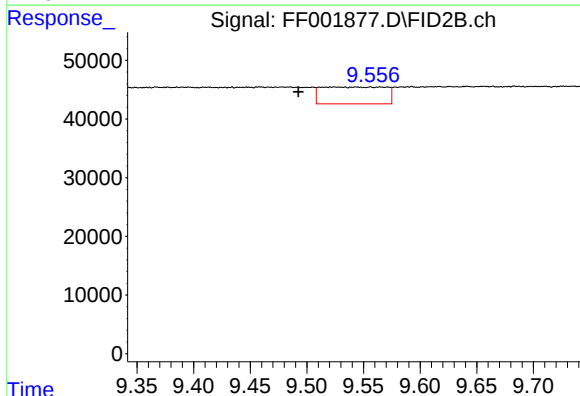


#5 N-HEXADECANE

R.T.: 9.524 min
Delta R.T.: 0.032 min
Response: 112806
Conc: 0.75 ug/ml

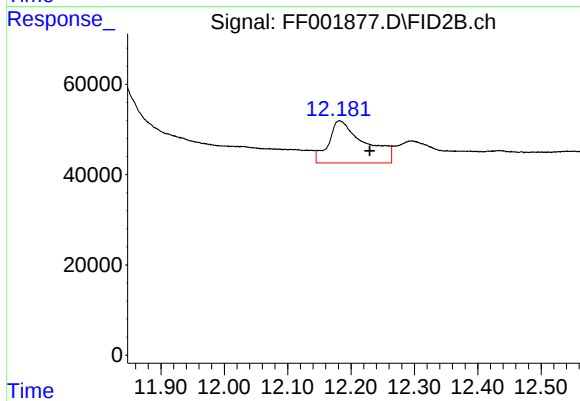

#7 N-EICOSANE


R.T.: 12.183 min
Delta R.T.: -0.046 min
Response: 372028
Conc: 2.50 ug/ml

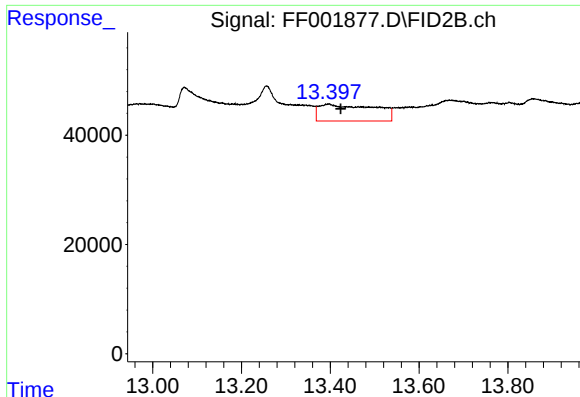

#8 N-DOCOSANE


R.T.: 13.396 min
Delta R.T.: -0.028 min
Response: 268138
Conc: 1.84 ug/ml

Instrument :
FID_F
ClientSampleId :

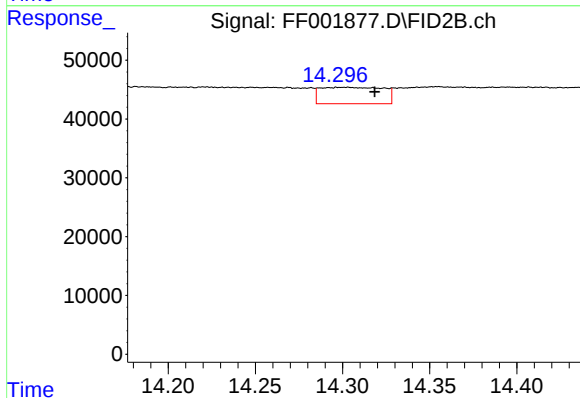


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.301 min
Delta R.T.: -0.018 min
Response: 70324
Conc: 0.56 ug/ml

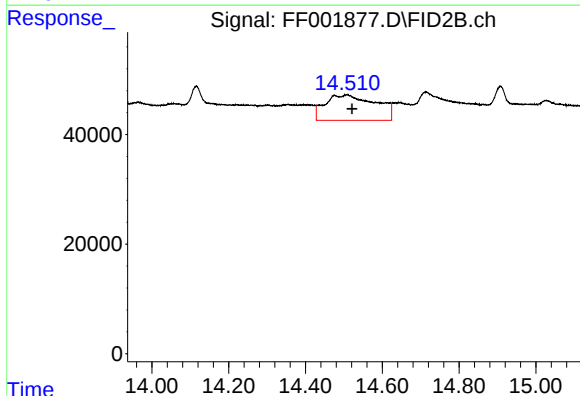


#10 N-TETRACOSANE

R.T.: 14.508 min
Delta R.T.: -0.013 min
Response: 429037
Conc: 3.01 ug/ml

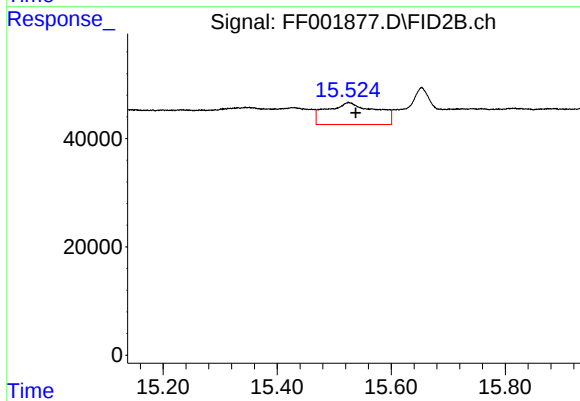

#11 N-HEXACOSANE

R.T.: 15.526 min
Delta R.T.: -0.012 min
Response: 243363
Conc: 1.73 ug/ml

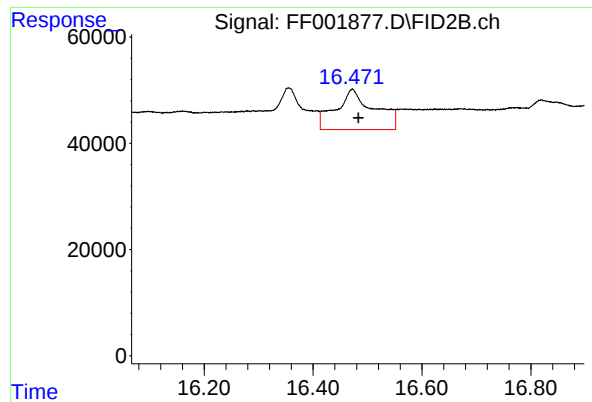

#12 N-OCTACOSANE

R.T.: 16.472 min
Delta R.T.: -0.011 min
Response: 375773
Conc: 2.68 ug/ml

Instrument :
FID_F
ClientSampleId :