

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001879.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 12:04
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:20:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.307	6986403	55.315 ug/ml
Target Compounds			
2) N-DECANE	4.092	7651193	52.465 ug/ml
3) N-DODECANE	6.100	7734084	51.885 ug/ml
4) N-TETRADECANE	7.885	7855750	52.122 ug/ml
5) N-HEXADECANE	9.477	7932379	52.987 ug/ml
6) N-OCTADECANE	10.913	7975432	52.914 ug/ml
7) N-EICOSANE	12.217	7857266	52.717 ug/ml
8) N-DOCOSANE	13.410	7906775	54.131 ug/ml
10) N-TETRACOSANE	14.510	7910434	55.453 ug/ml
11) N-HEXACOSANE	15.527	7818752	55.506 ug/ml
12) N-OCTACOSANE	16.473	7746249	55.244 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001879.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 12:04
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:20:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

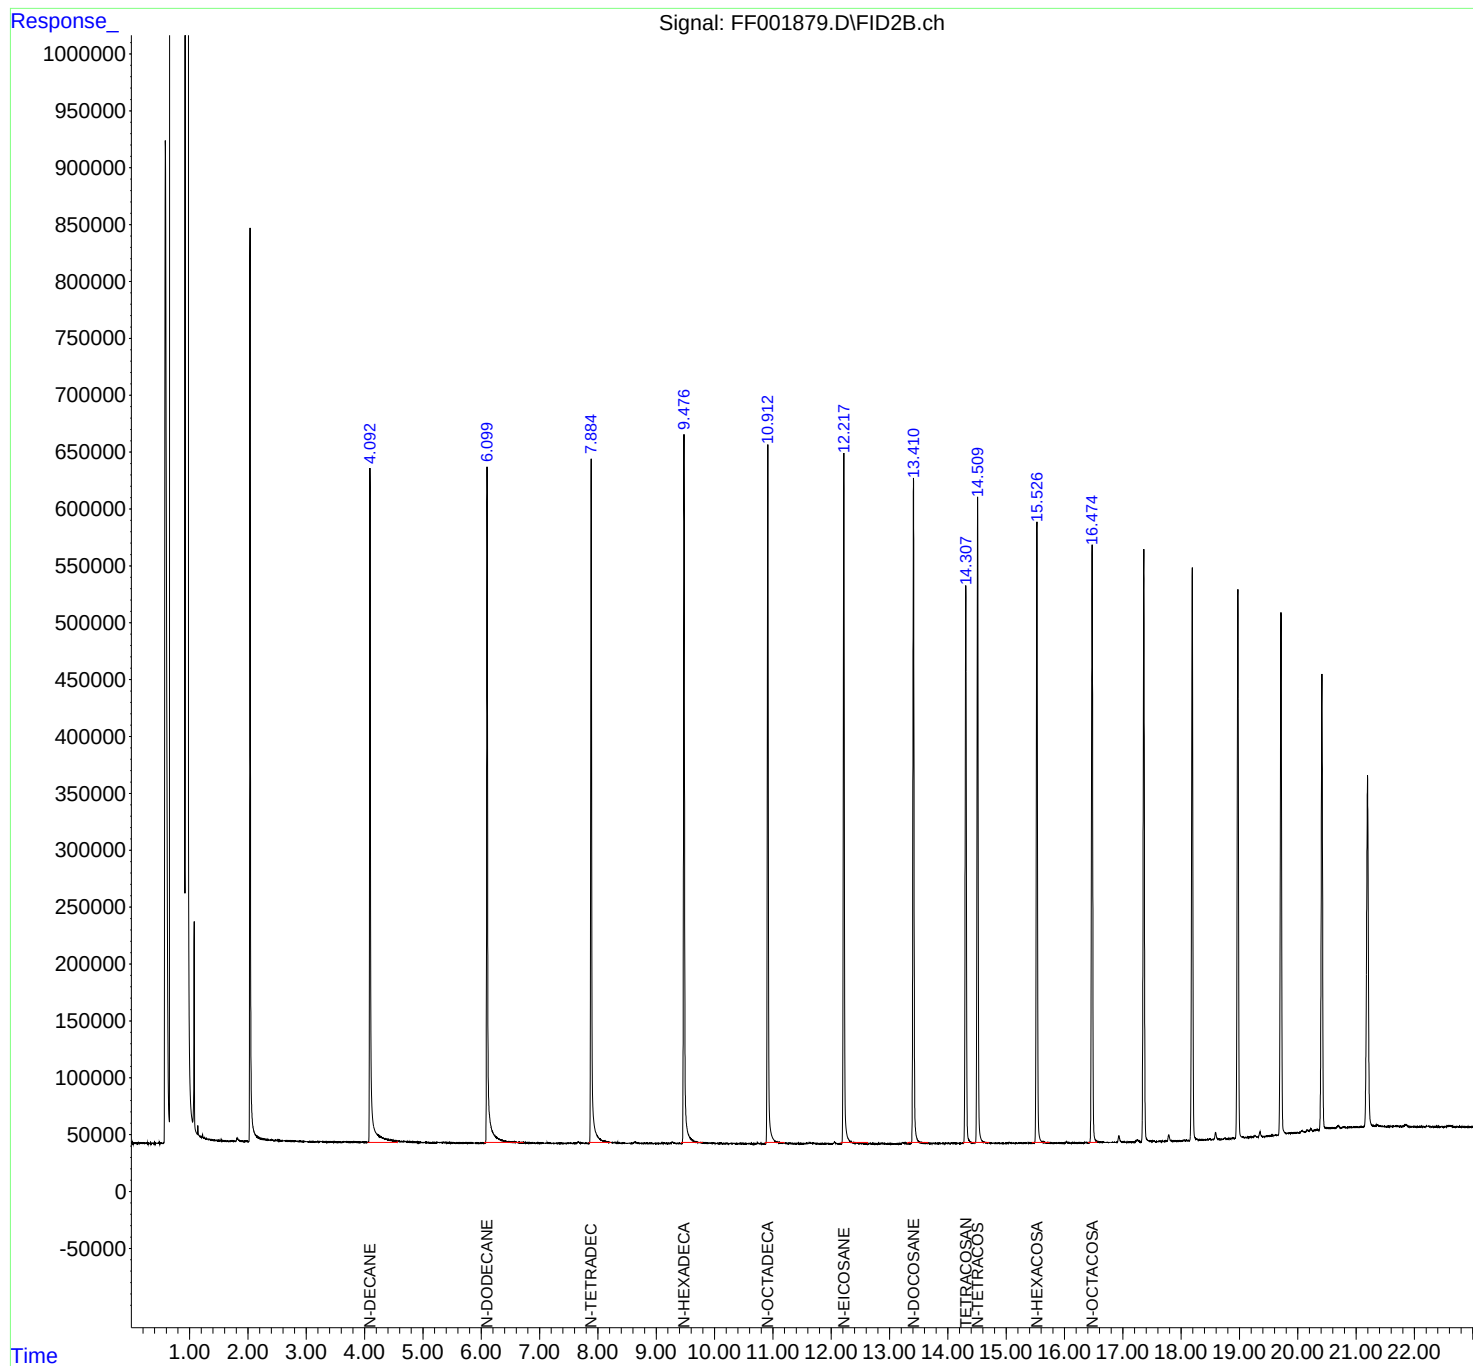


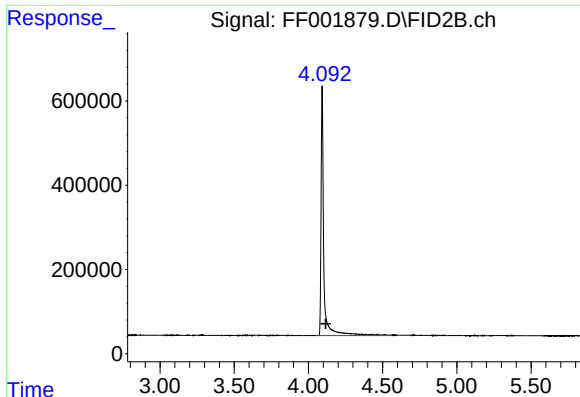

#2 N-DECANE


R.T.: 4.092 min
Delta R.T.: -0.025 min
Response: 7651193
Conc: 52.47 ug/ml

Instrument :
FID_F
ClientSampleId :

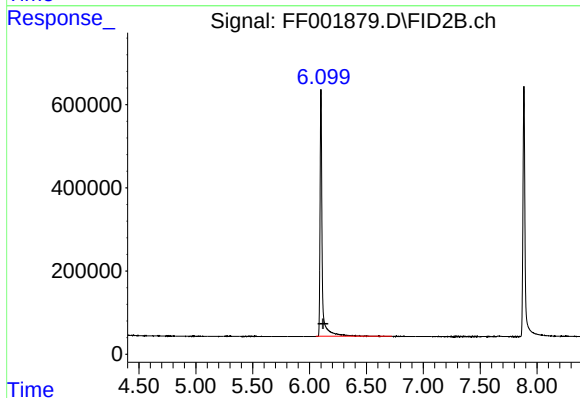


#3 N-DODECANE

R.T.: 6.100 min
Delta R.T.: -0.019 min
Response: 7734084
Conc: 51.88 ug/ml

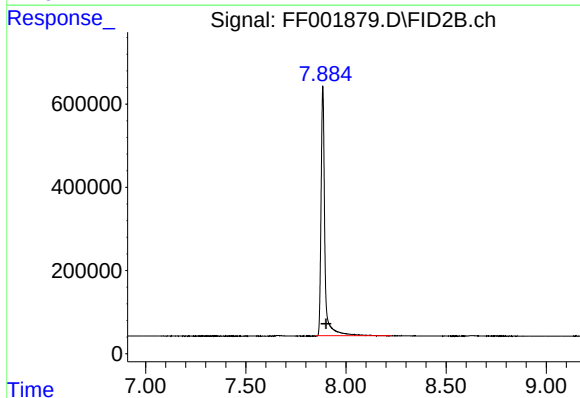


#4 N-TETRADECANE

R.T.: 7.885 min
Delta R.T.: -0.017 min
Response: 7855750
Conc: 52.12 ug/ml

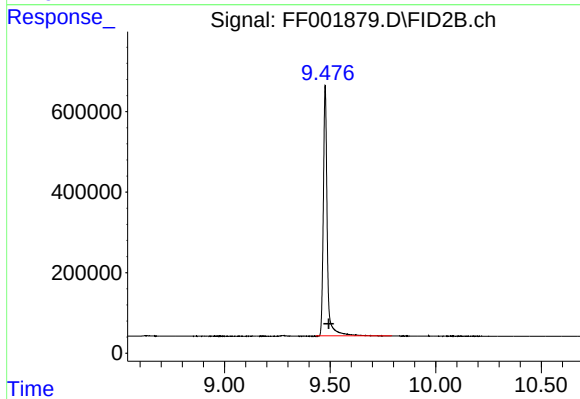

#5 N-HEXADECANE


R.T.: 9.477 min
Delta R.T.: -0.016 min
Response: 7932379
Conc: 52.99 ug/ml

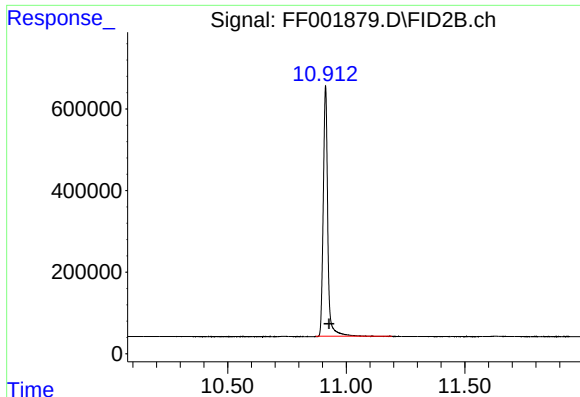

#6 N-OCTADECANE


R.T.: 10.913 min
Delta R.T.: -0.014 min
Response: 7975432
Conc: 52.91 ug/ml

Instrument :
FID_F
ClientSampleId :

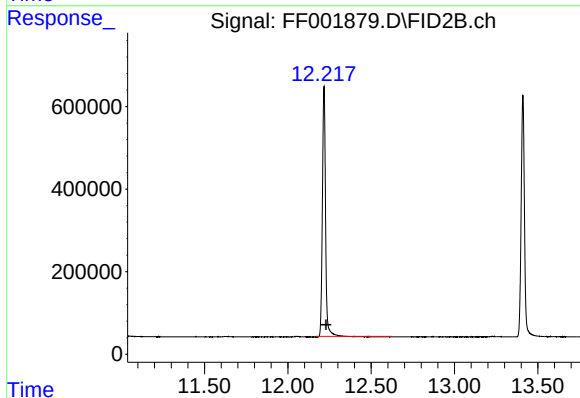


#7 N-EICOSANE

R.T.: 12.217 min
Delta R.T.: -0.013 min
Response: 7857266
Conc: 52.72 ug/ml

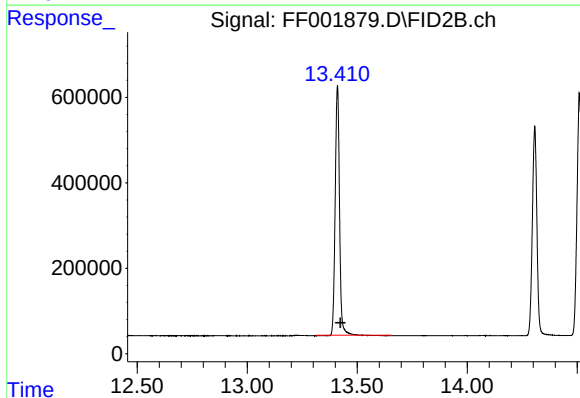


#8 N-DOCOSANE

R.T.: 13.410 min
Delta R.T.: -0.013 min
Response: 7906775
Conc: 54.13 ug/ml

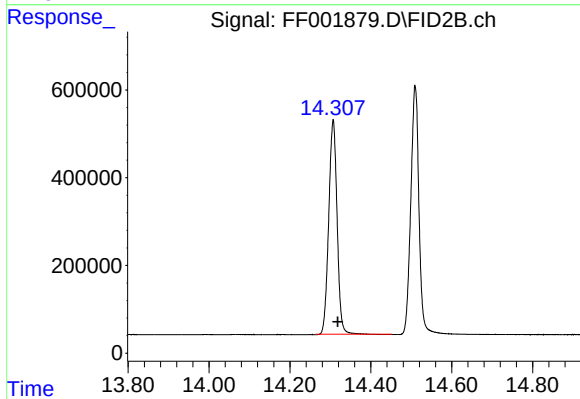

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.307 min
Delta R.T.: -0.012 min
Response: 6986403
Conc: 55.32 ug/ml

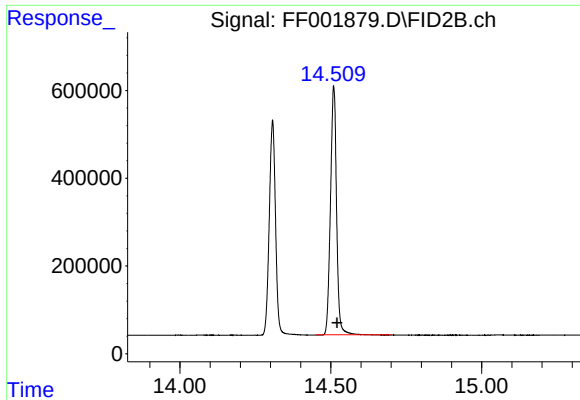

#10 N-TETRACOSANE


R.T.: 14.510 min
Delta R.T.: -0.011 min
Response: 7910434
Conc: 55.45 ug/ml

Instrument :
FID_F
ClientSampleId :

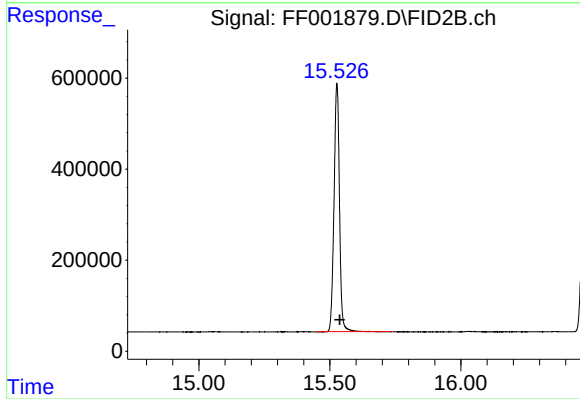

#11 N-HEXACOSANE

R.T.: 15.527 min
Delta R.T.: -0.011 min
Response: 7818752
Conc: 55.51 ug/ml

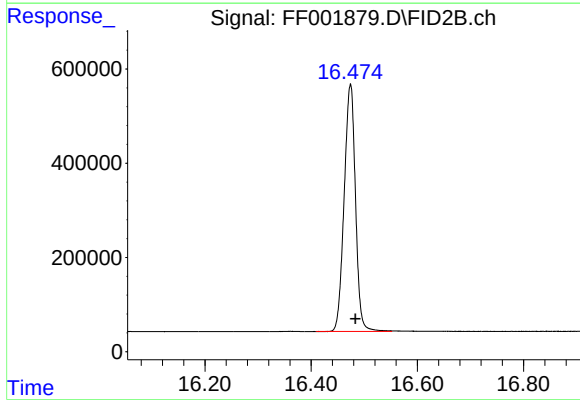

#12 N-OCTACOSANE

R.T.: 16.473 min
Delta R.T.: -0.010 min
Response: 7746249
Conc: 55.24 ug/ml