

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082018\  
 Data File : FF001881.D  
 Signal(s) : FID2B.ch  
 Acq On : 20 Aug 2018 14:09  
 Operator : AJ\SJ  
 Sample : PB112195BL  
 Misc :  
 ALS Vial : 55 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: Sample.e  
 Quant Time: Aug 21 03:20:19 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073018.M  
 Quant Title :  
 QLast Update : Fri Aug 03 12:00:27 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units   |
|-------------------------------|---------|----------|--------------|
| -----                         |         |          |              |
| System Monitoring Compounds   |         |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.305  | 2934239  | 23.232 ug/ml |
| Target Compounds              |         |          |              |
| 2) N-DECANE                   | 4.135   | 504      | 0.003 ug/ml  |
| 8) N-DOCOSANE                 | 13.458  | 10798    | 0.074 ug/ml  |
| 11) N-HEXACOSANE              | 15.604f | 33017    | 0.234 ug/ml  |
| 12) N-OCTACOSANE              | 16.518  | 78532    | 0.560 ug/ml  |
| -----                         |         |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082018\  
Data File : FF001881.D  
Signal(s) : FID2B.ch  
Acq On : 20 Aug 2018 14:09  
Operator : AJ\SJ  
Sample : PB112195BL  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: Sample.e  
Quant Time: Aug 21 03:20:19 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073018.M  
Quant Title :  
QLast Update : Fri Aug 03 12:00:27 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

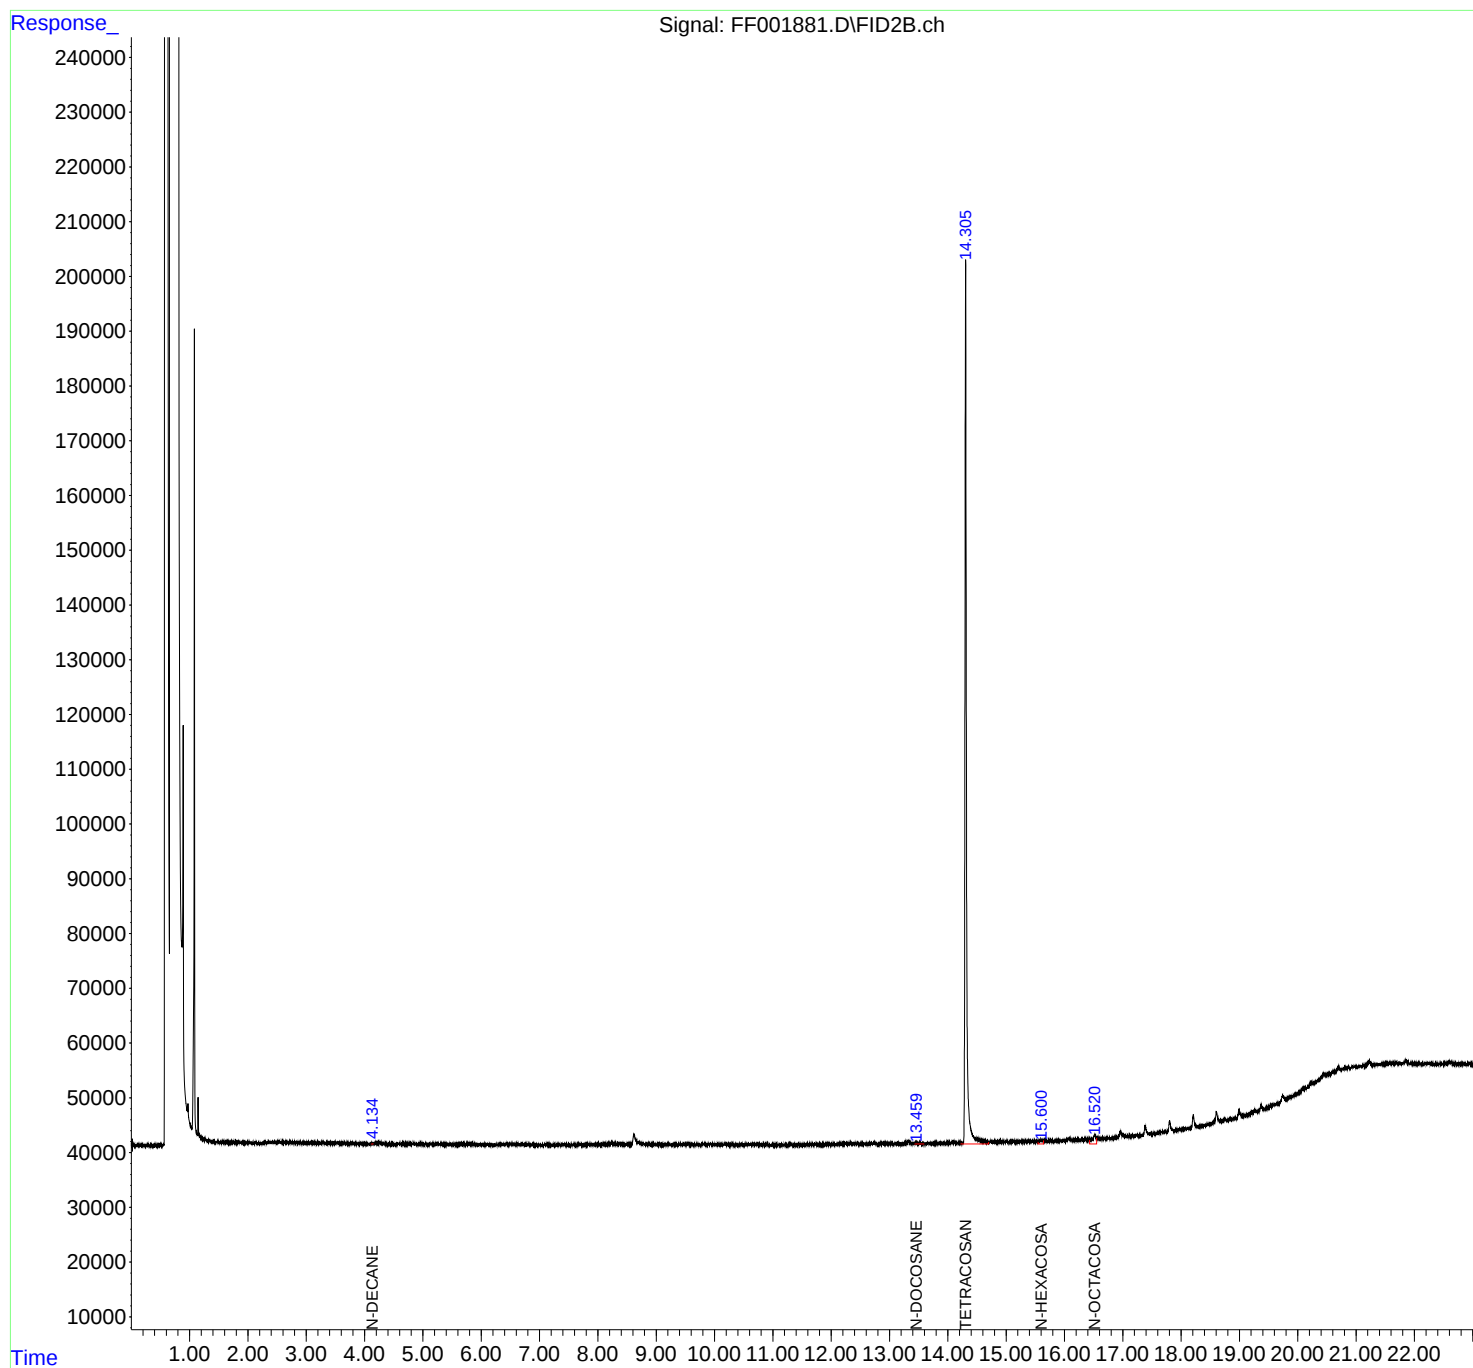


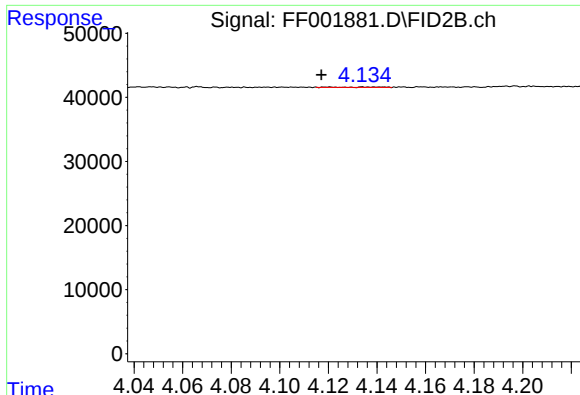

#2 N-DECANE


R.T.: 4.135 min  
Delta R.T.: 0.018 min  
Response: 504  
Conc: 0.00 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

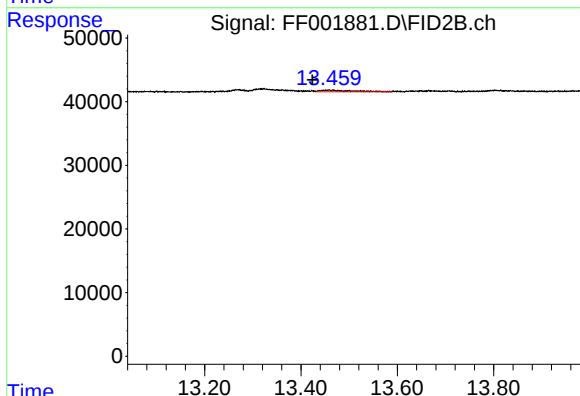


#8 N-DOCOSANE

R.T.: 13.458 min  
Delta R.T.: 0.034 min  
Response: 10798  
Conc: 0.07 ug/ml

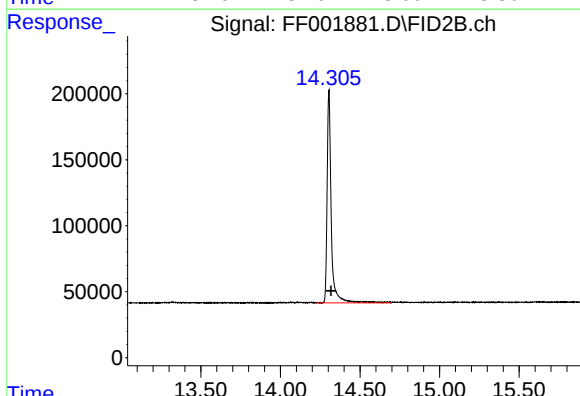


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.305 min  
Delta R.T.: -0.014 min  
Response: 2934239  
Conc: 23.23 ug/ml

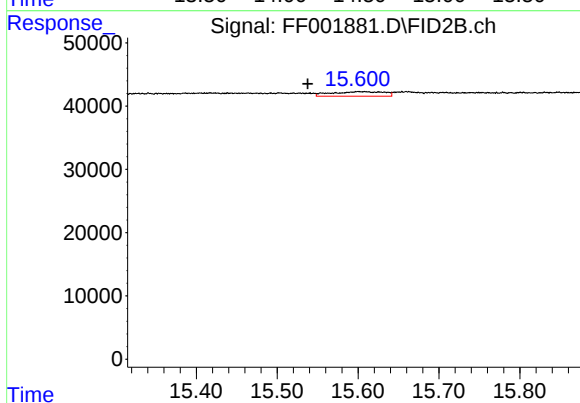

#11 N-HEXACOSANE

R.T.: 15.604 min  
Delta R.T.: 0.066 min  
Response: 33017  
Conc: 0.23 ug/ml

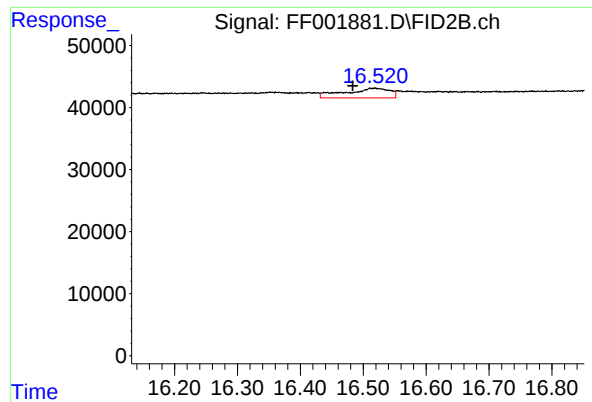

#12 N-OCTACOSANE

R.T.: 16.518 min  
Delta R.T.: 0.035 min  
Response: 78532  
Conc: 0.56 ug/ml

Instrument :  
FID\_F  
ClientSampleId :