

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001882.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 14:40
 Operator : AJ\SJ
 Sample : PB112195BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:20:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.306	2202599	17.439 ug/ml
Target Compounds			
2) N-DECANE	4.098	2331549	15.988 ug/ml
3) N-DODECANE	6.105	2450977	16.443 ug/ml
4) N-TETRADECANE	7.887	2553628	16.943 ug/ml
5) N-HEXADECANE	9.478	2569439	17.163 ug/ml
6) N-OCTADECANE	10.912	2627569	17.433 ug/ml
7) N-EICOSANE	12.216	2667325	17.896 ug/ml
8) N-DOCOSANE	13.410	2721134	18.629 ug/ml
10) N-TETRACOSANE	14.508	2838392	19.897 ug/ml
11) N-HEXACOSANE	15.525	2681282	19.035 ug/ml
12) N-OCTACOSANE	16.472	2705432	19.294 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001882.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 14:40
Operator : AJ\SJ
Sample : PB112195BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:20:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

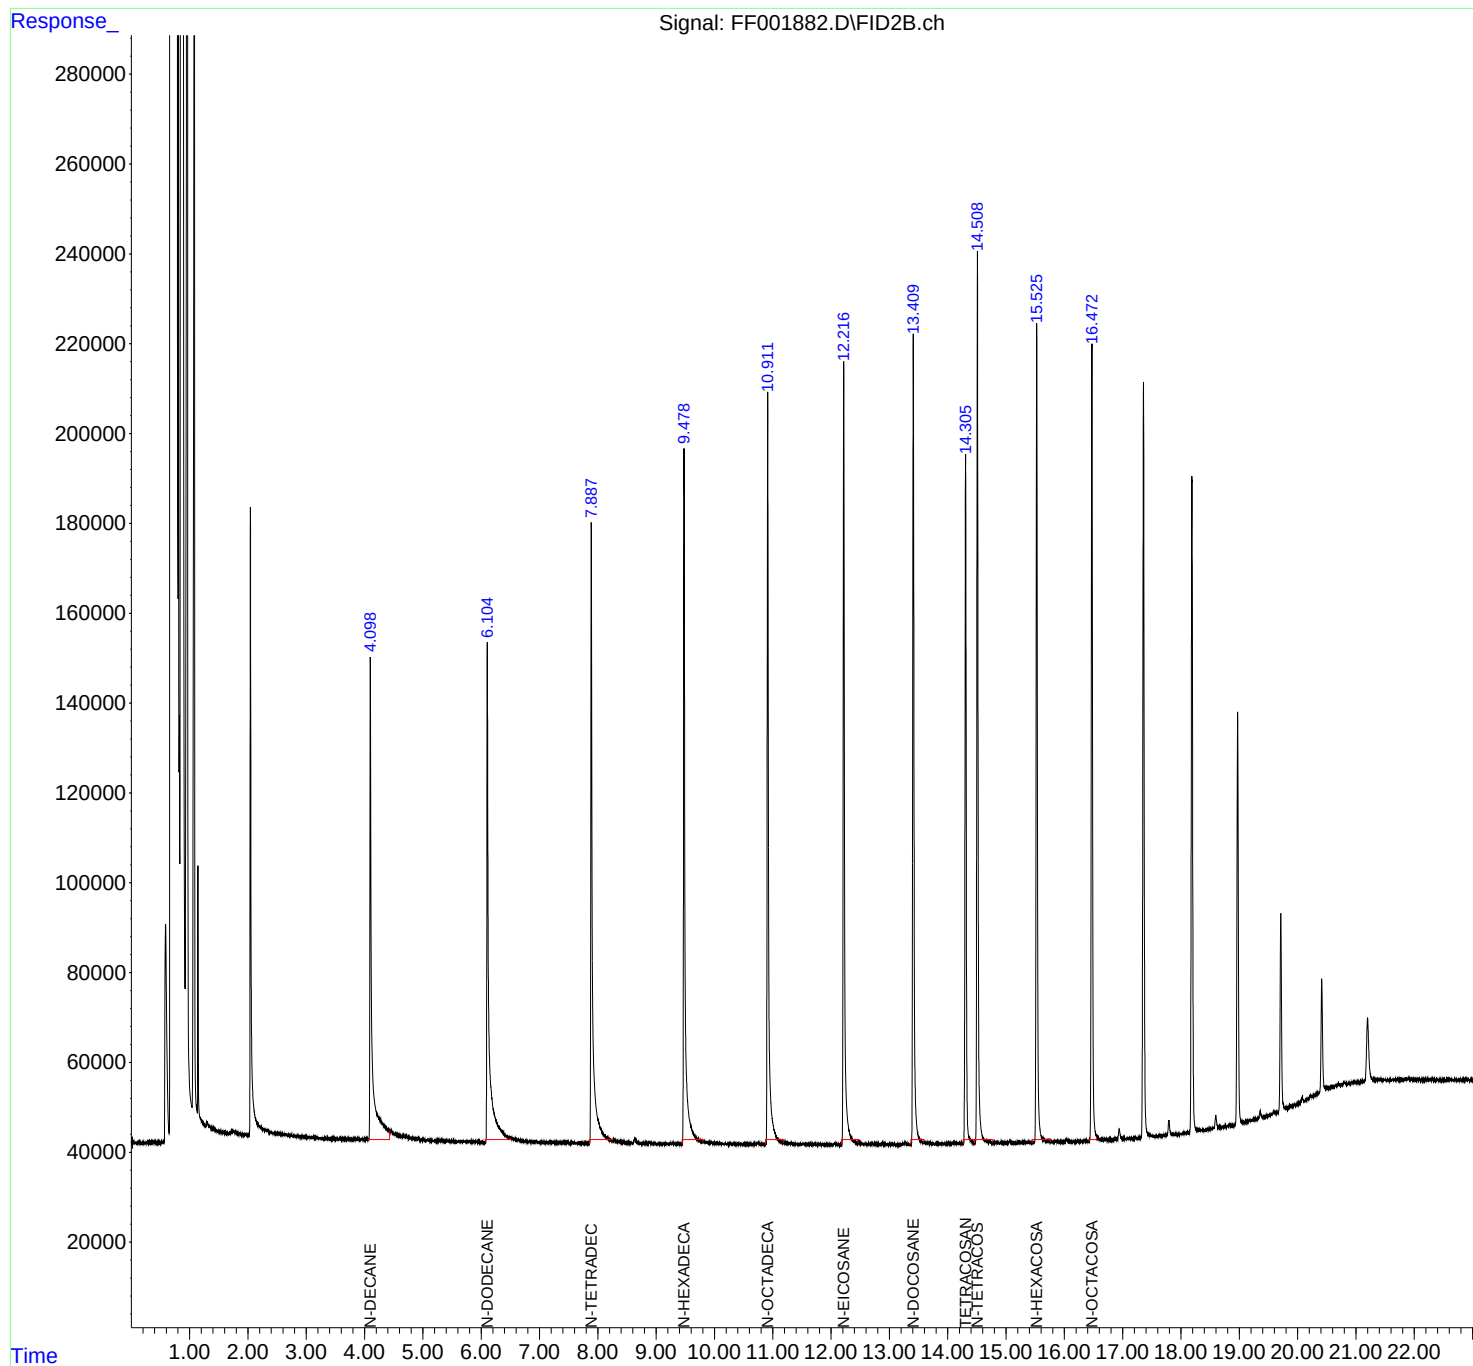


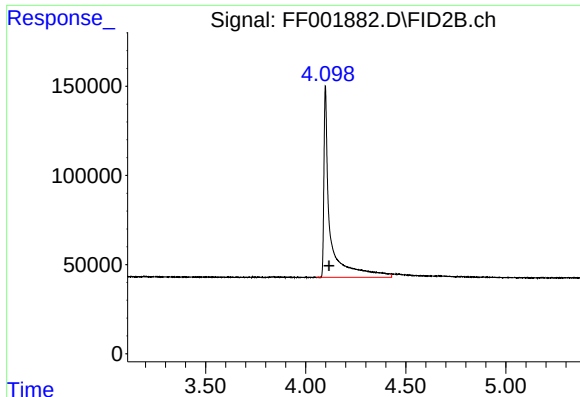

#2 N-DECANE


R.T.: 4.098 min
Delta R.T.: -0.019 min
Response: 2331549
Conc: 15.99 ug/ml

Instrument :
FID_F
ClientSampleId :

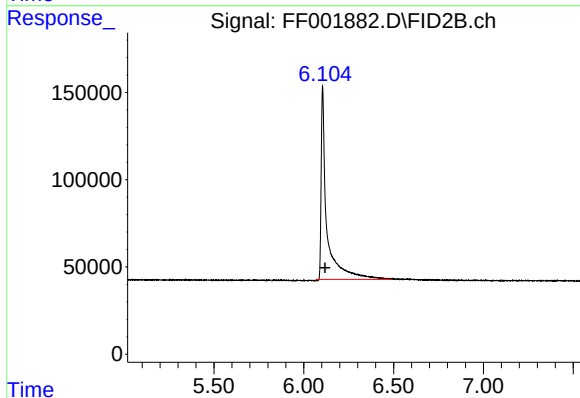


#3 N-DODECANE

R.T.: 6.105 min
Delta R.T.: -0.014 min
Response: 2450977
Conc: 16.44 ug/ml

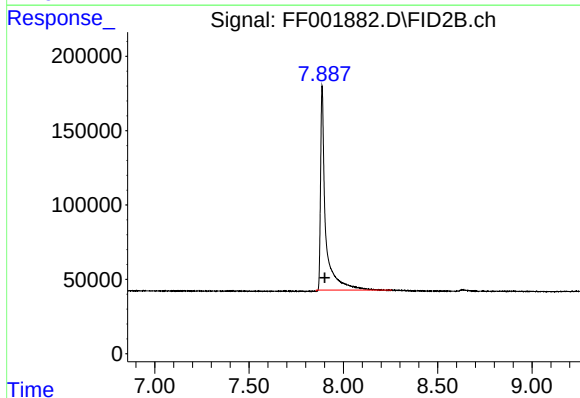


#4 N-TETRADECANE

R.T.: 7.887 min
Delta R.T.: -0.014 min
Response: 2553628
Conc: 16.94 ug/ml

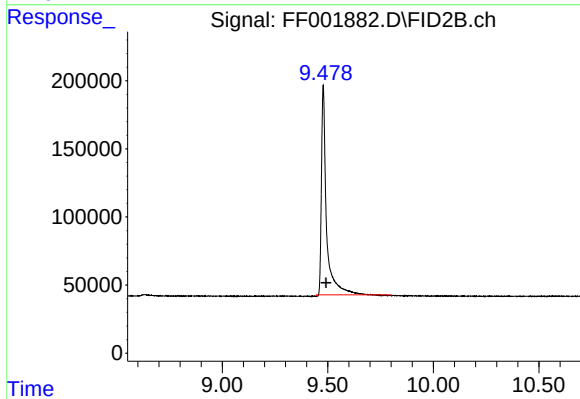

#5 N-HEXADECANE


R.T.: 9.478 min
Delta R.T.: -0.014 min
Response: 2569439
Conc: 17.16 ug/ml

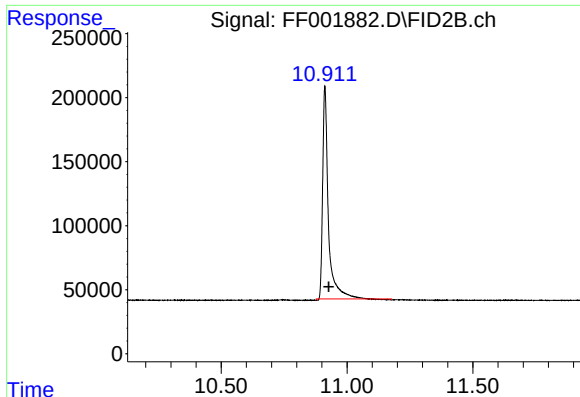

#6 N-OCTADECANE


R.T.: 10.912 min
Delta R.T.: -0.015 min
Response: 2627569
Conc: 17.43 ug/ml

Instrument :
FID_F
ClientSampleId :

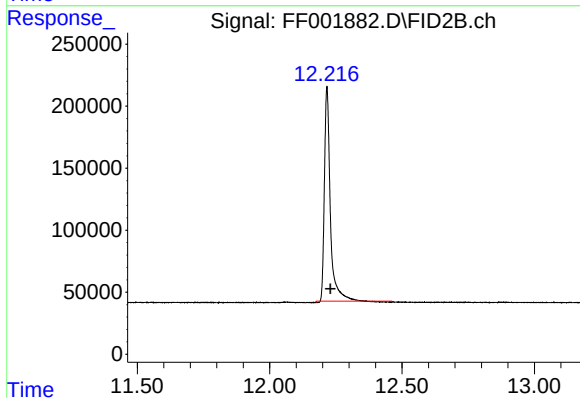


#7 N-EICOSANE

R.T.: 12.216 min
Delta R.T.: -0.013 min
Response: 2667325
Conc: 17.90 ug/ml

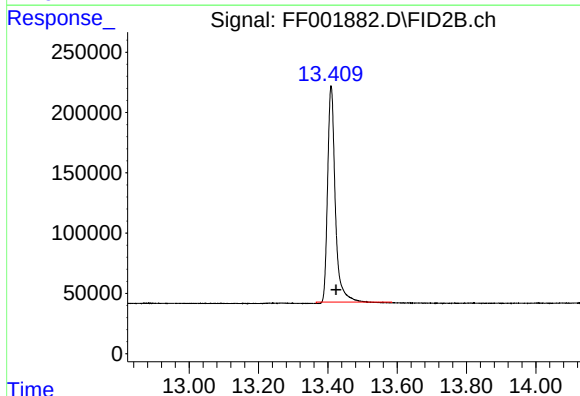


#8 N-DOCOSANE

R.T.: 13.410 min
Delta R.T.: -0.014 min
Response: 2721134
Conc: 18.63 ug/ml

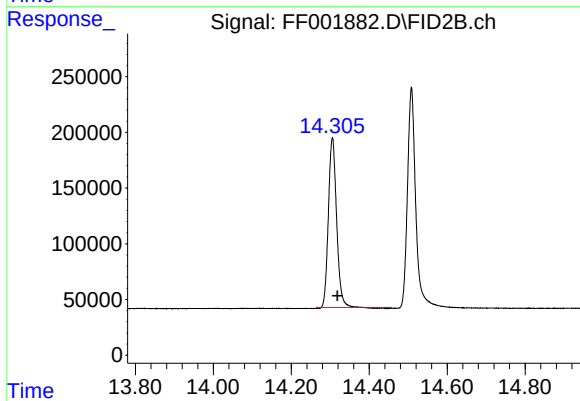

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.306 min
Delta R.T.: -0.013 min
Response: 2202599
Conc: 17.44 ug/ml

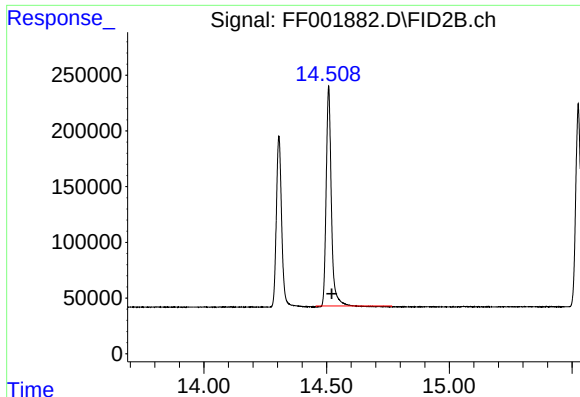

#10 N-TETRACOSANE


R.T.: 14.508 min
Delta R.T.: -0.013 min
Response: 2838392
Conc: 19.90 ug/ml

Instrument :
FID_F
ClientSampleId :

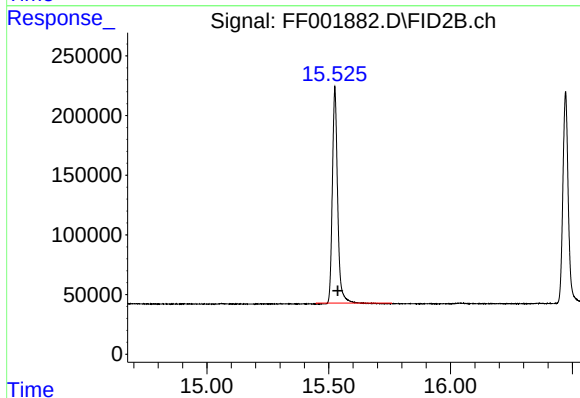

#11 N-HEXACOSANE

R.T.: 15.525 min
Delta R.T.: -0.013 min
Response: 2681282
Conc: 19.03 ug/ml

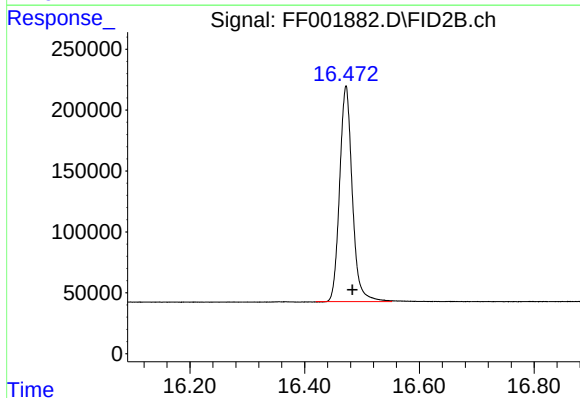

#12 N-OCTACOSANE

R.T.: 16.472 min
Delta R.T.: -0.011 min
Response: 2705432
Conc: 19.29 ug/ml