

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001884.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 15:40
 Operator : AJ\SJ
 Sample : J4524-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:20:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.304	2663671	21.090 ug/ml
Target Compounds			
5) N-HEXADECANE	9.500	60897	0.407 ug/ml
6) N-OCTADECANE	10.919	170475	1.131 ug/ml
7) N-EICOSANE	12.218	206853	1.388 ug/ml
8) N-DOCOSANE	13.411	168795	1.156 ug/ml
10) N-TETRACOSANE	14.508	243498	1.707 ug/ml
11) N-HEXACOSANE	15.527	324208	2.302 ug/ml
12) N-OCTACOSANE	16.471	437366	3.119 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001884.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 15:40
Operator : AJ\SJ
Sample : J4524-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:20:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

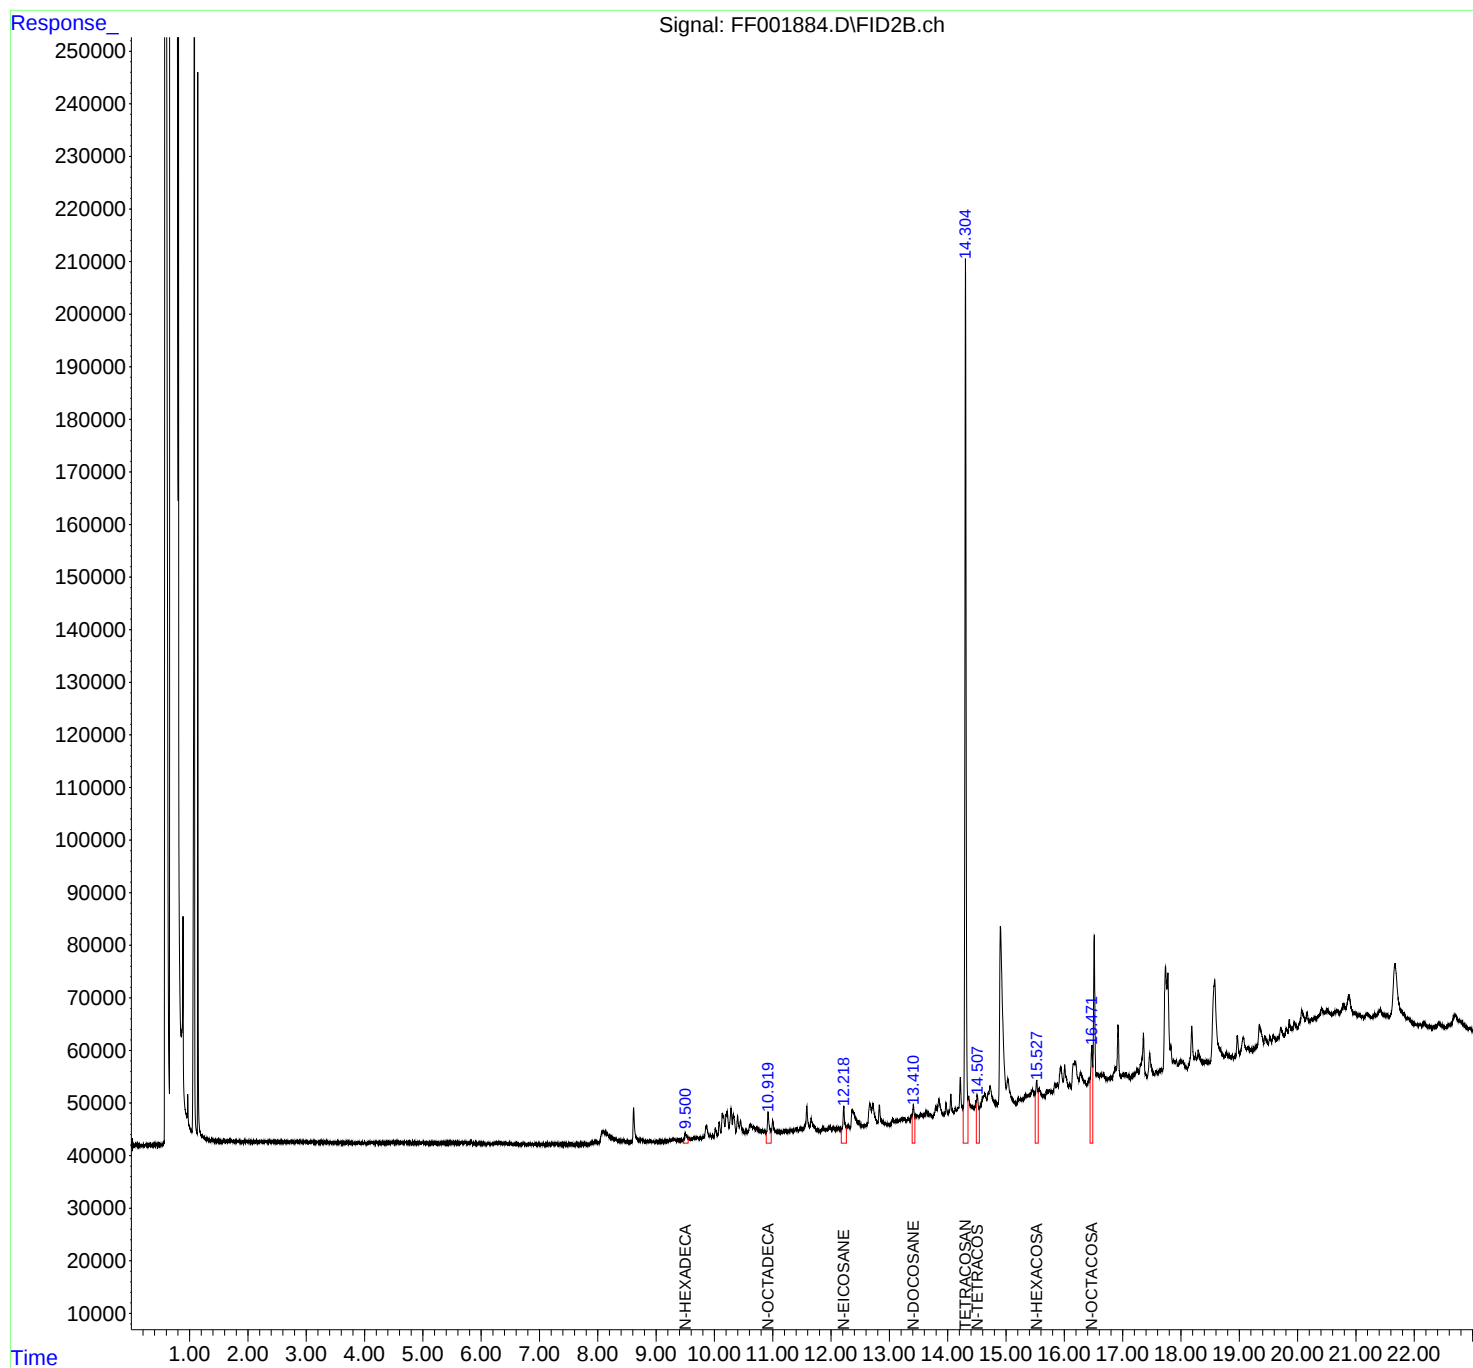


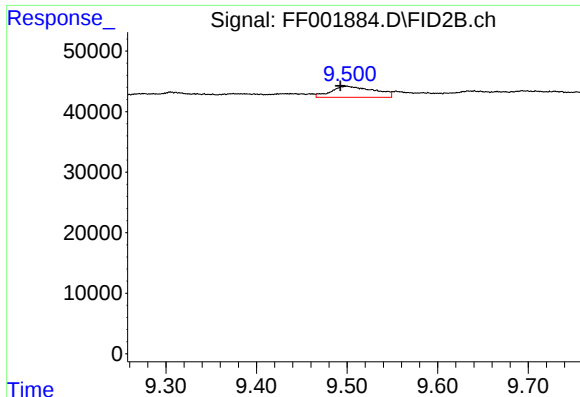

#5 N-HEXADECANE


R.T.: 9.500 min
Delta R.T.: 0.007 min
Response: 60897
Conc: 0.41 ug/ml

Instrument :
FID_F
ClientSampleId :

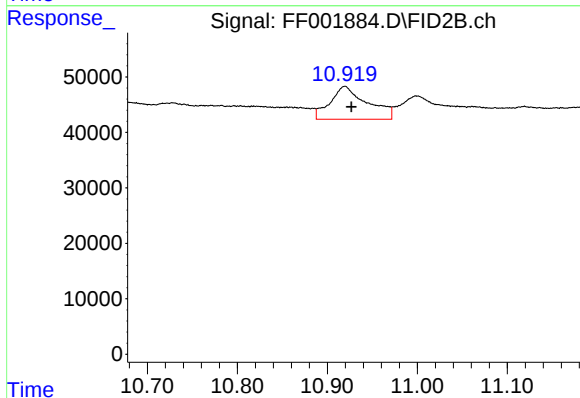


#6 N-OCTADECANE

R.T.: 10.919 min
Delta R.T.: -0.007 min
Response: 170475
Conc: 1.13 ug/ml

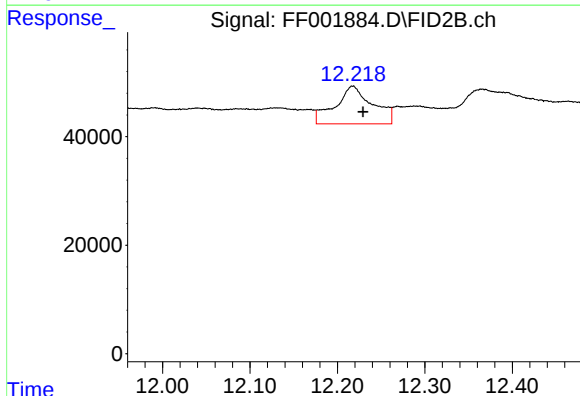


#7 N-EICOSANE

R.T.: 12.218 min
Delta R.T.: -0.012 min
Response: 206853
Conc: 1.39 ug/ml

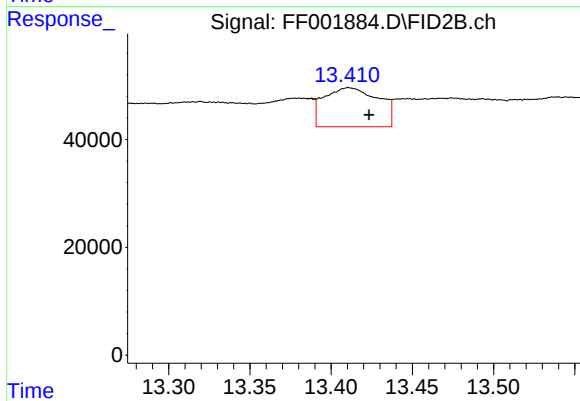

#8 N-DOCOSANE


R.T.: 13.411 min
Delta R.T.: -0.013 min
Response: 168795
Conc: 1.16 ug/ml

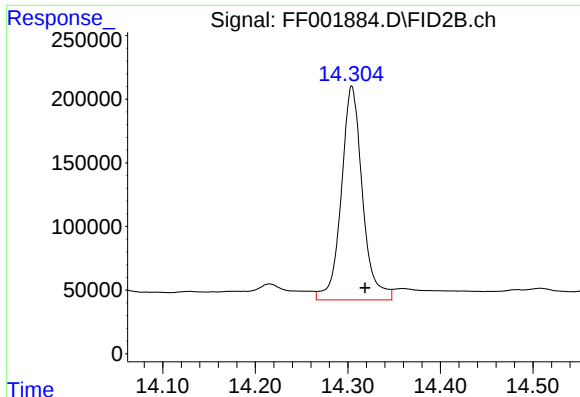

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.304 min
Delta R.T.: -0.014 min
Response: 2663671
Conc: 21.09 ug/ml

Instrument :
FID_F
ClientSampleId :

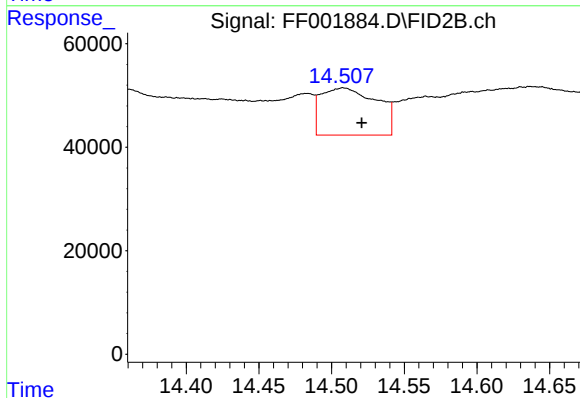


#10 N-TETRACOSANE

R.T.: 14.508 min
Delta R.T.: -0.013 min
Response: 243498
Conc: 1.71 ug/ml

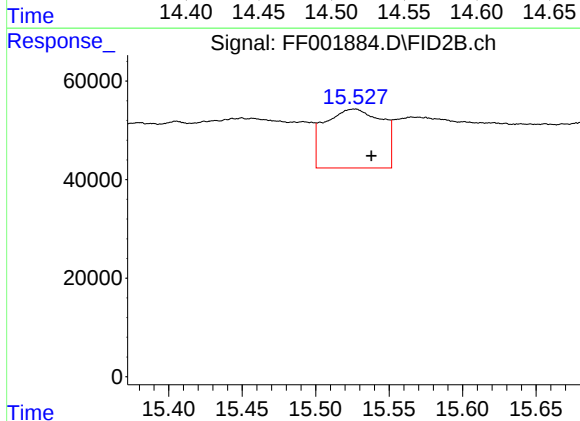

#11 N-HEXACOSANE

R.T.: 15.527 min
Delta R.T.: -0.011 min
Response: 324208
Conc: 2.30 ug/ml

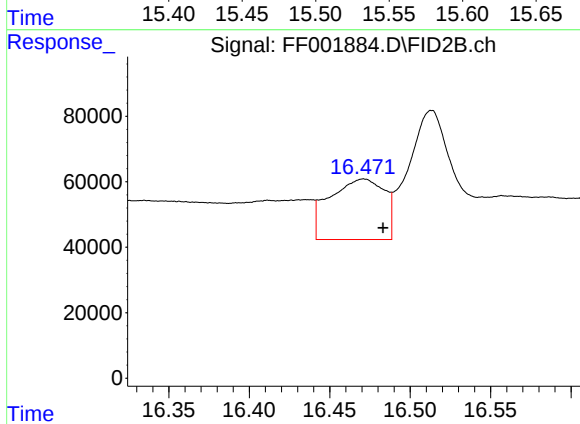

#12 N-OCTACOSANE

R.T.: 16.471 min
Delta R.T.: -0.012 min
Response: 437366
Conc: 3.12 ug/ml