

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001885.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 16:11
 Operator : AJ\SJ
 Sample : J4483-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:21:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.304	2299298	18.205 ug/ml
Target Compounds			
2) N-DECANE	4.114	4164	0.029 ug/ml
4) N-TETRADECANE	7.918	3033	0.020 ug/ml
5) N-HEXADECANE	9.494	4745	0.032 ug/ml
6) N-OCTADECANE	10.917	28526	0.189 ug/ml
7) N-EICOSANE	12.218	79269	0.532 ug/ml
8) N-DOCOSANE	13.410	77917	0.533 ug/ml
10) N-TETRACOSANE	14.507	115966	0.813 ug/ml
11) N-HEXACOSANE	15.524	203786	1.447 ug/ml
12) N-OCTACOSANE	16.470	273834	1.953 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001885.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 16:11
Operator : AJ\SJ
Sample : J4483-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:21:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

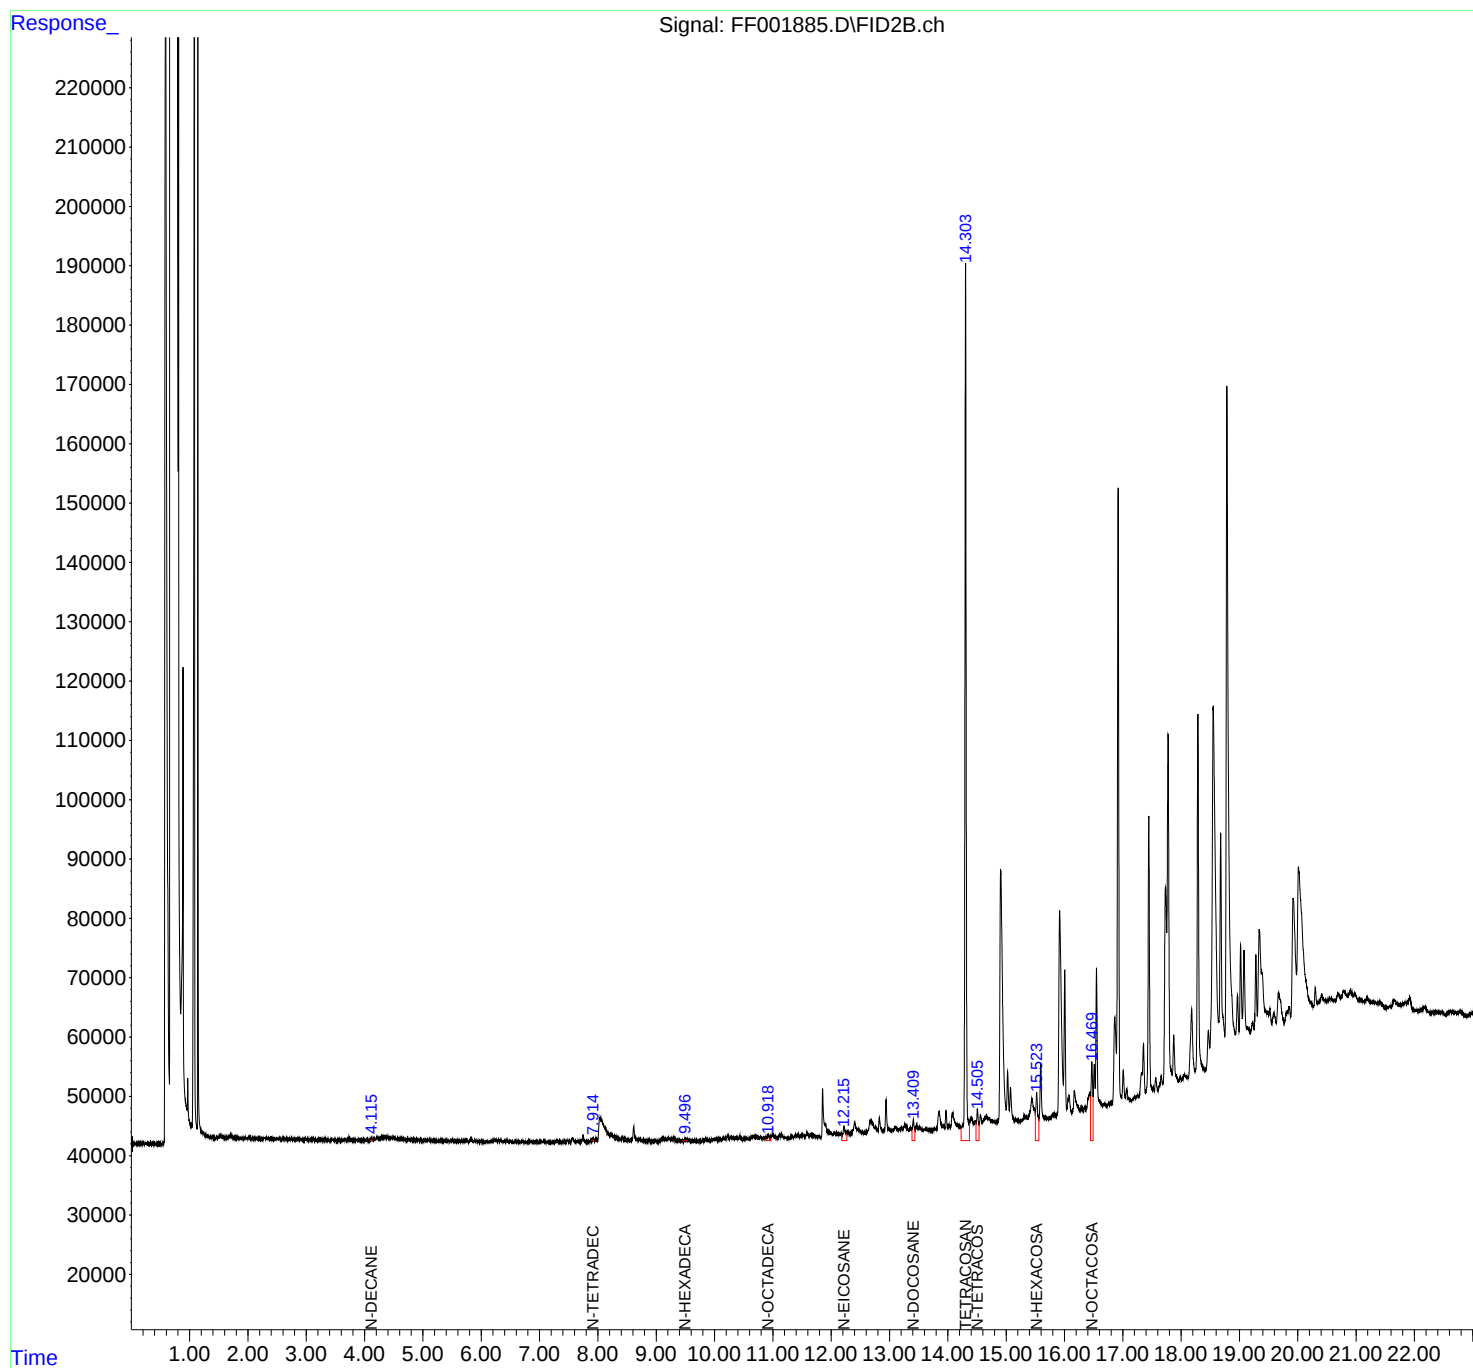


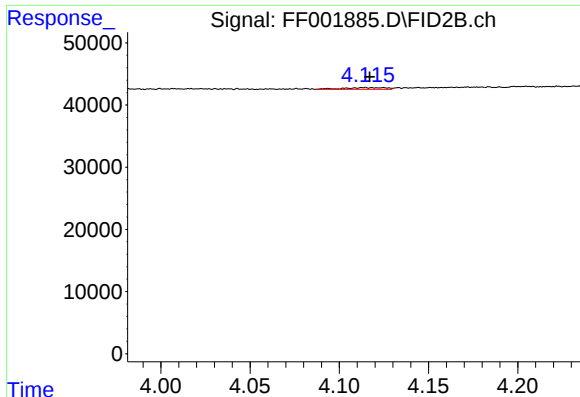

#2 N-DECANE


R.T.: 4.114 min
Delta R.T.: -0.003 min
Response: 4164
Conc: 0.03 ug/ml

Instrument :
FID_F
ClientSampleId :

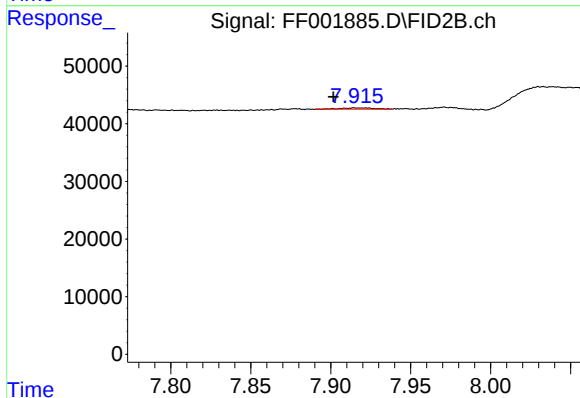


#4 N-TETRADECANE

R.T.: 7.918 min
Delta R.T.: 0.016 min
Response: 3033
Conc: 0.02 ug/ml

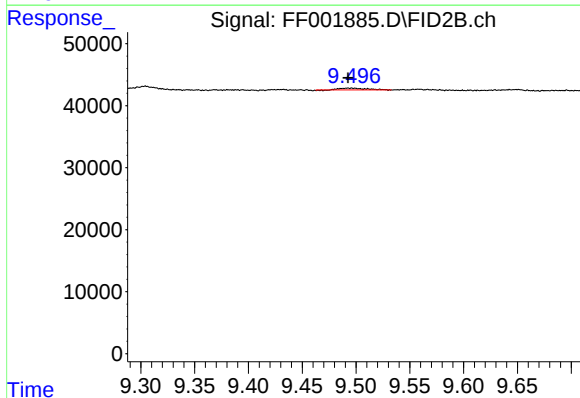


#5 N-HEXADECANE

R.T.: 9.494 min
Delta R.T.: 0.000 min
Response: 4745
Conc: 0.03 ug/ml

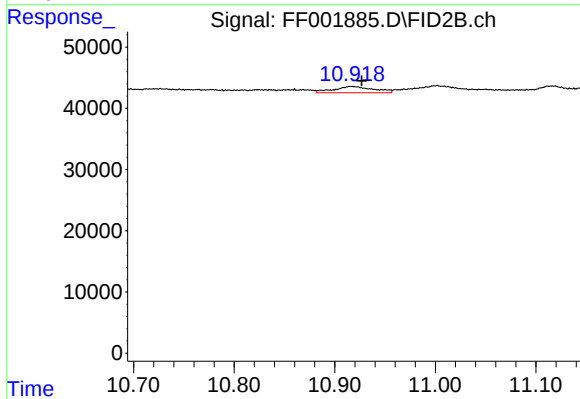

#6 N-OCTADECANE


R.T.: 10.917 min
Delta R.T.: -0.010 min
Response: 28526
Conc: 0.19 ug/ml

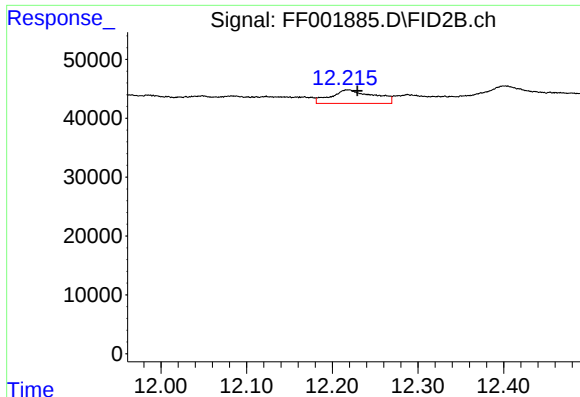

#7 N-EICOSANE


R.T.: 12.218 min
Delta R.T.: -0.011 min
Response: 79269
Conc: 0.53 ug/ml

Instrument :
FID_F
ClientSampleId :

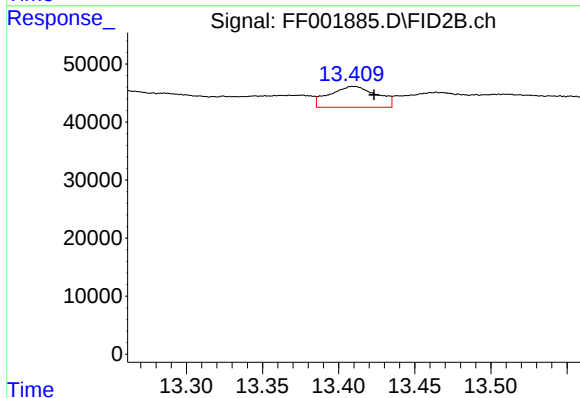


#8 N-DOCOSANE

R.T.: 13.410 min
Delta R.T.: -0.013 min
Response: 77917
Conc: 0.53 ug/ml

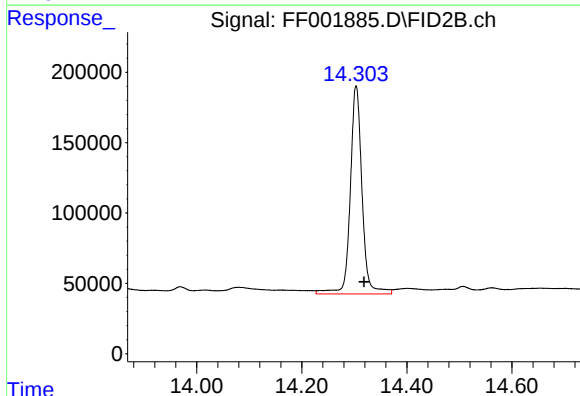


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.304 min
Delta R.T.: -0.015 min
Response: 2299298
Conc: 18.20 ug/ml

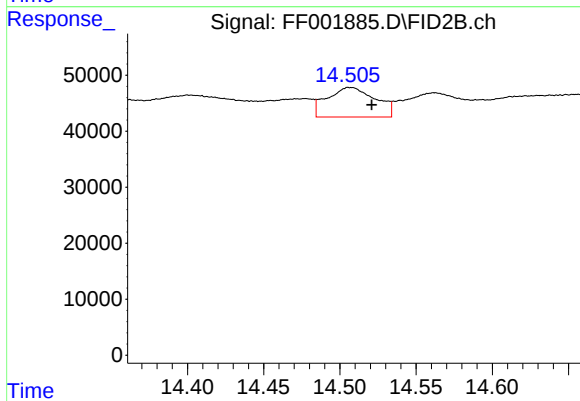

#10 N-TETRACOSANE


R.T.: 14.507 min
Delta R.T.: -0.014 min
Response: 115966
Conc: 0.81 ug/ml

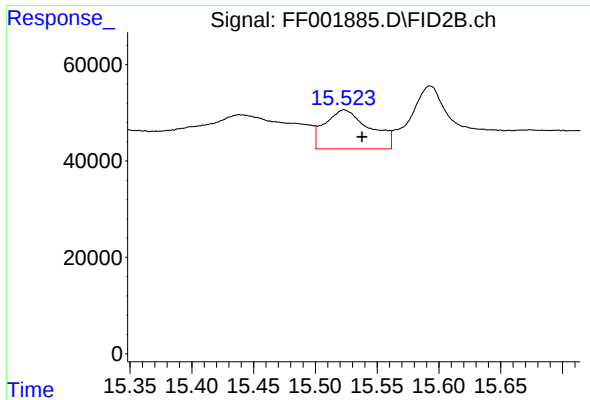

#11 N-HEXACOSANE

R.T.: 15.524 min
Delta R.T.: -0.014 min
Response: 203786
Conc: 1.45 ug/ml

Instrument :
FID_F
ClientSampleId :

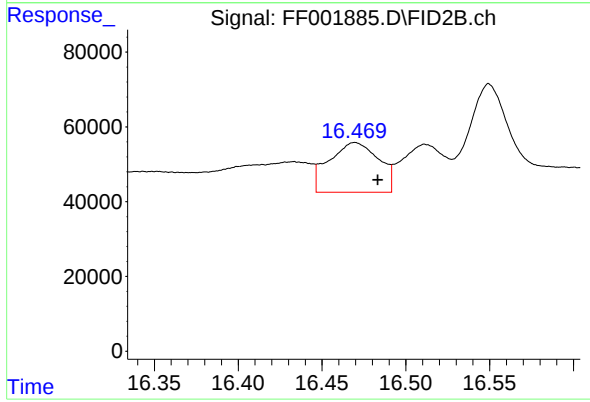

#12 N-OCTACOSANE

R.T.: 16.470 min
Delta R.T.: -0.013 min
Response: 273834
Conc: 1.95 ug/ml