

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001886.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 16:41
 Operator : AJ\SJ
 Sample : J4483-02MS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:21:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.303	3333106	26.390 ug/ml
Target Compounds			
2) N-DECANE	4.095	1840000	12.617 ug/ml
3) N-DODECANE	6.101	2173714	14.583 ug/ml
4) N-TETRADECANE	7.884	2557589	16.969 ug/ml
5) N-HEXADECANE	9.475	2731183	18.244 ug/ml
6) N-OCTADECANE	10.910	2864120	19.002 ug/ml
7) N-EICOSANE	12.214	2990101	20.062 ug/ml
8) N-DOCOSANE	13.406	3139933	21.496 ug/ml
10) N-TETRACOSANE	14.505	3353158	23.506 ug/ml
11) N-HEXACOSANE	15.523	3143800	22.318 ug/ml
12) N-OCTACOSANE	16.470	3322689	23.697 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001886.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 16:41
Operator : AJ\SJ
Sample : J4483-02MS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:21:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

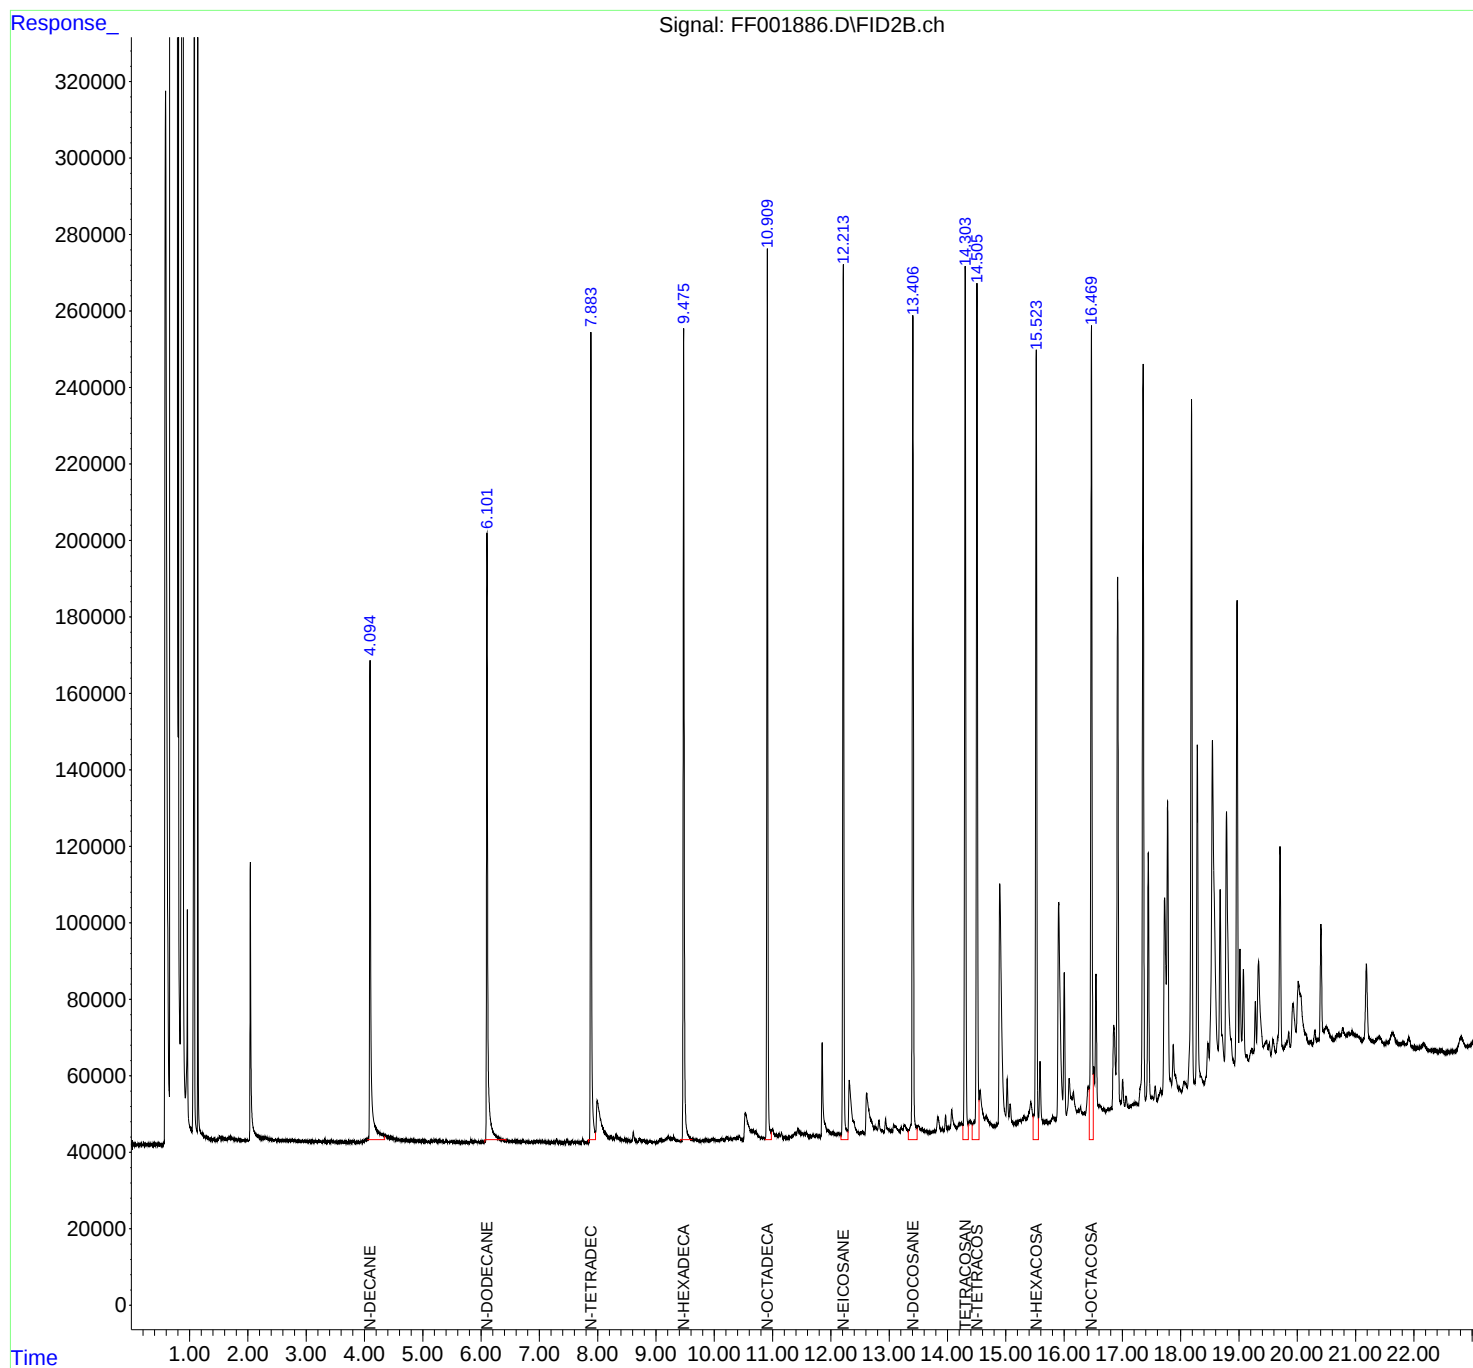


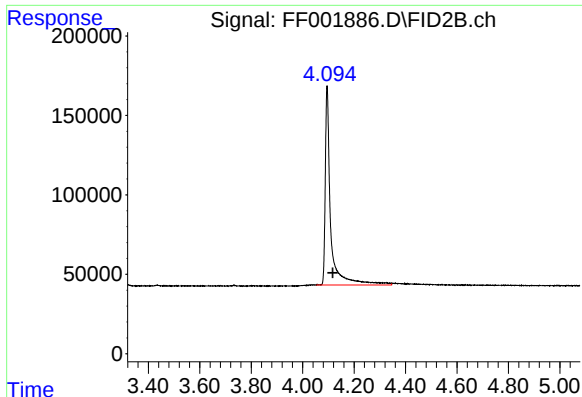

#2 N-DECANE


R.T.: 4.095 min
Delta R.T.: -0.022 min
Response: 184000
Conc: 12.62 ug/ml

Instrument :
FID_F
ClientSampleId :

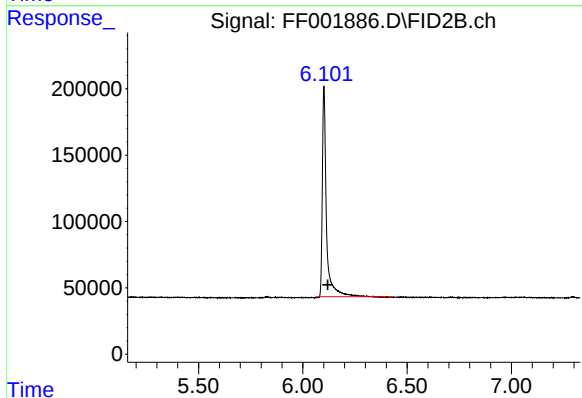


#3 N-DODECANE

R.T.: 6.101 min
Delta R.T.: -0.018 min
Response: 2173714
Conc: 14.58 ug/ml

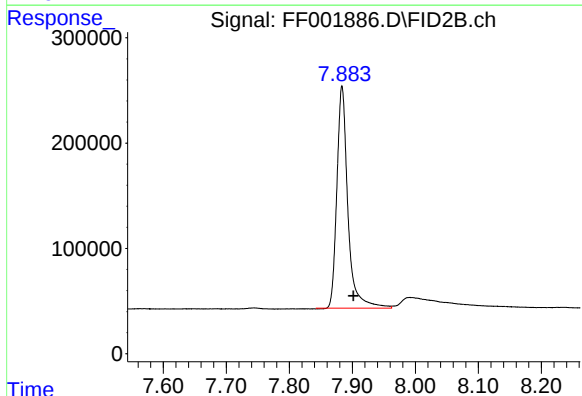


#4 N-TETRADECANE

R.T.: 7.884 min
Delta R.T.: -0.018 min
Response: 2557589
Conc: 16.97 ug/ml

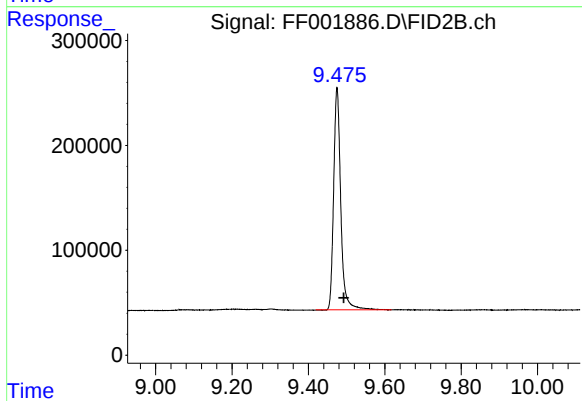

#5 N-HEXADECANE


R.T.: 9.475 min
Delta R.T.: -0.018 min
Response: 2731183
Conc: 18.24 ug/ml

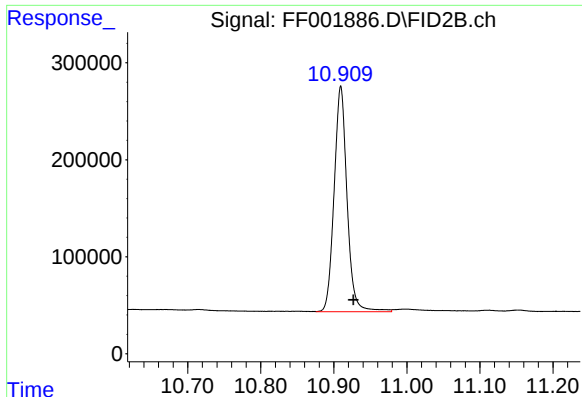

#6 N-OCTADECANE


R.T.: 10.910 min
Delta R.T.: -0.017 min
Response: 2864120
Conc: 19.00 ug/ml

Instrument :
FID_F
ClientSampleId :

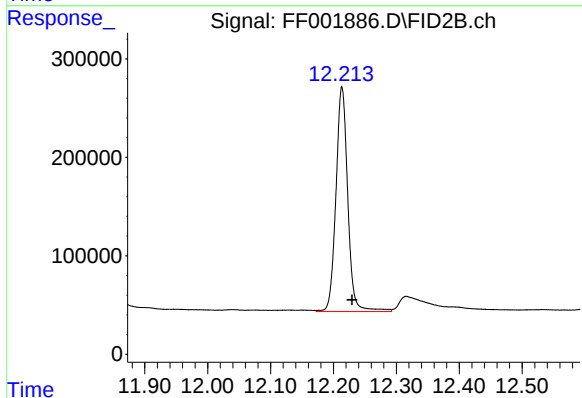


#7 N-EICOSANE

R.T.: 12.214 min
Delta R.T.: -0.016 min
Response: 2990101
Conc: 20.06 ug/ml

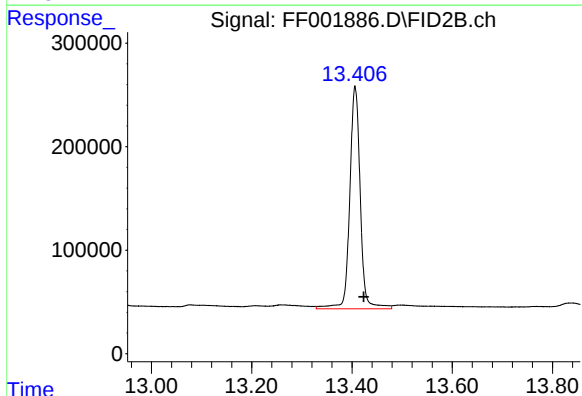


#8 N-DOCOSANE

R.T.: 13.406 min
Delta R.T.: -0.017 min
Response: 3139933
Conc: 21.50 ug/ml

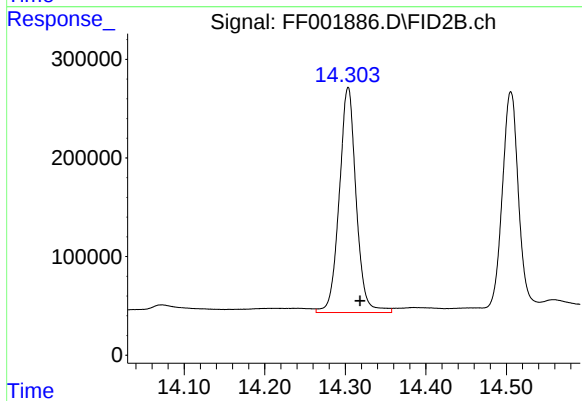

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.303 min
Delta R.T.: -0.015 min
Response: 3333106
Conc: 26.39 ug/ml

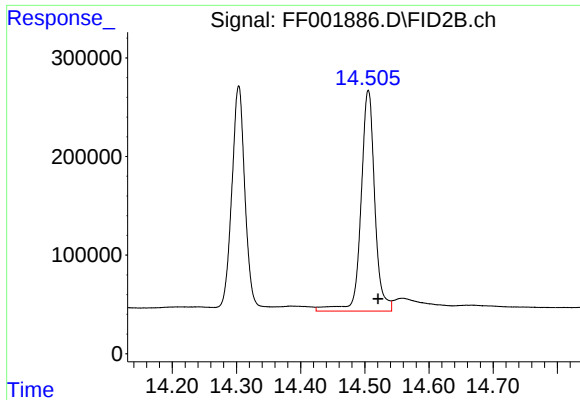

#10 N-TETRACOSANE


R.T.: 14.505 min
Delta R.T.: -0.015 min
Response: 3353158
Conc: 23.51 ug/ml

Instrument :
FID_F
ClientSampleId :

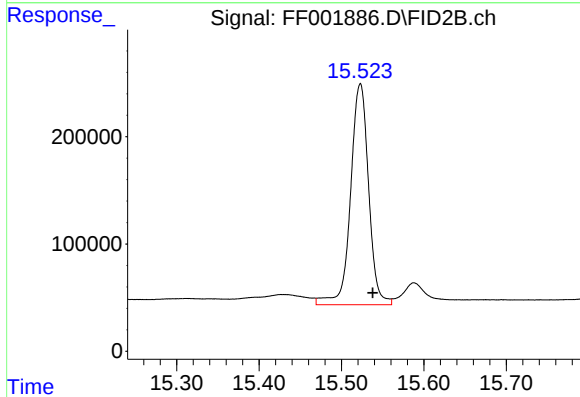

#11 N-HEXACOSANE

R.T.: 15.523 min
Delta R.T.: -0.015 min
Response: 3143800
Conc: 22.32 ug/ml

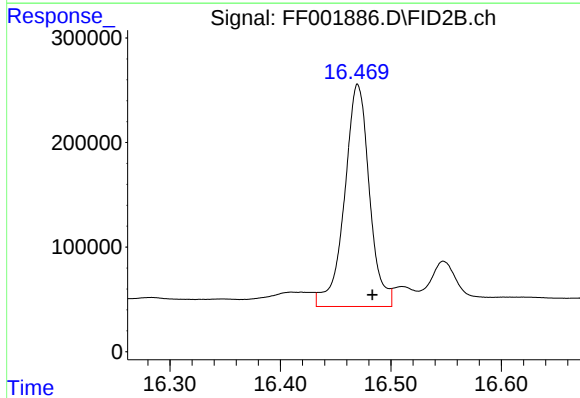

#12 N-OCTACOSANE

R.T.: 16.470 min
Delta R.T.: -0.013 min
Response: 3322689
Conc: 23.70 ug/ml