

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001887.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 17:12
 Operator : AJ\SJ
 Sample : J4483-02MSD
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:21:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.304	3450911	27.323 ug/ml
Target Compounds			
2) N-DECANE	4.094	1894408	12.990 ug/ml
3) N-DODECANE	6.100	2217611	14.877 ug/ml
4) N-TETRADECANE	7.883	2674563	17.745 ug/ml
5) N-HEXADECANE	9.475	2843552	18.994 ug/ml
6) N-OCTADECANE	10.909	2993044	19.858 ug/ml
7) N-EICOSANE	12.214	3113277	20.888 ug/ml
8) N-DOCOSANE	13.407	3272173	22.402 ug/ml
10) N-TETRACOSANE	14.507	3476881	24.373 ug/ml
11) N-HEXACOSANE	15.524	3270125	23.215 ug/ml
12) N-OCTACOSANE	16.471	3770476	26.890 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001887.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 17:12
Operator : AJ\SJ
Sample : J4483-02MSD
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:21:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

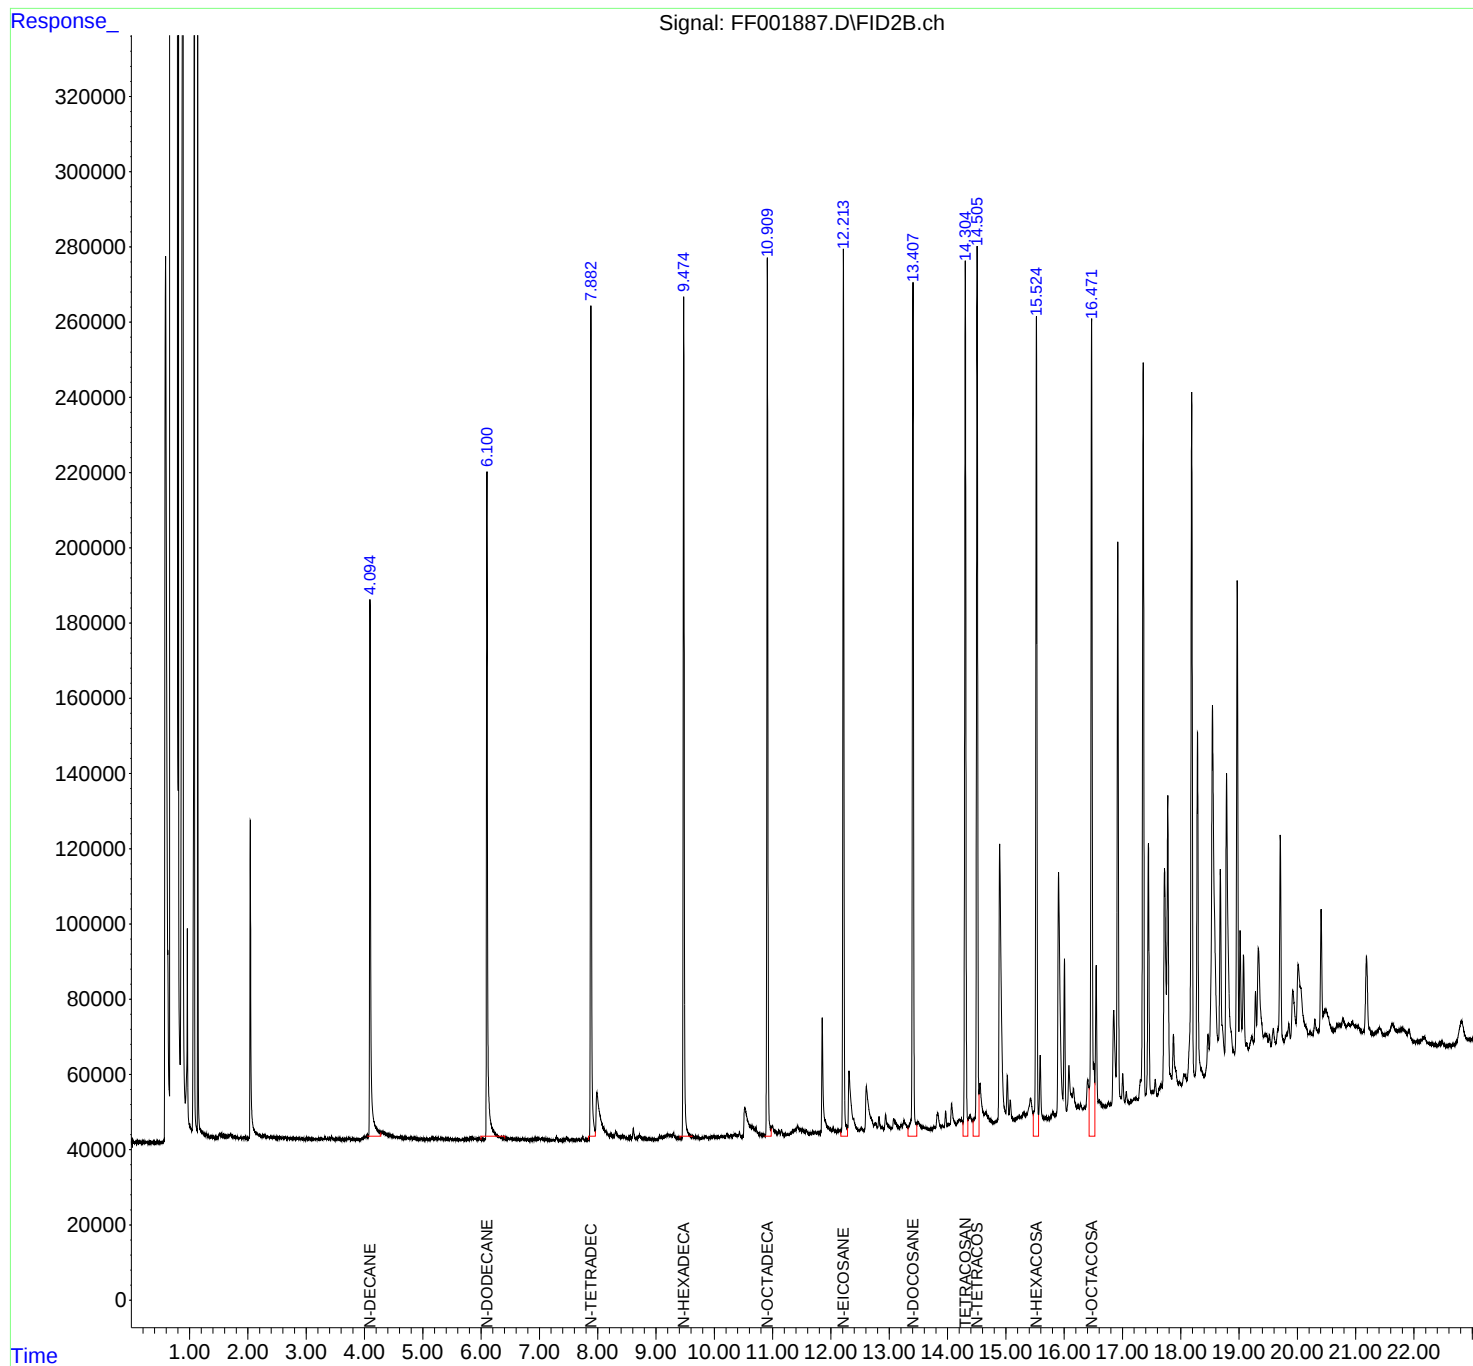


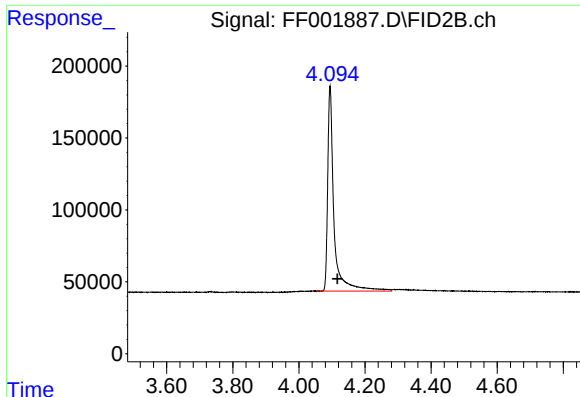

#2 N-DECANE


R.T.: 4.094 min
Delta R.T.: -0.023 min
Response: 1894408
Conc: 12.99 ug/ml

Instrument :
FID_F
ClientSampleId :

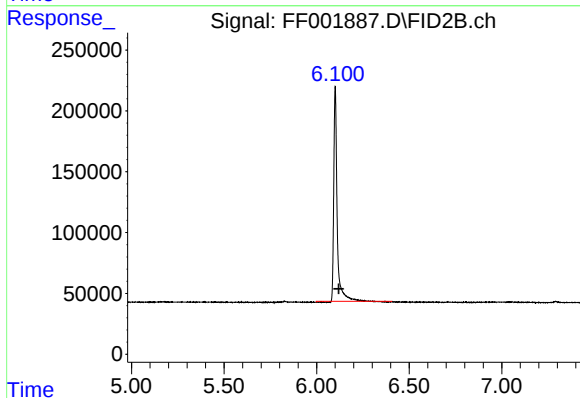


#3 N-DODECANE

R.T.: 6.100 min
Delta R.T.: -0.019 min
Response: 2217611
Conc: 14.88 ug/ml

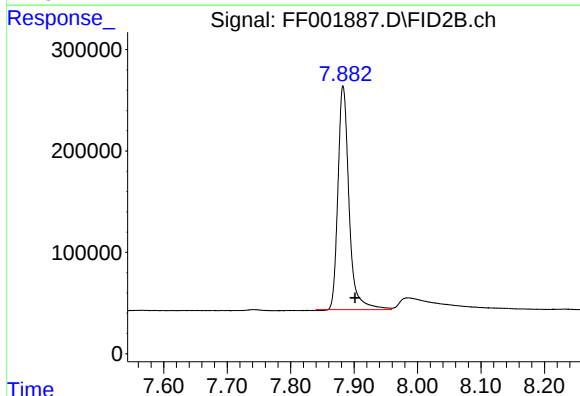


#4 N-TETRADECANE

R.T.: 7.883 min
Delta R.T.: -0.019 min
Response: 2674563
Conc: 17.75 ug/ml

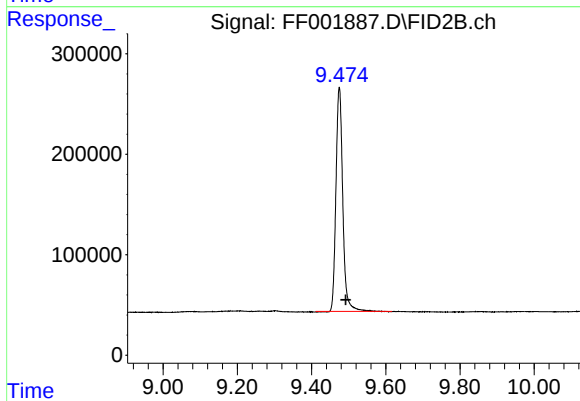

#5 N-HEXADECANE


R.T.: 9.475 min
Delta R.T.: -0.018 min
Response: 2843552
Conc: 18.99 ug/ml

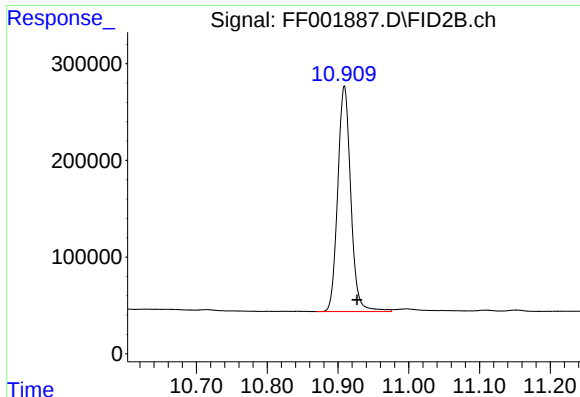

#6 N-OCTADECANE


R.T.: 10.909 min
Delta R.T.: -0.018 min
Response: 2993044
Conc: 19.86 ug/ml

Instrument :
FID_F
ClientSampleId :

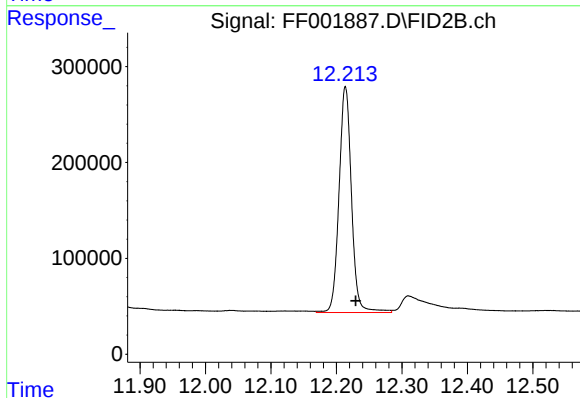


#7 N-EICOSANE

R.T.: 12.214 min
Delta R.T.: -0.016 min
Response: 3113277
Conc: 20.89 ug/ml

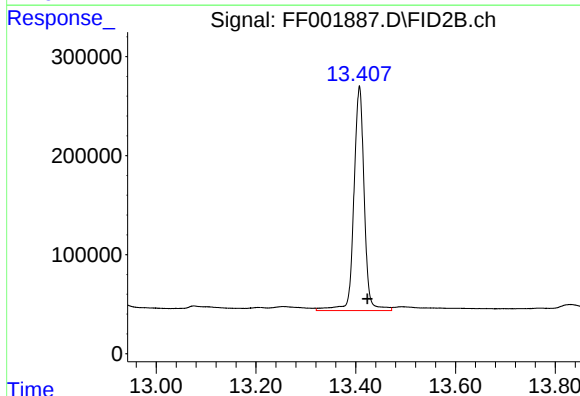


#8 N-DOCOSANE

R.T.: 13.407 min
Delta R.T.: -0.016 min
Response: 3272173
Conc: 22.40 ug/ml

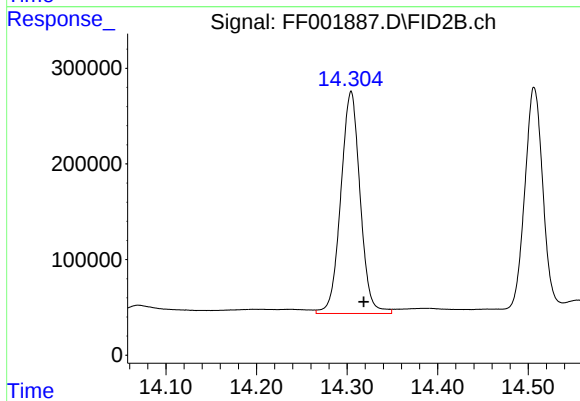

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.304 min
Delta R.T.: -0.014 min
Response: 3450911
Conc: 27.32 ug/ml

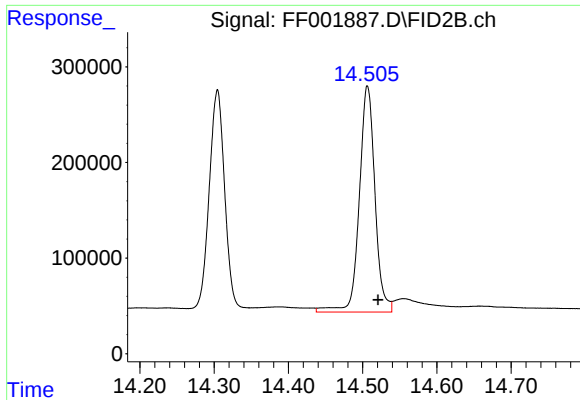

#10 N-TETRACOSANE


R.T.: 14.507 min
Delta R.T.: -0.014 min
Response: 3476881
Conc: 24.37 ug/ml

Instrument :
FID_F
ClientSampleId :

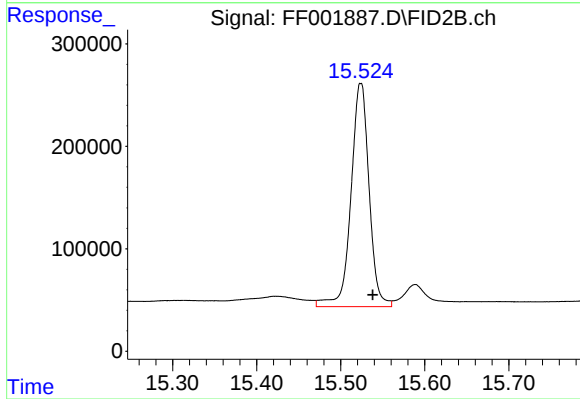

#11 N-HEXACOSANE

R.T.: 15.524 min
Delta R.T.: -0.014 min
Response: 3270125
Conc: 23.21 ug/ml

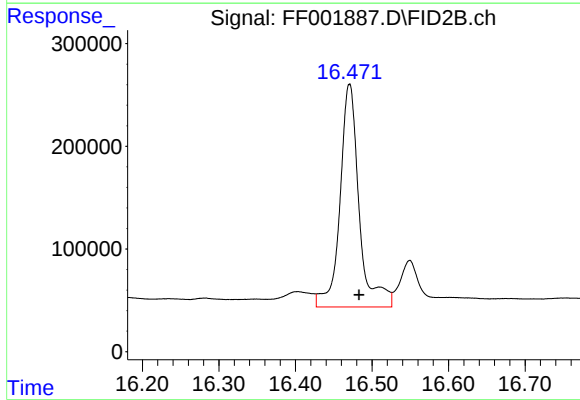

#12 N-OCTACOSANE

R.T.: 16.471 min
Delta R.T.: -0.013 min
Response: 3770476
Conc: 26.89 ug/ml