

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001888.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 17:43
 Operator : AJ\SJ
 Sample : J4509-02
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:21:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.303	2421477	19.172 ug/ml
Target Compounds			
2) N-DECANE	4.114	9686	0.066 ug/ml
7) N-EICOSANE	12.214	8961	0.060 ug/ml
8) N-DOCOSANE	13.406	17531	0.120 ug/ml
10) N-TETRACOSANE	14.506	46424	0.325 ug/ml
11) N-HEXACOSANE	15.523	110234	0.783 ug/ml
12) N-OCTACOSANE	16.469	163757	1.168 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001888.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 17:43
Operator : AJ\SJ
Sample : J4509-02
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:21:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

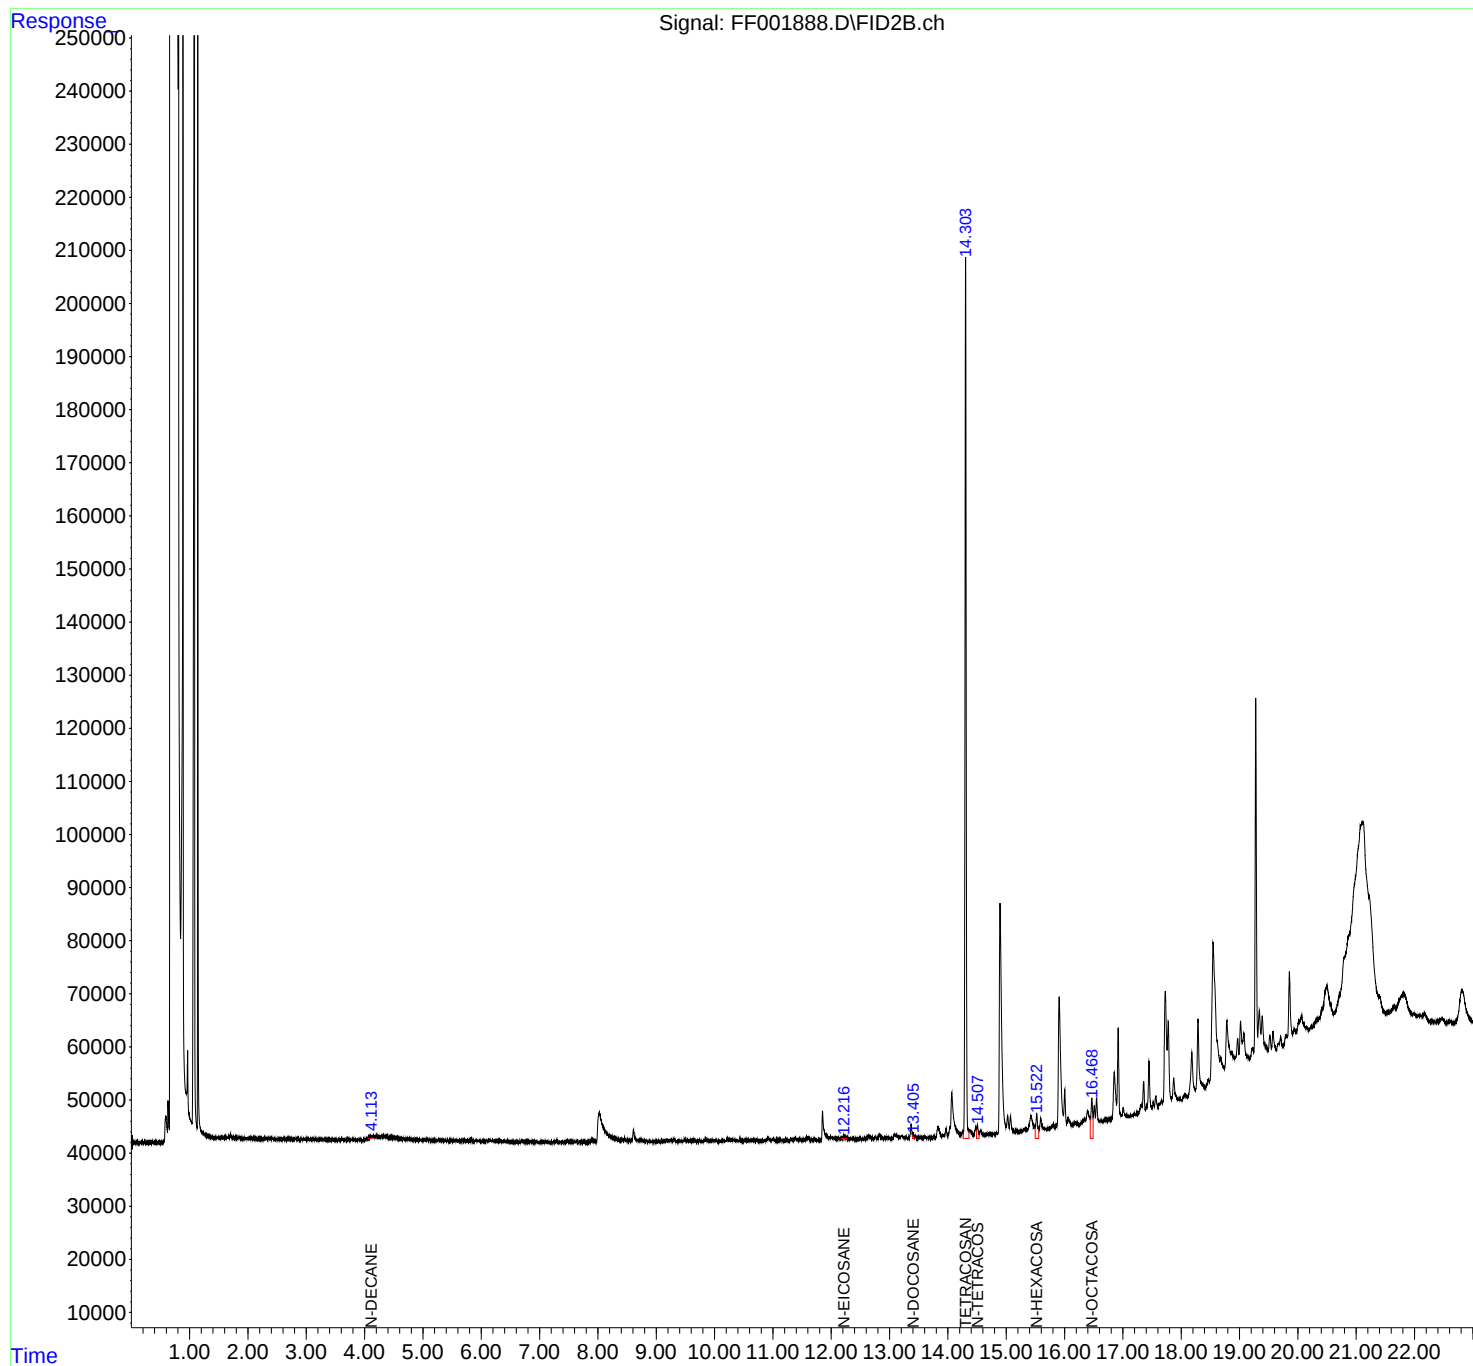


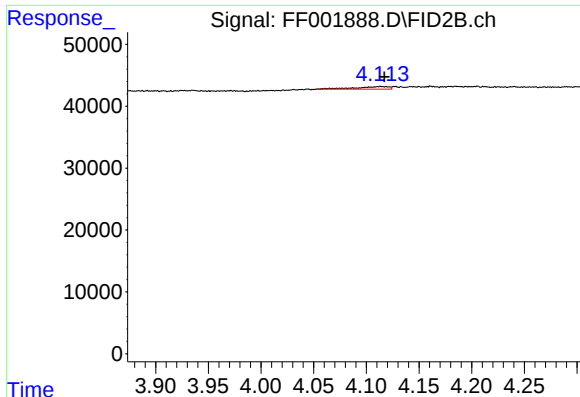

#2 N-DECANE


R.T.: 4.114 min
Delta R.T.: -0.003 min
Response: 9686
Conc: 0.07 ug/ml

Instrument :
FID_F
ClientSampleId :

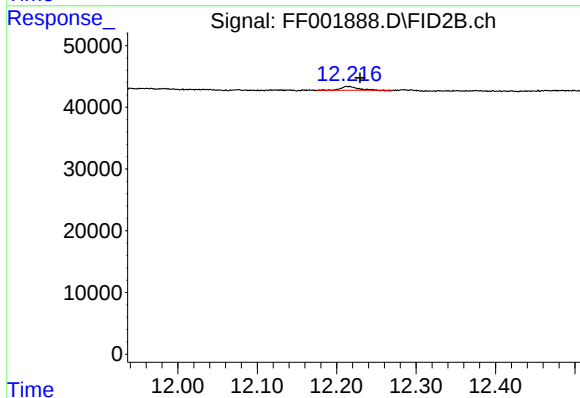


#7 N-EICOSANE

R.T.: 12.214 min
Delta R.T.: -0.015 min
Response: 8961
Conc: 0.06 ug/ml

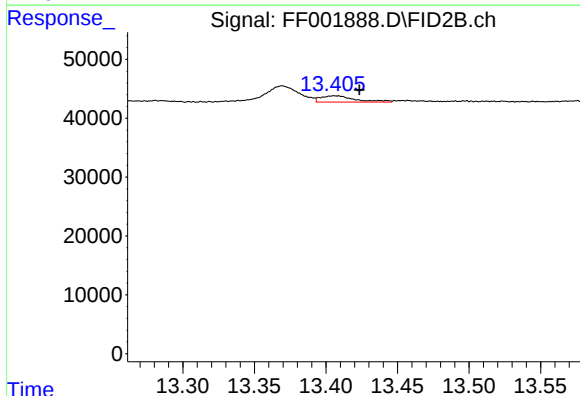


#8 N-DOCOSANE

R.T.: 13.406 min
Delta R.T.: -0.017 min
Response: 17531
Conc: 0.12 ug/ml

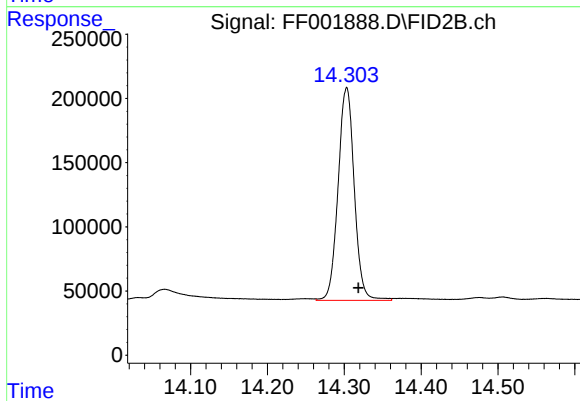

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.303 min
Delta R.T.: -0.015 min
Response: 2421477
Conc: 19.17 ug/ml

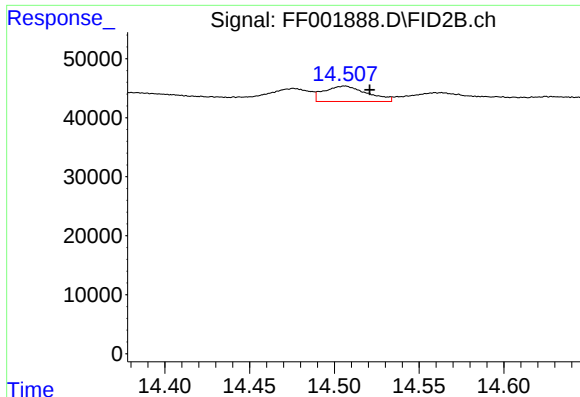

#10 N-TETRACOSANE


R.T.: 14.506 min
Delta R.T.: -0.015 min
Response: 46424
Conc: 0.33 ug/ml

Instrument :
FID_F
ClientSampleId :

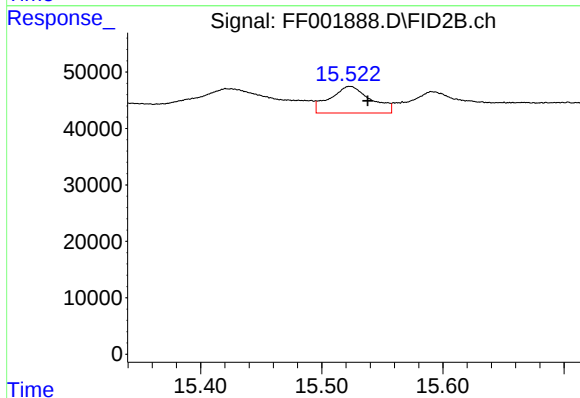

#11 N-HEXACOSANE

R.T.: 15.523 min
Delta R.T.: -0.015 min
Response: 110234
Conc: 0.78 ug/ml

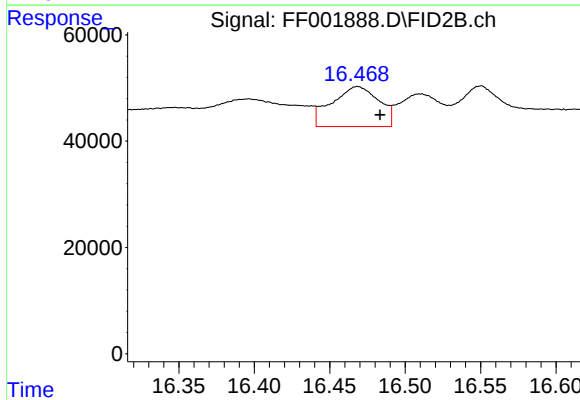

#12 N-OCTACOSANE

R.T.: 16.469 min
Delta R.T.: -0.015 min
Response: 163757
Conc: 1.17 ug/ml