

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
 Data File : FF001889.D
 Signal(s) : FID2B.ch
 Acq On : 20 Aug 2018 19:28
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Aug 21 03:21:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.299	2687340	21.277 ug/ml
Target Compounds			
2) N-DECANE	4.117	24	0.000 ug/ml
3) N-DODECANE	6.093	4054	0.027 ug/ml
4) N-TETRADECANE	7.920	52306	0.347 ug/ml
5) N-HEXADECANE	9.444	13650	0.091 ug/ml
6) N-OCTADECANE	10.868f	18557	0.123 ug/ml
7) N-EICOSANE	12.217	35923	0.241 ug/ml
8) N-DOCOSANE	13.405	28407	0.194 ug/ml
10) N-TETRACOSANE	14.506	51024	0.358 ug/ml
11) N-HEXACOSANE	15.525	46837	0.332 ug/ml
12) N-OCTACOSANE	16.469	260472	1.858 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082018\
Data File : FF001889.D
Signal(s) : FID2B.ch
Acq On : 20 Aug 2018 19:28
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Aug 21 03:21:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

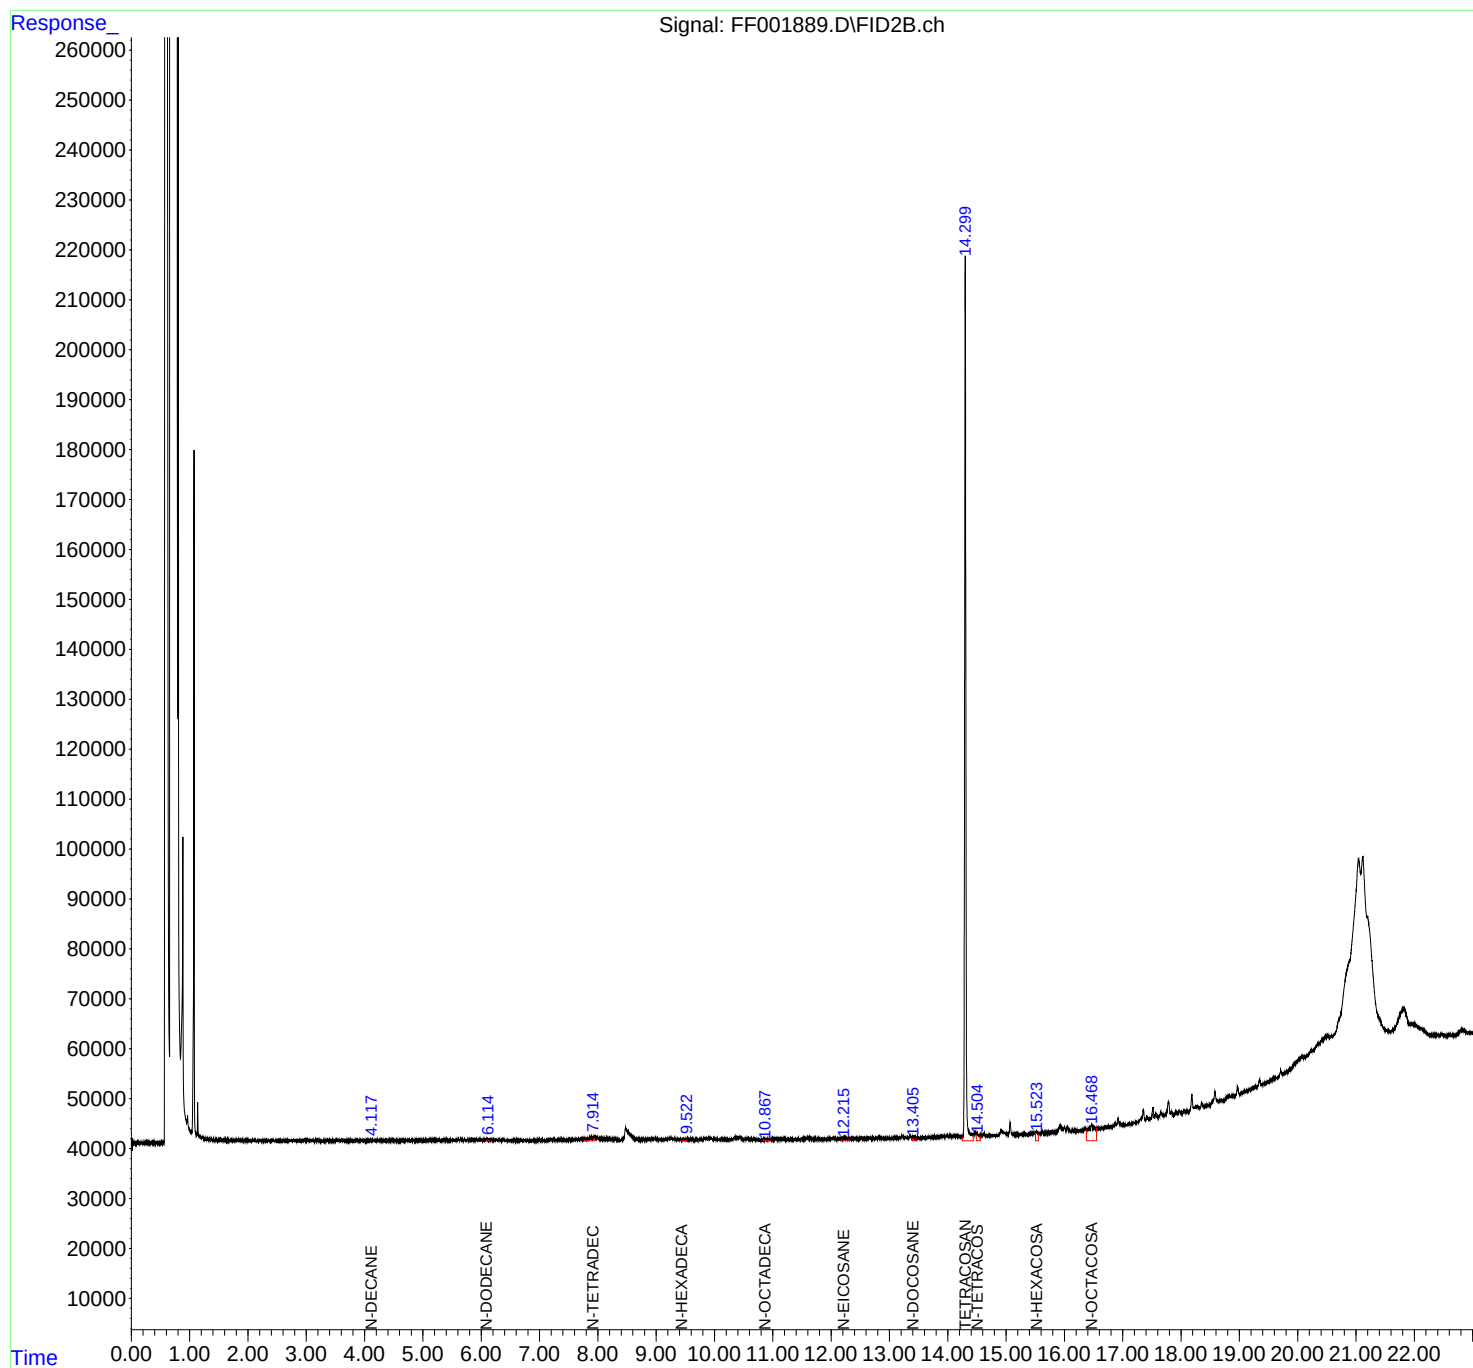


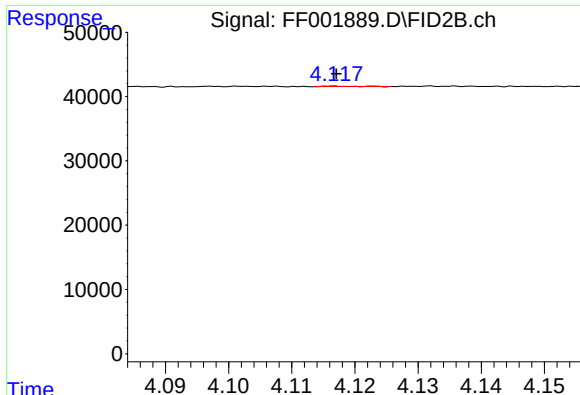

#2 N-DECANE


R.T.: 4.117 min
Delta R.T.: 0.000 min
Response: 24
Conc: 0.00 ug/ml

Instrument :
FID_F
ClientSampleId :

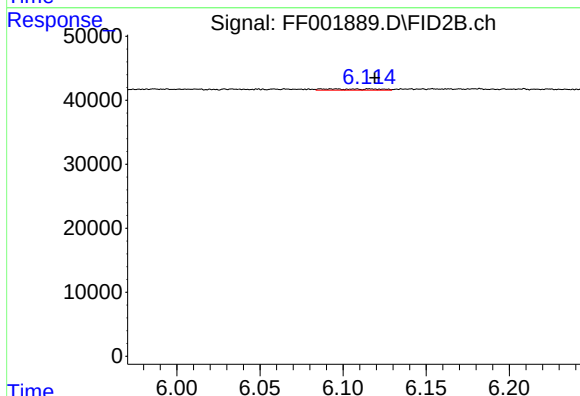


#3 N-DODECANE

R.T.: 6.093 min
Delta R.T.: -0.026 min
Response: 4054
Conc: 0.03 ug/ml

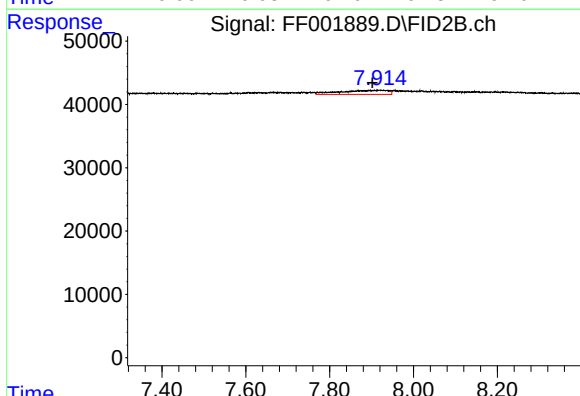


#4 N-TETRADECANE

R.T.: 7.920 min
Delta R.T.: 0.018 min
Response: 52306
Conc: 0.35 ug/ml

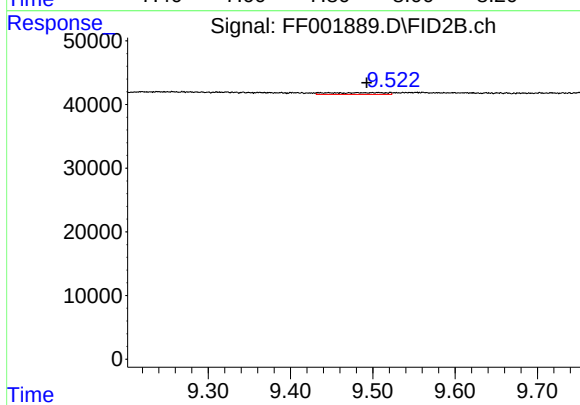

#5 N-HEXADECANE


R.T.: 9.444 min
Delta R.T.: -0.049 min
Response: 13650
Conc: 0.09 ug/ml

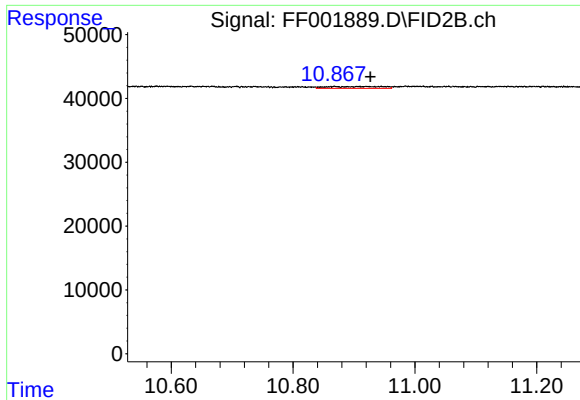

#6 N-OCTADECANE


R.T.: 10.868 min
Delta R.T.: -0.059 min
Response: 18557
Conc: 0.12 ug/ml

Instrument :
FID_F
ClientSampleId :

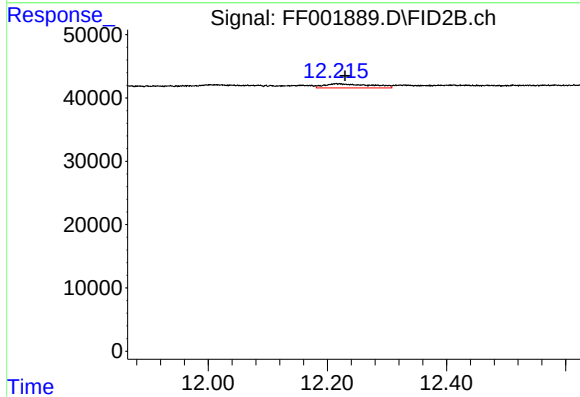


#7 N-EICOSANE

R.T.: 12.217 min
Delta R.T.: -0.013 min
Response: 35923
Conc: 0.24 ug/ml

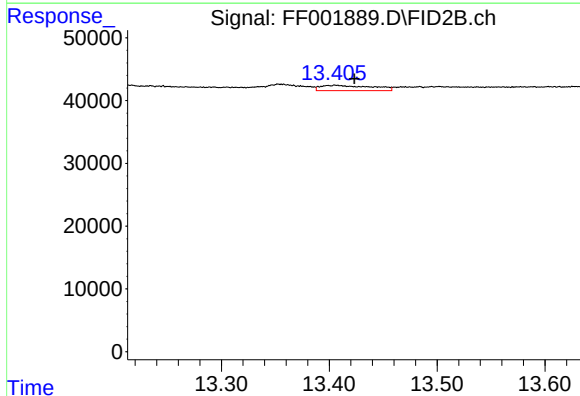


#8 N-DOCOSANE

R.T.: 13.405 min
Delta R.T.: -0.018 min
Response: 28407
Conc: 0.19 ug/ml

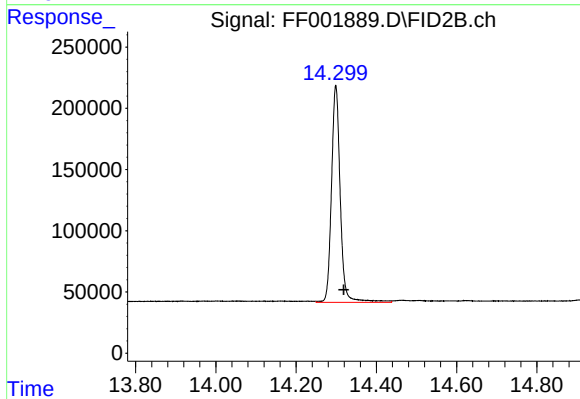

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.299 min
Delta R.T.: -0.019 min
Response: 2687340
Conc: 21.28 ug/ml

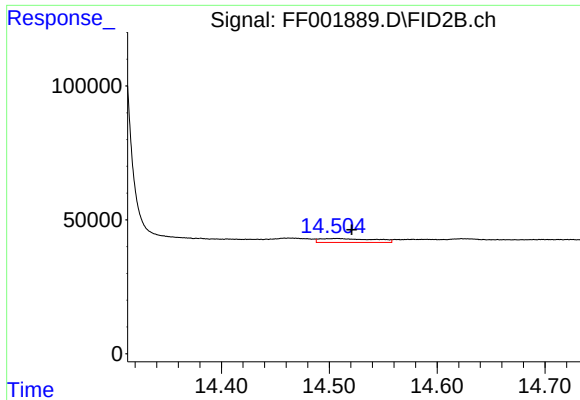

#10 N-TETRACOSANE


R.T.: 14.506 min
Delta R.T.: -0.015 min
Response: 51024
Conc: 0.36 ug/ml

Instrument :
FID_F
ClientSampleId :

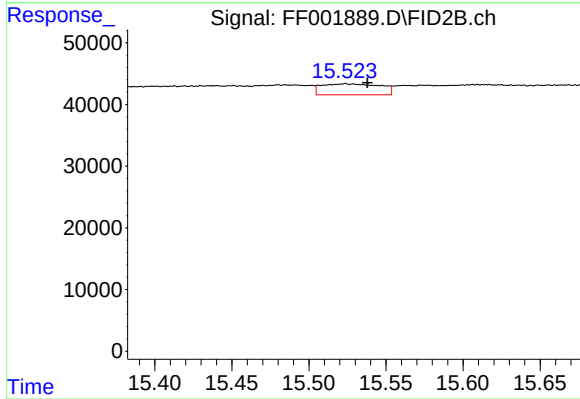

#11 N-HEXACOSANE

R.T.: 15.525 min
Delta R.T.: -0.013 min
Response: 46837
Conc: 0.33 ug/ml

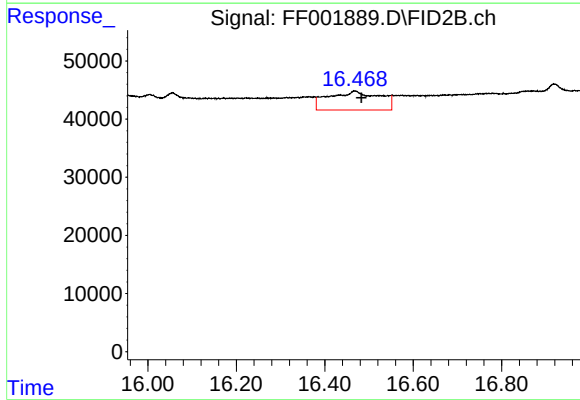

#12 N-OCTACOSANE

R.T.: 16.469 min
Delta R.T.: -0.015 min
Response: 260472
Conc: 1.86 ug/ml