

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
 Data File : FF001895.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2018 14:51
 Operator : AJ\SJ
 Sample : J4573-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 22 01:27:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.302	3778776	29.919 ug/ml
Target Compounds			
4) N-TETRADECANE	7.877	268893	1.784 ug/ml
5) N-HEXADECANE	9.471	201933	1.349 ug/ml
6) N-OCTADECANE	10.905	518696	3.441 ug/ml
7) N-EICOSANE	12.210	1374559	9.222 ug/ml
8) N-DOCOSANE	13.410	1207886	8.269 ug/ml
10) N-TETRACOSANE	14.503	3620960	25.383 ug/ml
11) N-HEXACOSANE	15.521	429371	3.048 ug/ml
12) N-OCTACOSANE	16.517	1083627	7.728 ug/ml
14) N-DOTRIACONTANE	18.179	225694	1.730 ug/ml
15) N-TETRATRIACONTANE	18.963	257672	2.132 ug/ml
16) N-HEXATRIACONTANE	19.699	448414	4.030 ug/ml
18) N-TETRACONTANE	21.264	449063	4.508 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
Data File : FF001895.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2018 14:51
Operator : AJ\SJ
Sample : J4573-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:27:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

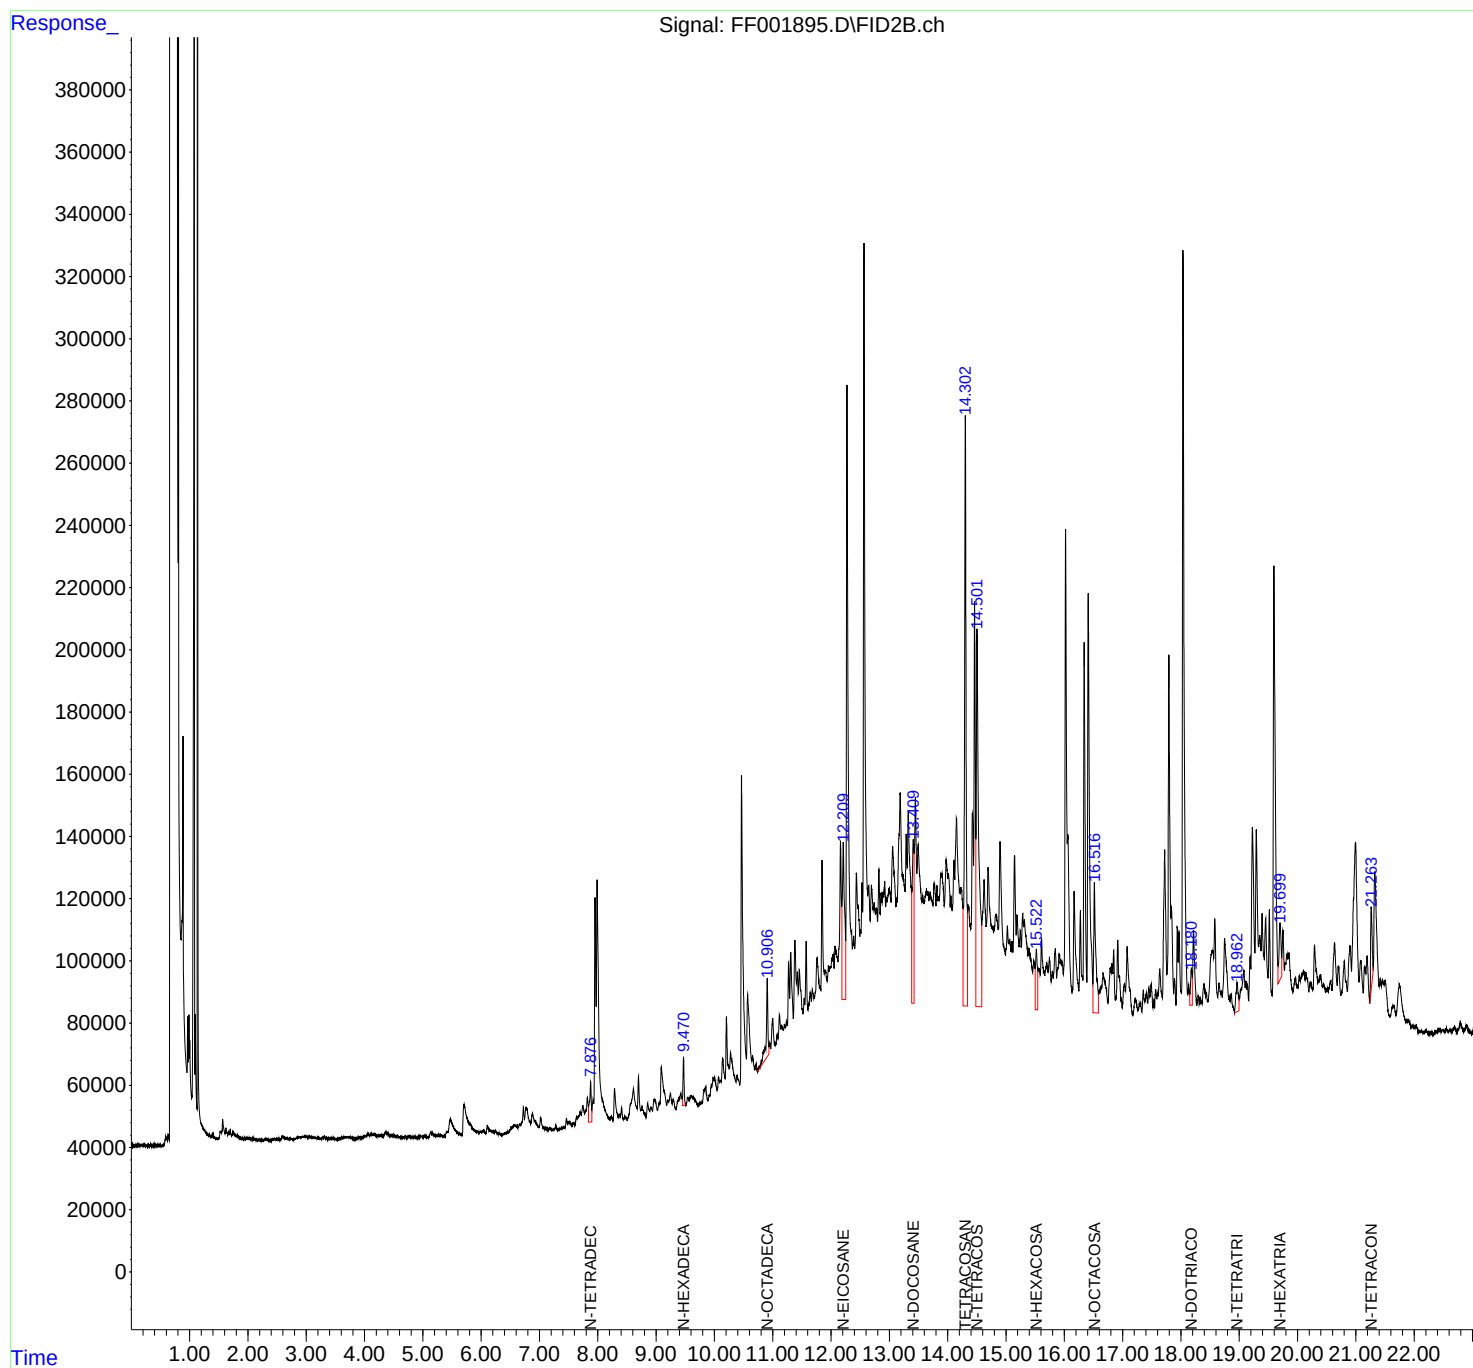


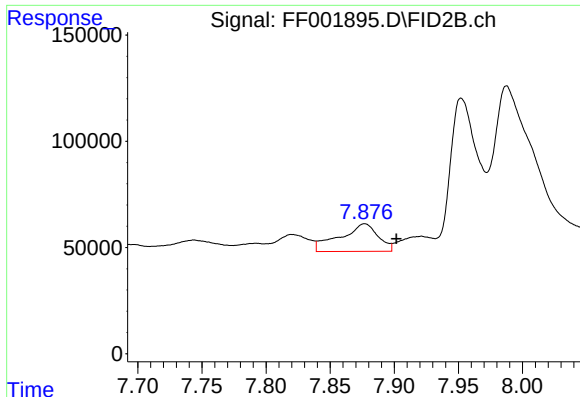

#4 N-TETRADECANE


R.T.: 7.877 min
Delta R.T.: -0.025 min
Response: 268893
Conc: 1.78 ug/ml

Instrument :
FID_F
ClientSampleId :

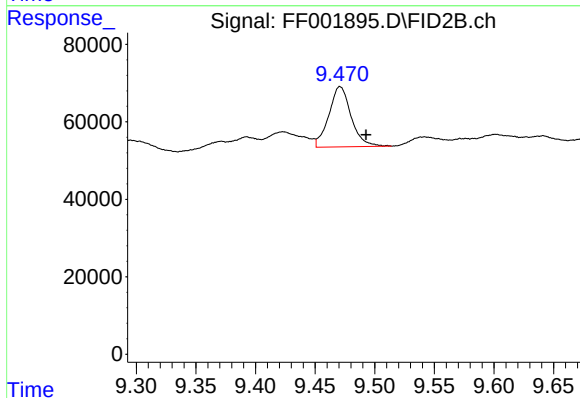


#5 N-HEXADECANE

R.T.: 9.471 min
Delta R.T.: -0.022 min
Response: 201933
Conc: 1.35 ug/ml

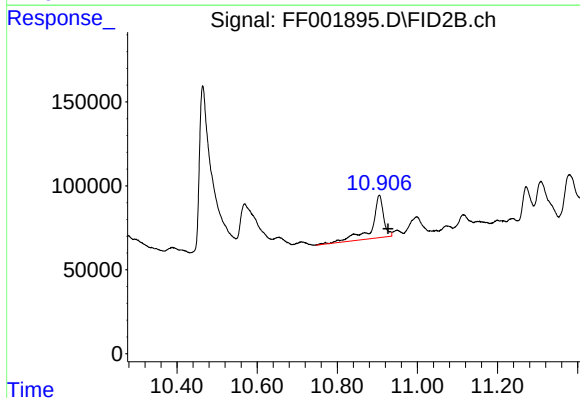


#6 N-OCTADECANE

R.T.: 10.905 min
Delta R.T.: -0.022 min
Response: 518696
Conc: 3.44 ug/ml

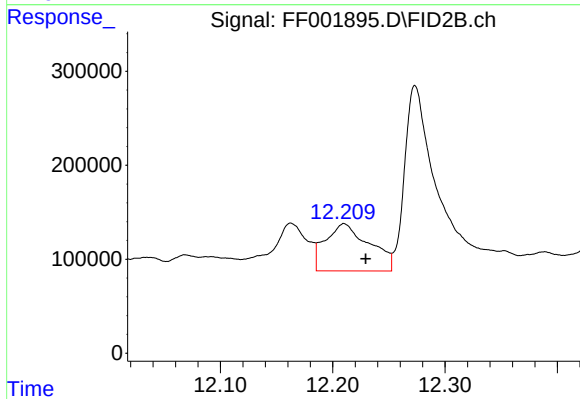

#7 N-EICOSANE


R.T.: 12.210 min
Delta R.T.: -0.019 min
Response: 1374559
Conc: 9.22 ug/ml

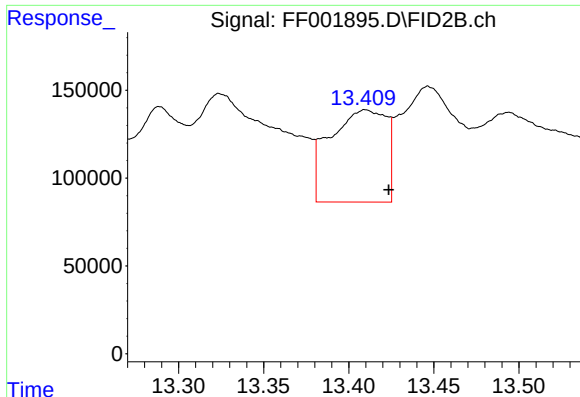

#8 N-DOCOSANE


R.T.: 13.410 min
Delta R.T.: -0.014 min
Response: 1207886
Conc: 8.27 ug/ml

Instrument :
FID_F
ClientSampleId :

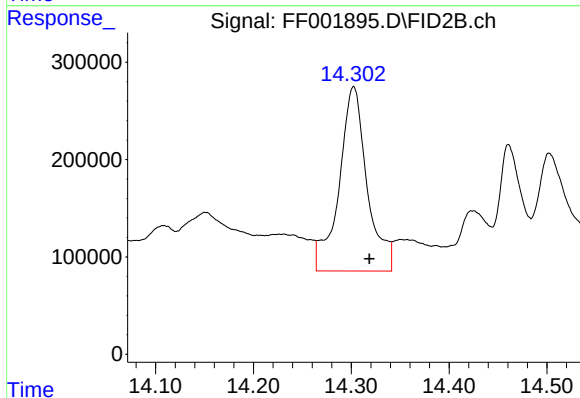


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.302 min
Delta R.T.: -0.016 min
Response: 3778776
Conc: 29.92 ug/ml

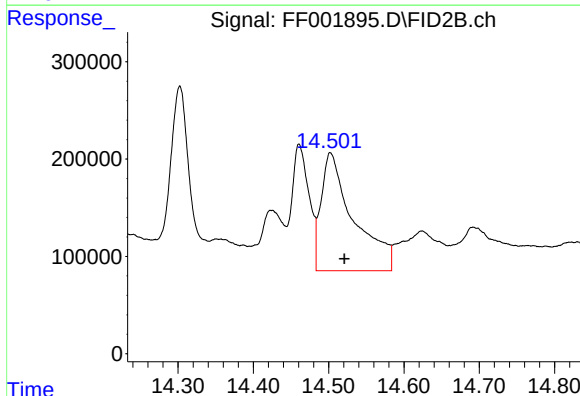


#10 N-TETRACOSANE

R.T.: 14.503 min
Delta R.T.: -0.018 min
Response: 3620960
Conc: 25.38 ug/ml

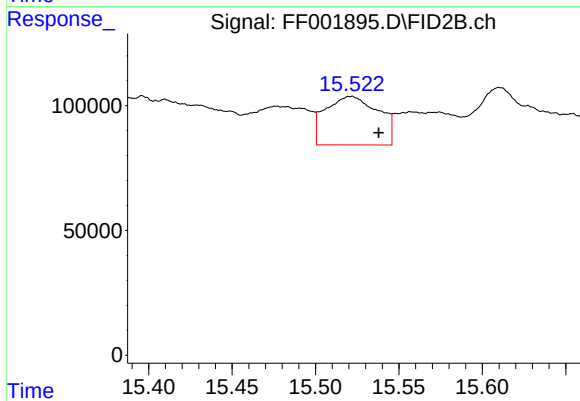

#11 N-HEXACOSANE


R.T.: 15.521 min
Delta R.T.: -0.017 min
Response: 429371
Conc: 3.05 ug/ml

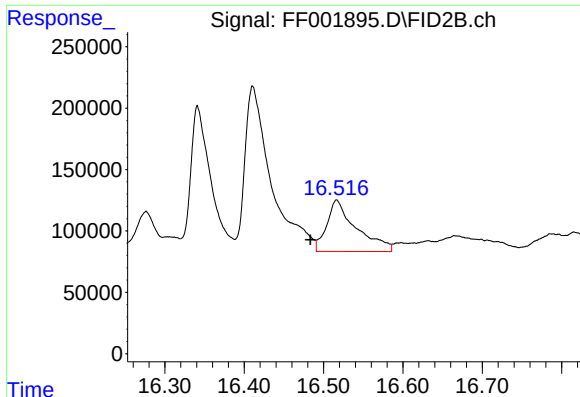

#12 N-OCTACOSANE


R.T.: 16.517 min
Delta R.T.: 0.033 min
Response: 1083627
Conc: 7.73 ug/ml

Instrument :
FID_F
ClientSampleId :

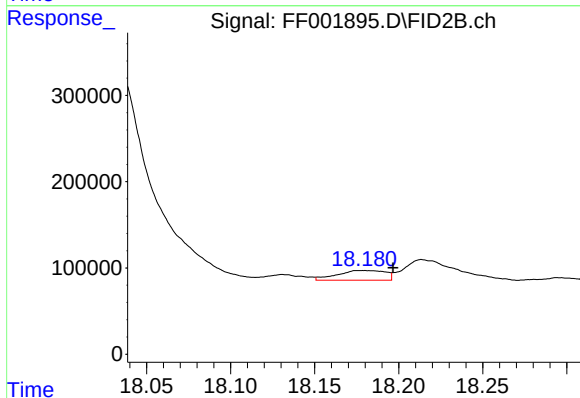


#14 N-DOTRIACONTANE

R.T.: 18.179 min
Delta R.T.: -0.018 min
Response: 225694
Conc: 1.73 ug/ml

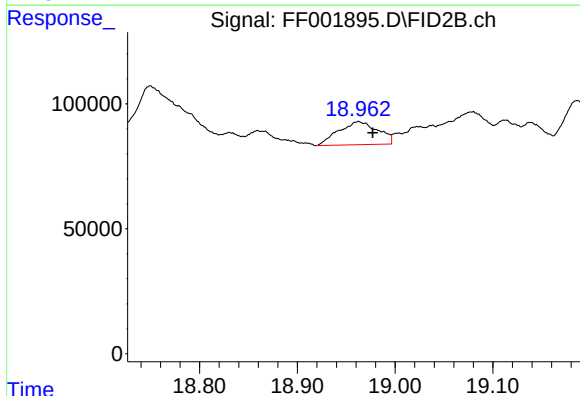


#15 N-TETRATRIACONTANE

R.T.: 18.963 min
Delta R.T.: -0.015 min
Response: 257672
Conc: 2.13 ug/ml

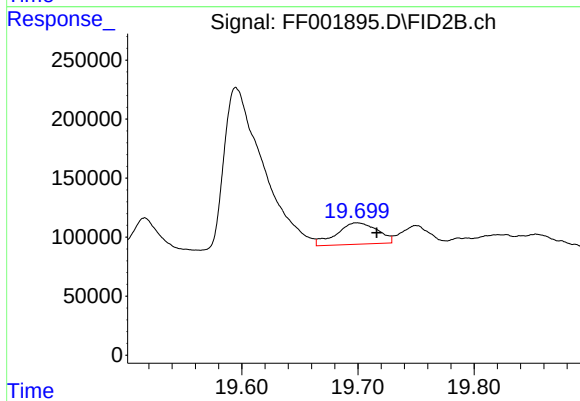

#16 N-HEXATRIACONTANE

R.T.: 19.699 min
Delta R.T.: -0.017 min
Response: 448414
Conc: 4.03 ug/ml

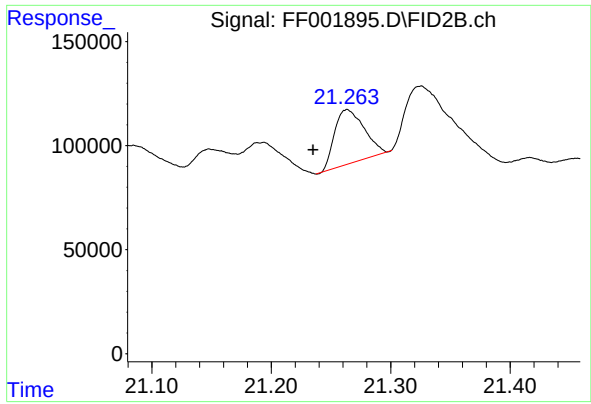

#18 N-TETRACONTANE

R.T.: 21.264 min
Delta R.T.: 0.029 min
Response: 449063
Conc: 4.51 ug/ml

Instrument :
FID_F
ClientSampleId :