

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082118\  
 Data File : FF001899.D  
 Signal(s) : FID2B.ch  
 Acq On : 21 Aug 2018 16:52  
 Operator : AJ\SJ  
 Sample : J4271-09 10X  
 Misc :  
 ALS Vial : 59 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Aug 22 01:27:46 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073018.M  
 Quant Title :  
 QLast Update : Fri Aug 03 12:00:27 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.301 | 271835   | 2.152 ug/ml  |
| Target Compounds              |        |          |              |
| 7) N-EICOSANE                 | 12.272 | 1583361  | 10.623 ug/ml |
| 10) N-TETRACOSANE             | 14.502 | 926796   | 6.497 ug/ml  |
| 12) N-OCTACOSANE              | 16.516 | 206805   | 1.475 ug/ml  |
| 16) N-HEXATRIACONTANE         | 19.707 | 57983    | 0.521 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082118\  
Data File : FF001899.D  
Signal(s) : FID2B.ch  
Acq On : 21 Aug 2018 16:52  
Operator : AJ\SJ  
Sample : J4271-09 10X  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 22 01:27:46 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF073018.M  
Quant Title :  
QLast Update : Fri Aug 03 12:00:27 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

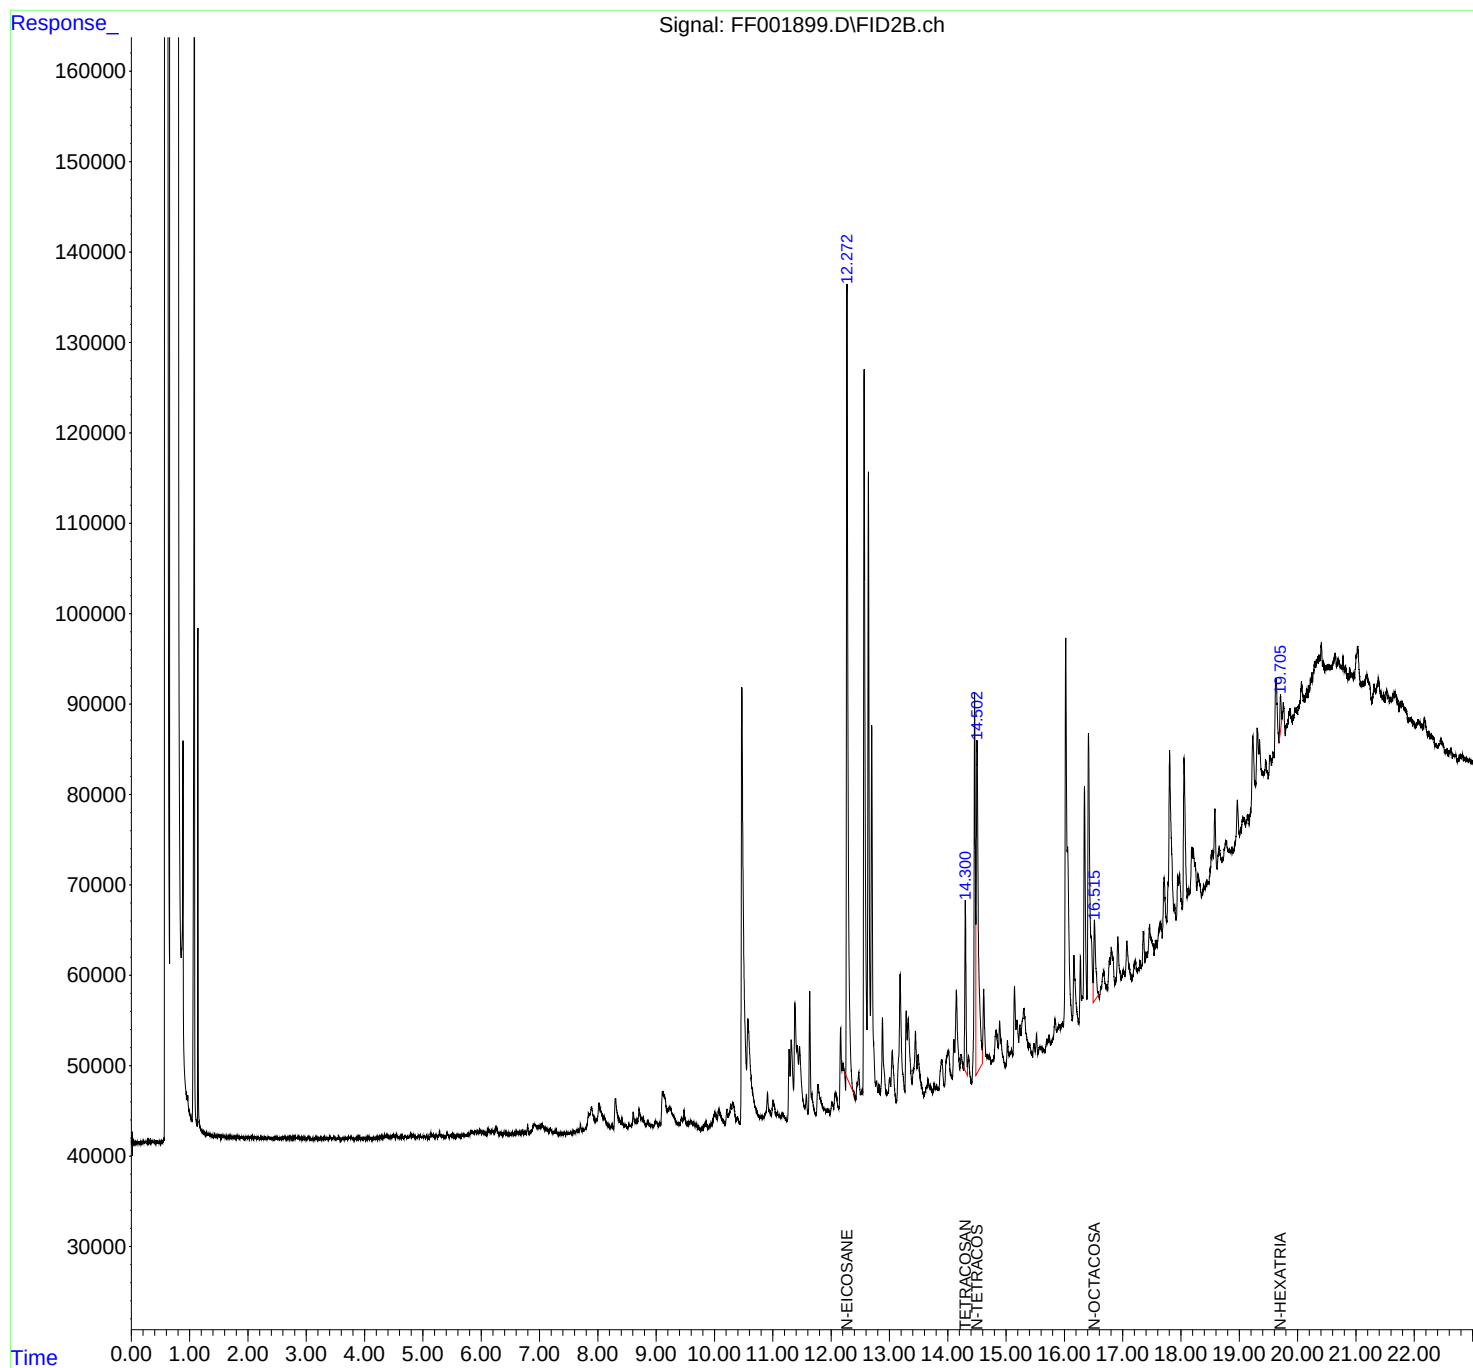


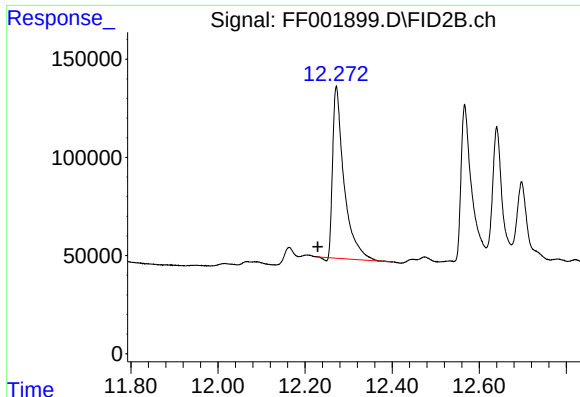

#7 N-EICOSANE


R.T.: 12.272 min  
Delta R.T.: 0.043 min  
Response: 1583361  
Conc: 10.62 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

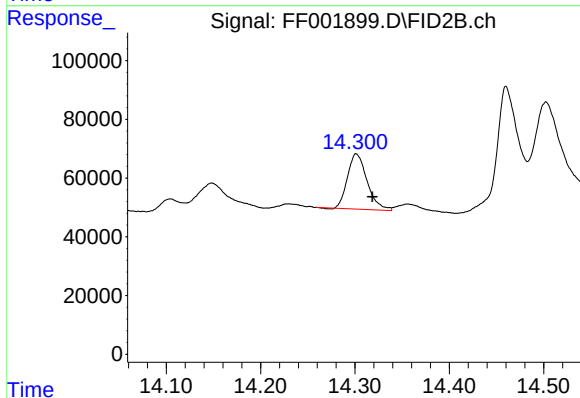


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.301 min  
Delta R.T.: -0.017 min  
Response: 271835  
Conc: 2.15 ug/ml

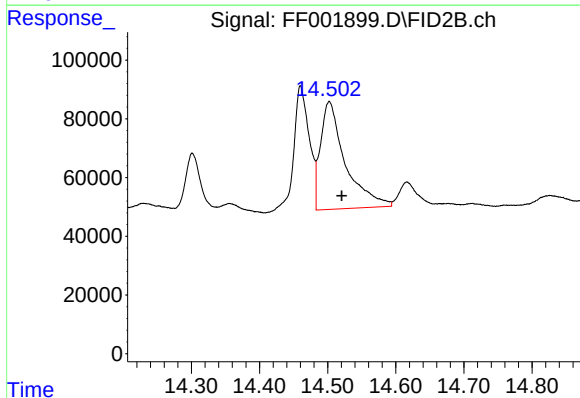


#10 N-TETRACOSANE

R.T.: 14.502 min  
Delta R.T.: -0.018 min  
Response: 926796  
Conc: 6.50 ug/ml

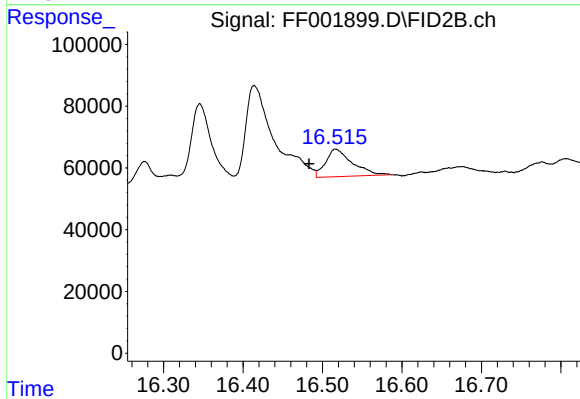

#12 N-OCTACOSANE

R.T.: 16.516 min  
Delta R.T.: 0.033 min  
Response: 206805  
Conc: 1.47 ug/ml

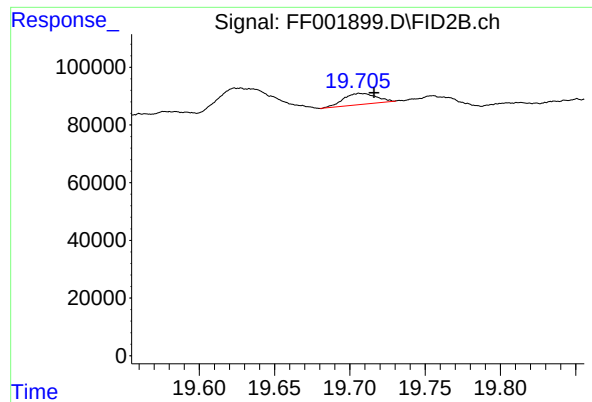

#16 N-HEXATRIACONTANE

R.T.: 19.707 min  
Delta R.T.: -0.009 min  
Response: 57983  
Conc: 0.52 ug/ml

Instrument :  
FID\_F  
ClientSampleId :