

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
 Data File : FF001900.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2018 17:23
 Operator : AJ\SJ
 Sample : J4271-13 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 22 01:27:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.303	317026	2.510 ug/ml
Target Compounds			
7) N-EICOSANE	12.272	1826779	12.257 ug/ml
10) N-TETRACOSANE	14.501	902269	6.325 ug/ml
12) N-OCTACOSANE	16.465	169385	1.208 ug/ml
14) N-DOTRIACONTANE	18.184	22564	0.173 ug/ml
15) N-TETRATRIACONTANE	18.970	206150	1.705 ug/ml
16) N-HEXATRIACONTANE	19.708	111699	1.004 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
Data File : FF001900.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2018 17:23
Operator : AJ\SJ
Sample : J4271-13 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:27:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

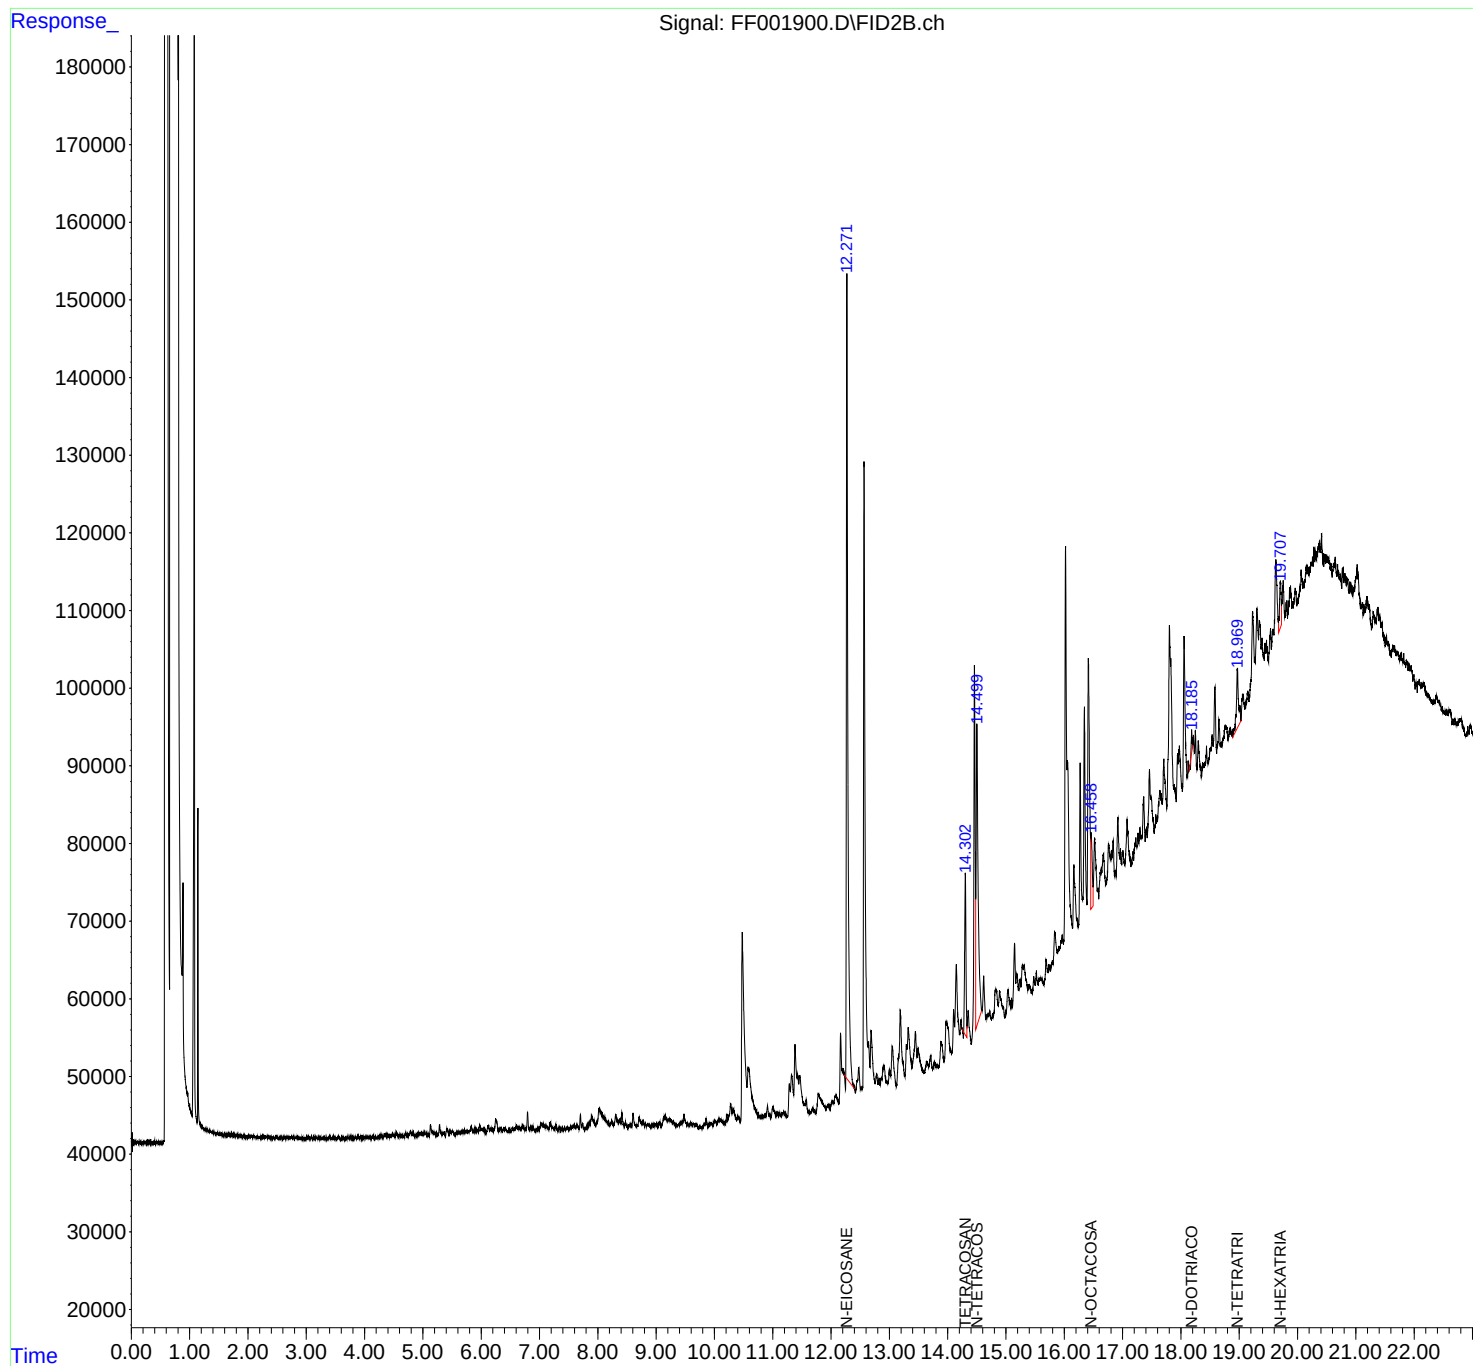


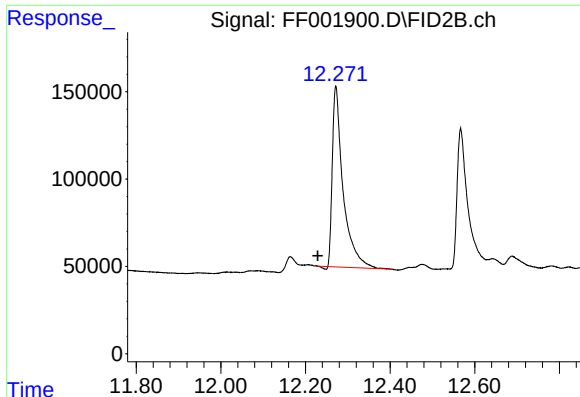

#7 N-EICOSANE


R.T.: 12.272 min
Delta R.T.: 0.042 min
Response: 1826779
Conc: 12.26 ug/ml

Instrument :
FID_F
ClientSampleId :

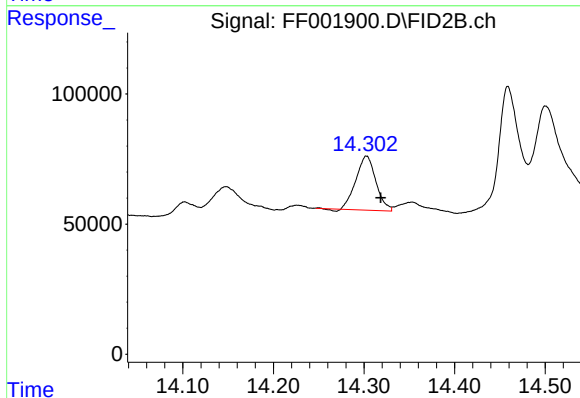


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.303 min
Delta R.T.: -0.016 min
Response: 317026
Conc: 2.51 ug/ml

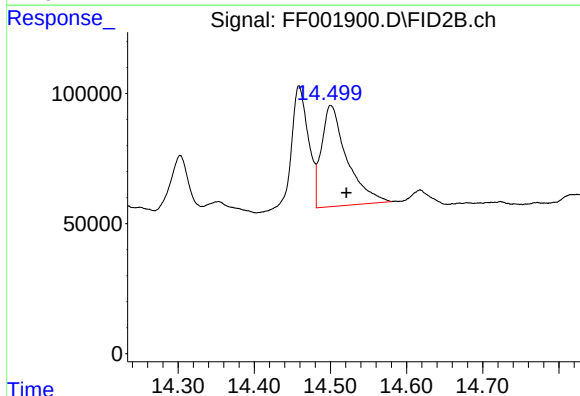


#10 N-TETRACOSANE

R.T.: 14.501 min
Delta R.T.: -0.020 min
Response: 902269
Conc: 6.32 ug/ml

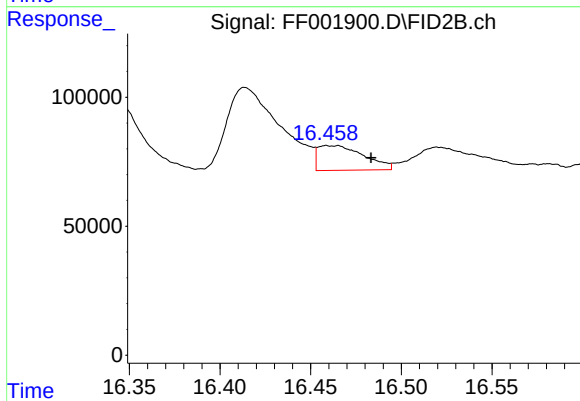

#12 N-OCTACOSANE


R.T.: 16.465 min
Delta R.T.: -0.018 min
Response: 169385
Conc: 1.21 ug/ml

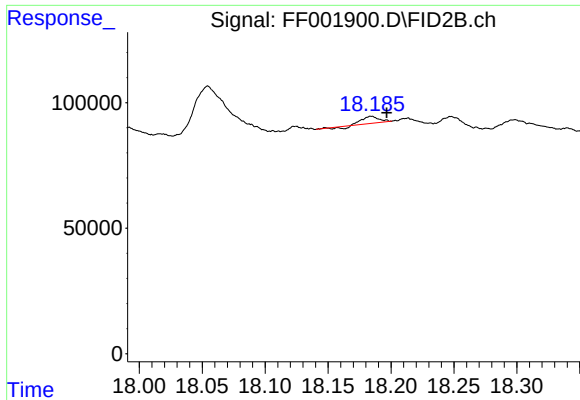

#14 N-DOTRIACONTANE


R.T.: 18.184 min
Delta R.T.: -0.012 min
Response: 22564
Conc: 0.17 ug/ml

Instrument :
FID_F
ClientSampleId :

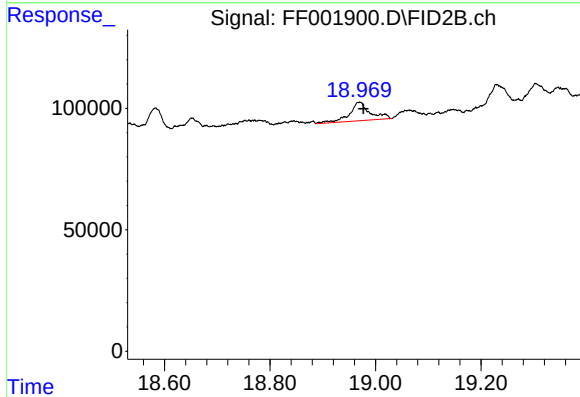

#15 N-TETRATRIACONTANE

R.T.: 18.970 min
Delta R.T.: -0.007 min
Response: 206150
Conc: 1.71 ug/ml

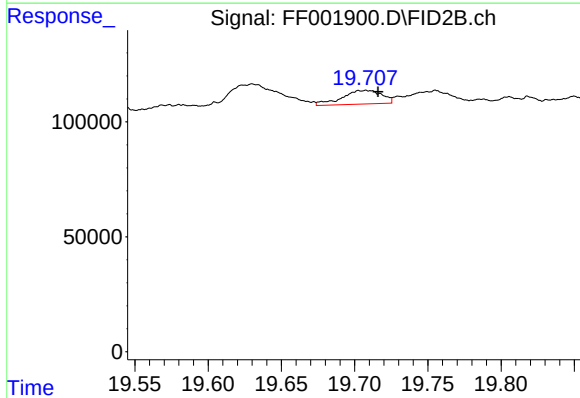

#16 N-HEXATRIACONTANE

R.T.: 19.708 min
Delta R.T.: -0.008 min
Response: 111699
Conc: 1.00 ug/ml