

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
 Data File : FF001904.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2018 19:25
 Operator : AJ\SJ
 Sample : J4277-05 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 22 01:28:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.302	105241	0.833 ug/ml
Target Compounds			
7) N-EICOSANE	12.293f	269778	1.810 ug/ml
12) N-OCTACOSANE	16.465	242791	1.732 ug/ml
13) N-TRIACONTANE	17.356	277009	2.001 ug/ml
14) N-DOTRIACONTANE	18.184	125605	0.963 ug/ml
15) N-TETRATRIACONTANE	18.968	171995	1.423 ug/ml
16) N-HEXATRIACONTANE	19.713	82422	0.741 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
Data File : FF001904.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2018 19:25
Operator : AJ\SJ
Sample : J4277-05 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:28:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

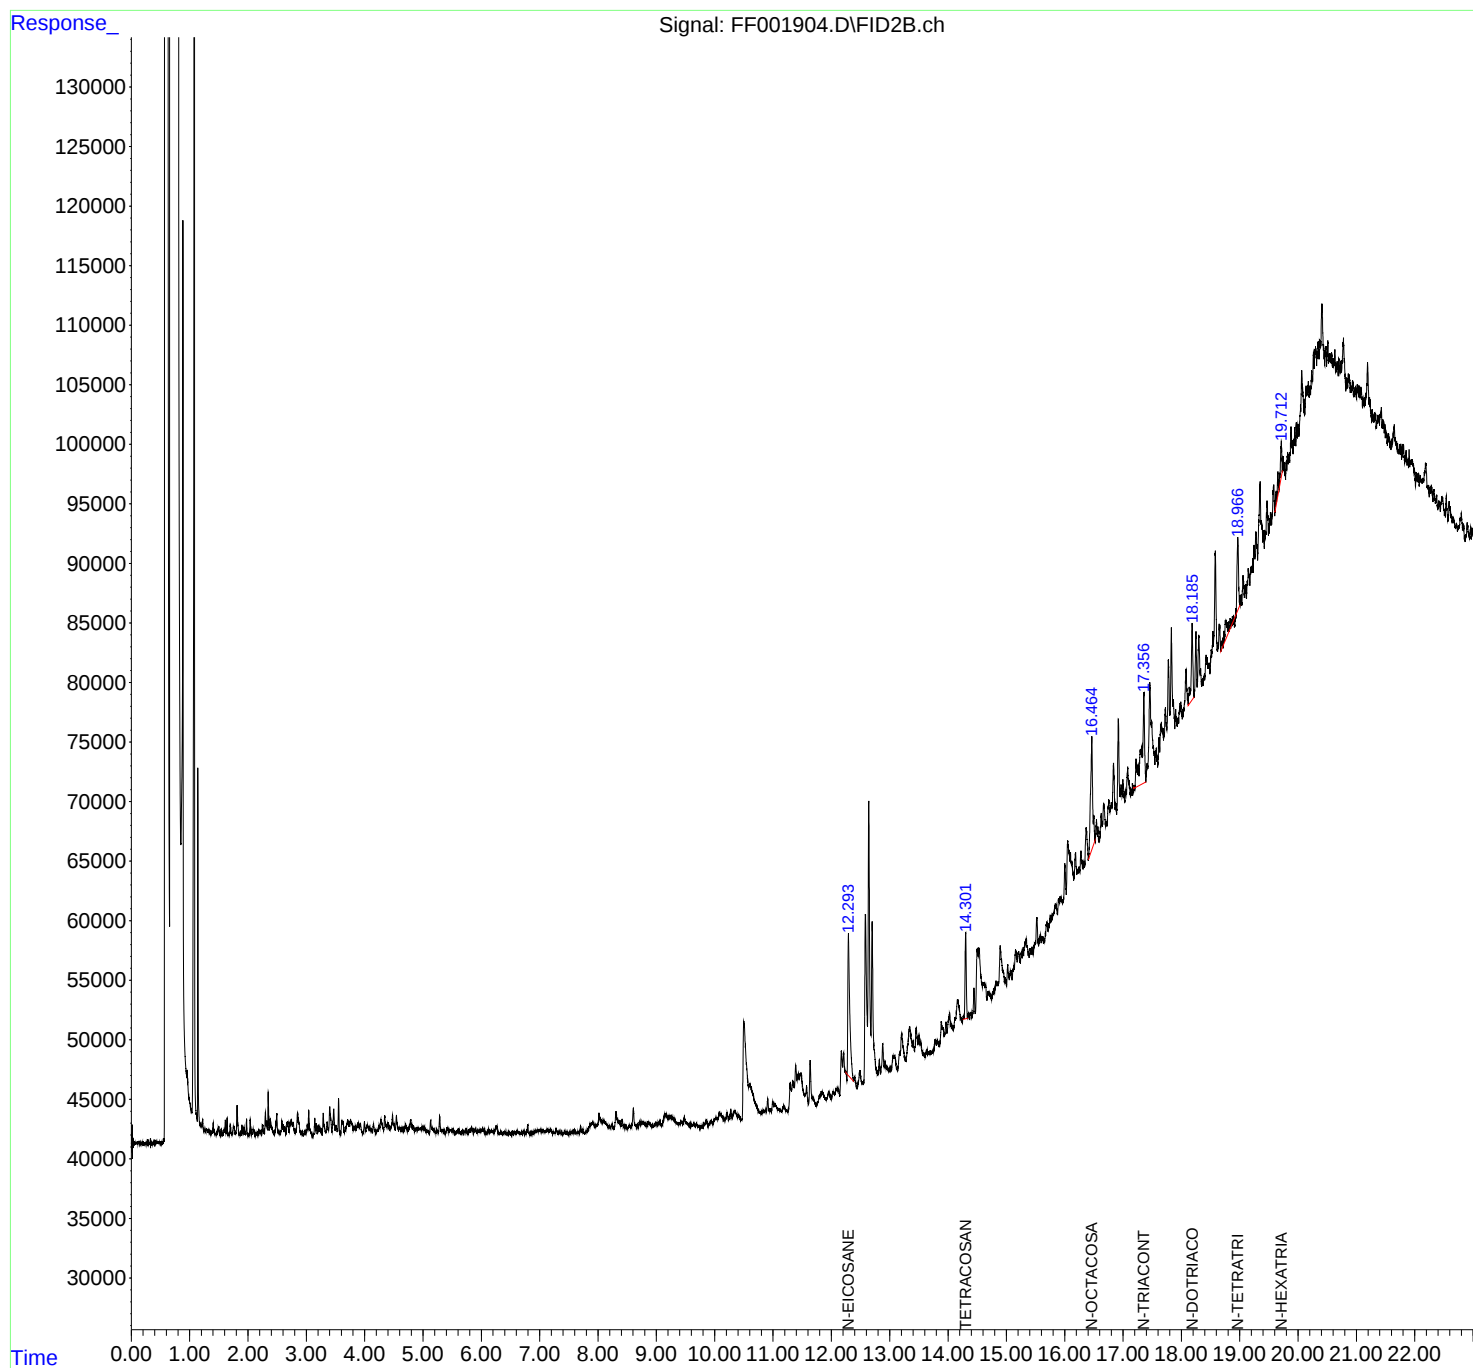


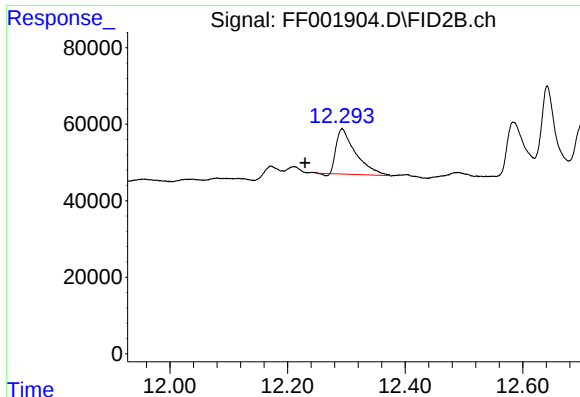

#7 N-EICOSANE


R.T.: 12.293 min
Delta R.T.: 0.064 min
Response: 269778
Conc: 1.81 ug/ml

Instrument :
FID_F
ClientSampleId :

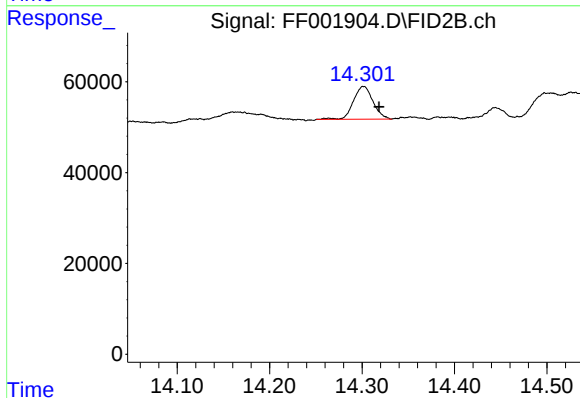


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.302 min
Delta R.T.: -0.017 min
Response: 105241
Conc: 0.83 ug/ml

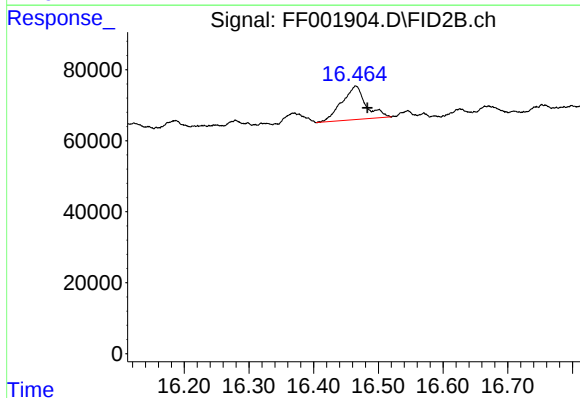


#12 N-OCTACOSANE

R.T.: 16.465 min
Delta R.T.: -0.018 min
Response: 242791
Conc: 1.73 ug/ml

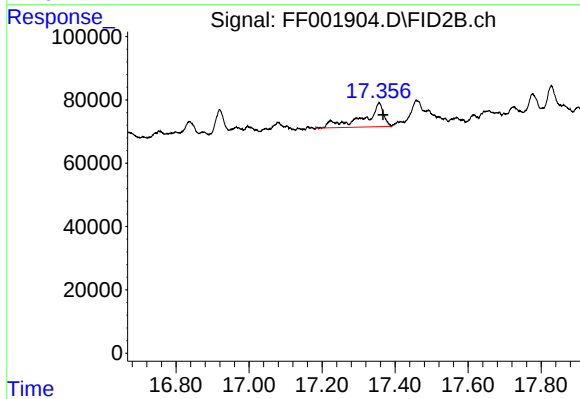

#13 N-TRIACONTANE


R.T.: 17.356 min
Delta R.T.: -0.011 min
Response: 277009
Conc: 2.00 ug/ml

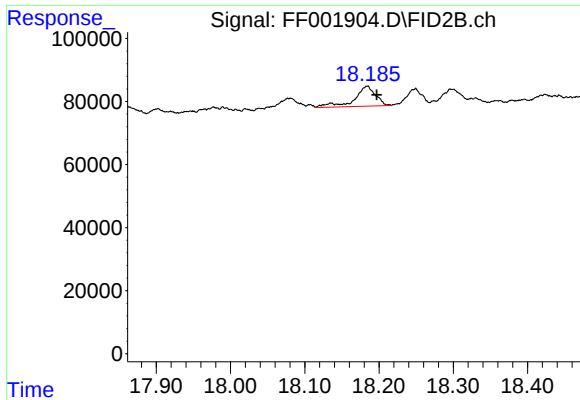

#14 N-DOTRIACONTANE


R.T.: 18.184 min
Delta R.T.: -0.013 min
Response: 125605
Conc: 0.96 ug/ml

Instrument :
FID_F
ClientSampleId :

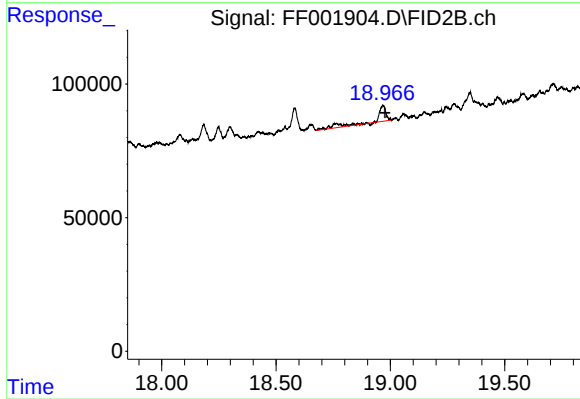

#15 N-TETRATRIACONTANE

R.T.: 18.968 min
Delta R.T.: -0.009 min
Response: 171995
Conc: 1.42 ug/ml

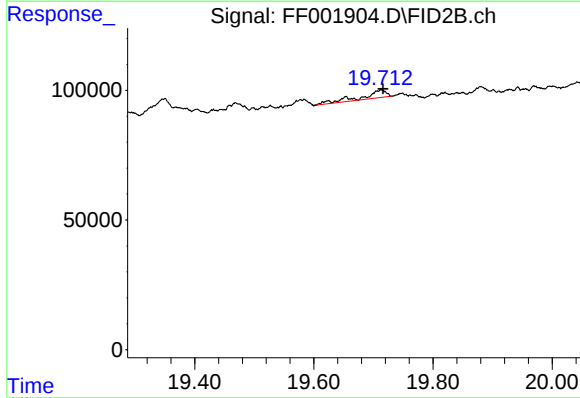

#16 N-HEXATRIACONTANE

R.T.: 19.713 min
Delta R.T.: -0.003 min
Response: 82422
Conc: 0.74 ug/ml