

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
 Data File : FF001907.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2018 20:57
 Operator : AJ\SJ
 Sample : J4573-10 5X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 22 01:29:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.302	377580	2.990 ug/ml
Target Compounds			
4) N-TETRADECANE	7.964f	94754	0.629 ug/ml
6) N-OCTADECANE	10.908	109901	0.729 ug/ml
7) N-EICOSANE	12.211	119663	0.803 ug/ml
8) N-DOCOSANE	13.443	79714	0.546 ug/ml
10) N-TETRACOSANE	14.504	511193	3.583 ug/ml
12) N-OCTACOSANE	16.511	461029	3.288 ug/ml
14) N-DOTRIACONTANE	18.198	650240	4.984 ug/ml
16) N-HEXATRIACONTANE	19.707	188738	1.696 ug/ml
18) N-TETRACONTANE	21.290f	36727	0.369 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
Data File : FF001907.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2018 20:57
Operator : AJ\SJ
Sample : J4573-10 5X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:29:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

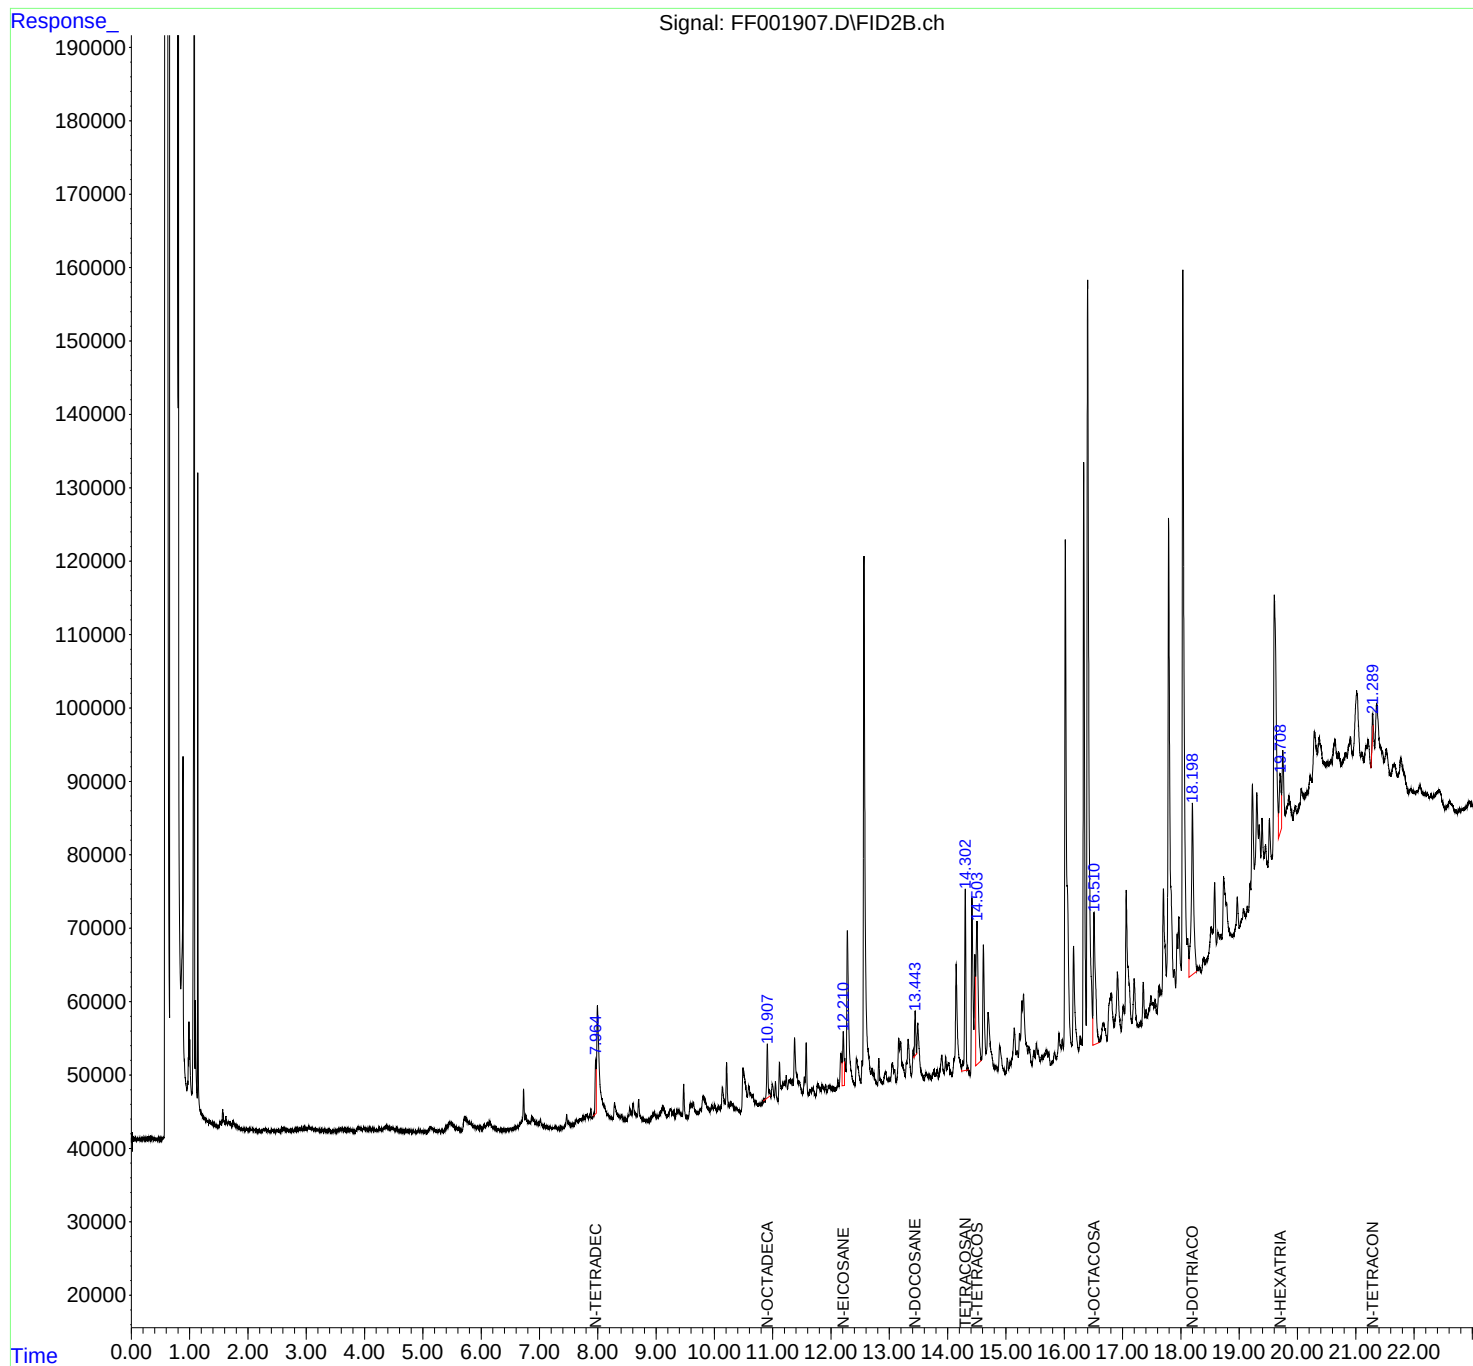


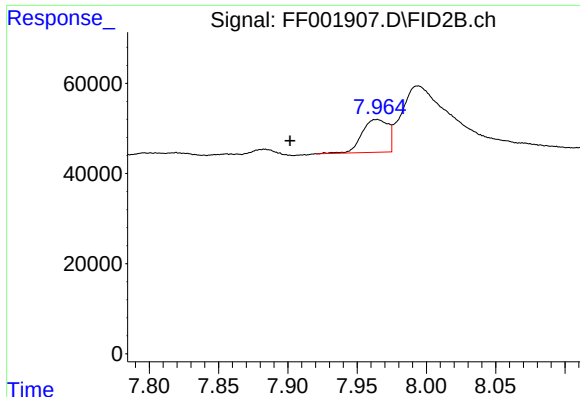

#4 N-TETRADECANE


R.T.: 7.964 min
Delta R.T.: 0.062 min
Response: 94754
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

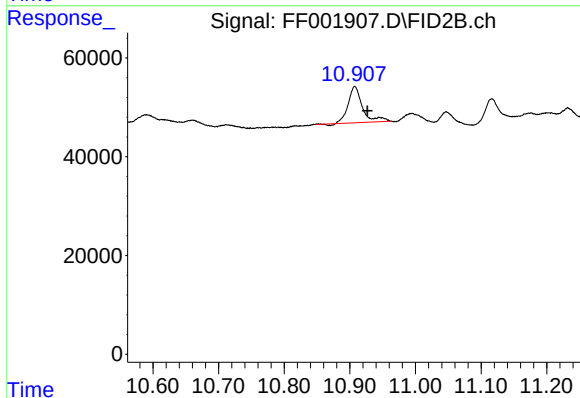


#6 N-OCTADECANE

R.T.: 10.908 min
Delta R.T.: -0.019 min
Response: 109901
Conc: 0.73 ug/ml

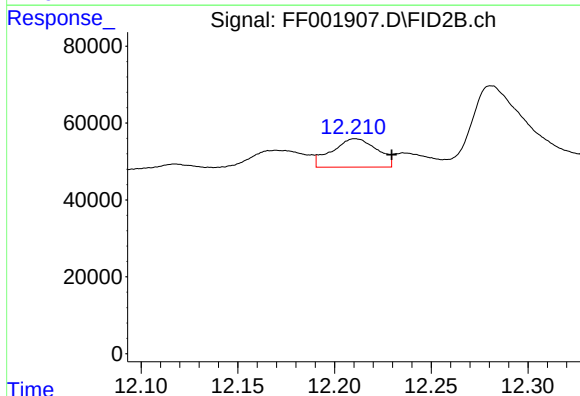


#7 N-EICOSANE

R.T.: 12.211 min
Delta R.T.: -0.019 min
Response: 119663
Conc: 0.80 ug/ml

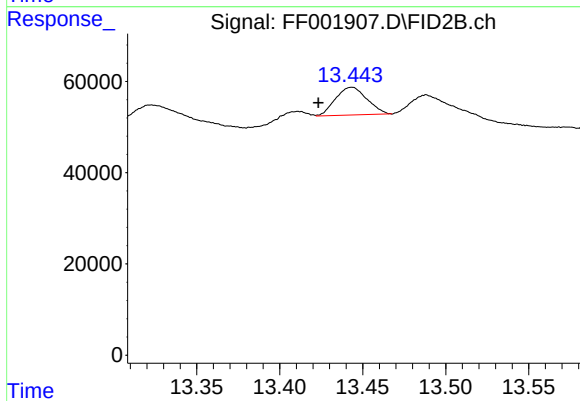

#8 N-DOCOSANE


R.T.: 13.443 min
Delta R.T.: 0.020 min
Response: 79714
Conc: 0.55 ug/ml

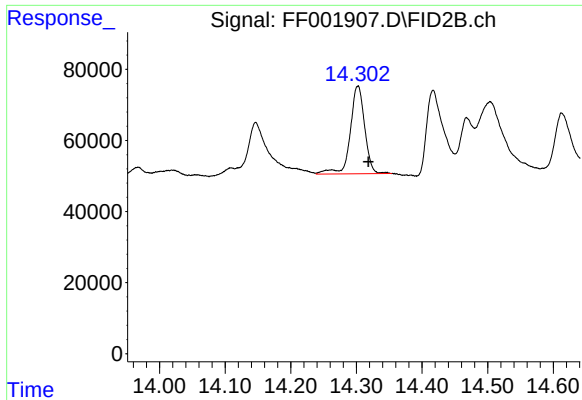

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.302 min
Delta R.T.: -0.016 min
Response: 377580
Conc: 2.99 ug/ml

Instrument :
FID_F
ClientSampleId :

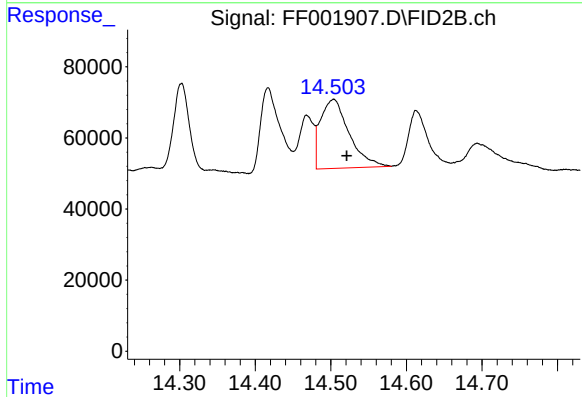


#10 N-TETRACOSANE

R.T.: 14.504 min
Delta R.T.: -0.017 min
Response: 511193
Conc: 3.58 ug/ml

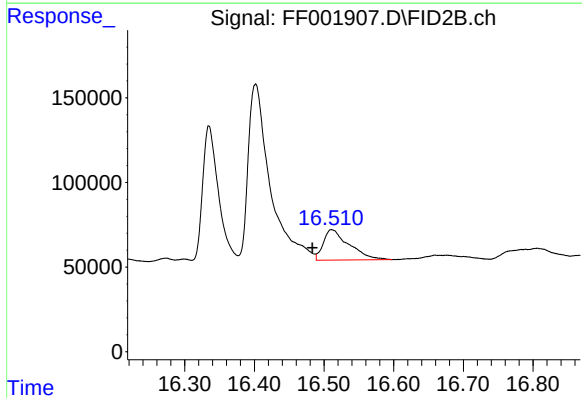


#12 N-OCTACOSANE

R.T.: 16.511 min
Delta R.T.: 0.028 min
Response: 461029
Conc: 3.29 ug/ml

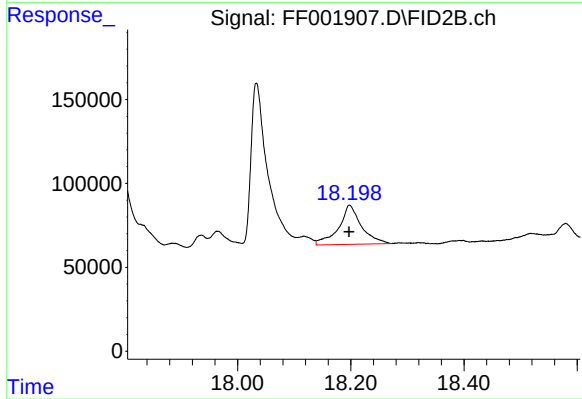

#14 N-DOTRIACONTANE


R.T.: 18.198 min
Delta R.T.: 0.001 min
Response: 650240
Conc: 4.98 ug/ml

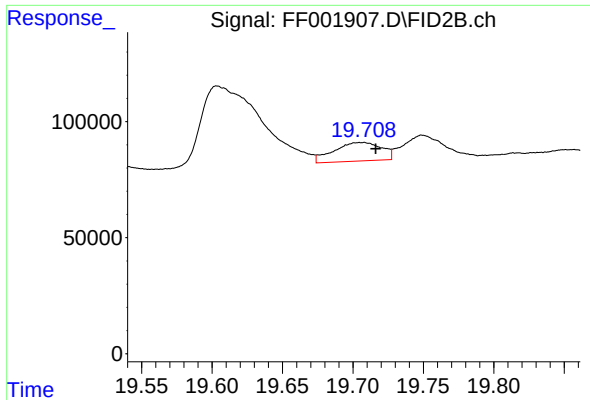

#16 N-HEXATRIACONTANE

R.T.: 19.707 min
Delta R.T.: -0.009 min
Response: 188738
Conc: 1.70 ug/ml

Instrument :
FID_F
ClientSampleId :

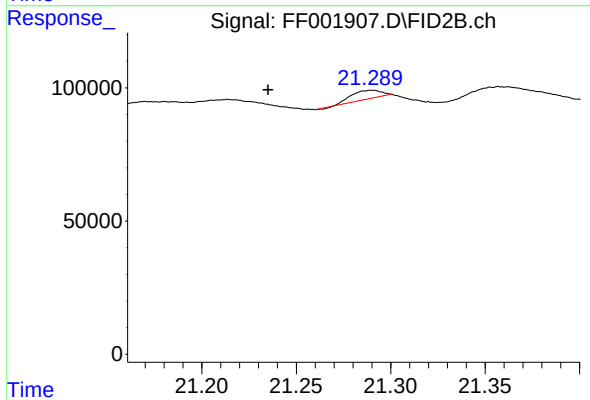

#18 N-TETRACONTANE

R.T.: 21.290 min
Delta R.T.: 0.055 min
Response: 36727
Conc: 0.37 ug/ml