

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
 Data File : FF001908.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2018 21:28
 Operator : AJ\SJ
 Sample : J4573-05 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 22 01:29:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.301	499259	3.953 ug/ml
Target Compounds			
7) N-EICOSANE	12.269	1936263	12.991 ug/ml
10) N-TETRACOSANE	14.497	1214844	8.516 ug/ml
12) N-OCTACOSANE	16.517	277062	1.976 ug/ml
14) N-DOTRIACONTANE	18.185	6910	0.053 ug/ml
16) N-HEXATRIACONTANE	19.707	87708	0.788 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082118\
Data File : FF001908.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2018 21:28
Operator : AJ\SJ
Sample : J4573-05 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:29:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

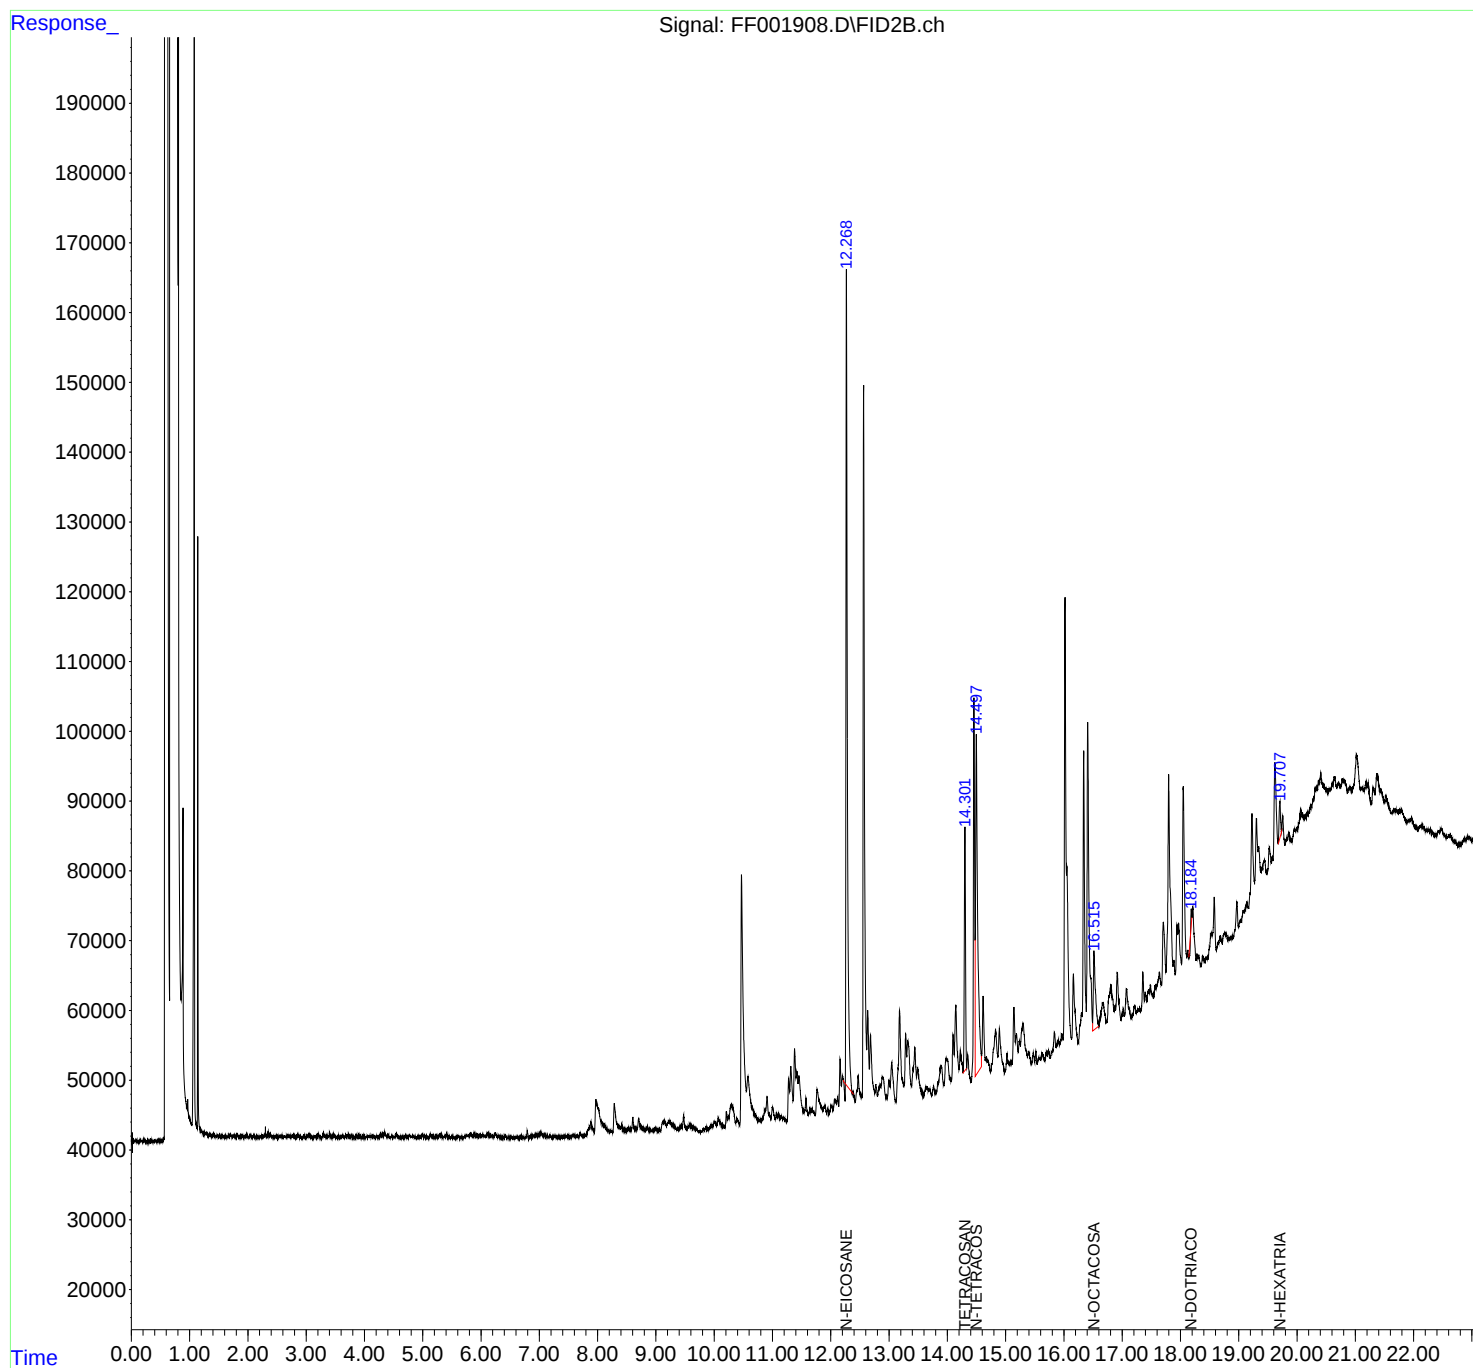


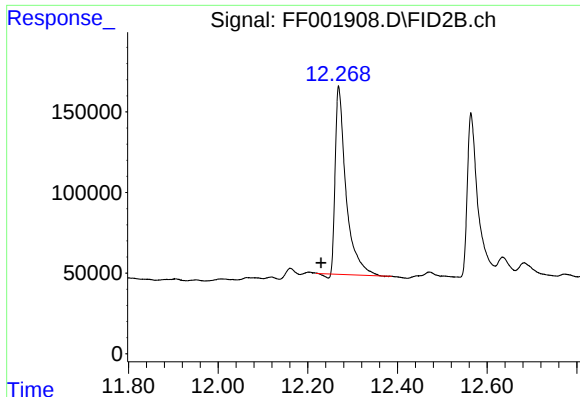

#7 N-EICOSANE


R.T.: 12.269 min
Delta R.T.: 0.040 min
Response: 1936263
Conc: 12.99 ug/ml

Instrument :
FID_F
ClientSampleId :

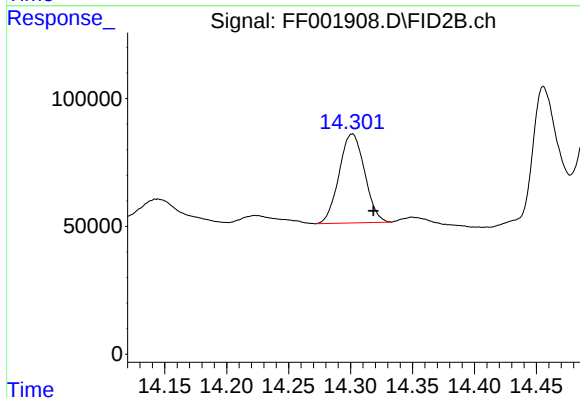


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.301 min
Delta R.T.: -0.017 min
Response: 499259
Conc: 3.95 ug/ml

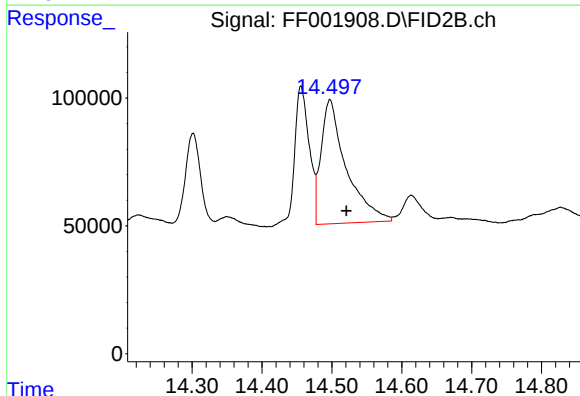


#10 N-TETRACOSANE

R.T.: 14.497 min
Delta R.T.: -0.024 min
Response: 1214844
Conc: 8.52 ug/ml

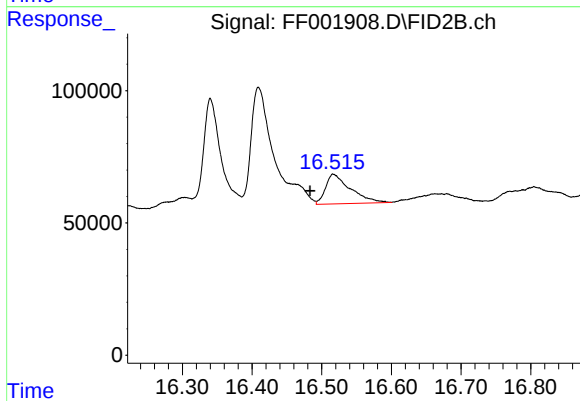

#12 N-OCTACOSANE


R.T.: 16.517 min
Delta R.T.: 0.033 min
Response: 277062
Conc: 1.98 ug/ml

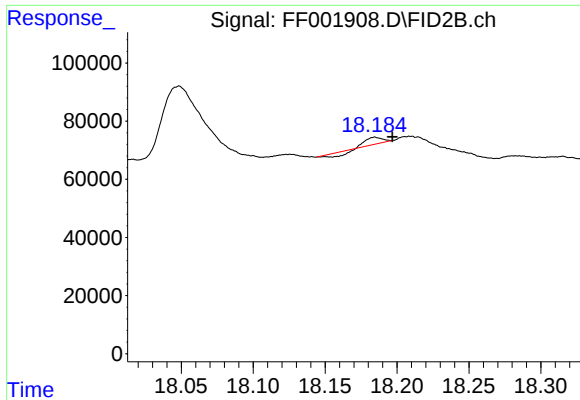

#14 N-DOTRIACONTANE

R.T.: 18.185 min
Delta R.T.: -0.012 min
Response: 6910
Conc: 0.05 ug/ml

Instrument :
FID_F
ClientSampleId :

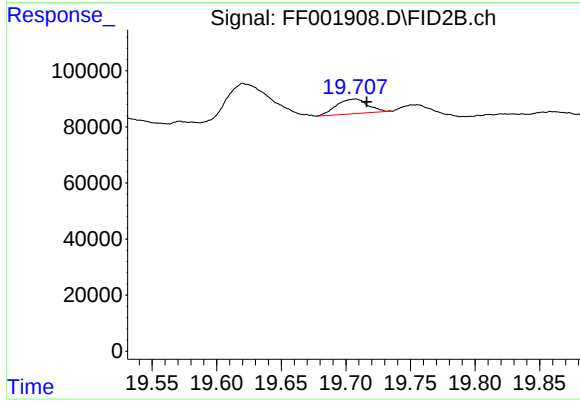

#16 N-HEXATRIACONTANE

R.T.: 19.707 min
Delta R.T.: -0.010 min
Response: 87708
Conc: 0.79 ug/ml