

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082120\
 Data File : FF007402.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2020 16:11
 Operator : DD\AJ
 Sample : L3734-06 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 EROC-BF-1E

Integration File: autoint1.e
 Quant Time: Aug 22 00:42:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	184992	1.355 ug/ml
Target Compounds			
7) N-EICOSANE	12.712f	257783	1.665 ug/ml
10) N-TETRACOSANE	14.939	177690	1.125 ug/ml
11) N-HEXACOSANE	15.977	110321	0.704 ug/ml
12) N-OCTACOSANE	16.930	227190	1.448 ug/ml
13) N-TRIACONTANE	17.819	252619	1.611 ug/ml
14) N-DOTRIACONTANE	18.655	237652	1.604 ug/ml
15) N-TETRATRIACONTANE	19.442	171168	1.415 ug/ml
16) N-HEXATRIACONTANE	20.191	363365	3.928 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082120\
Data File : FF007402.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2020 16:11
Operator : DD\AJ
Sample : L3734-06 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EROC-BF-1E

Integration File: autoint1.e
Quant Time: Aug 22 00:42:49 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

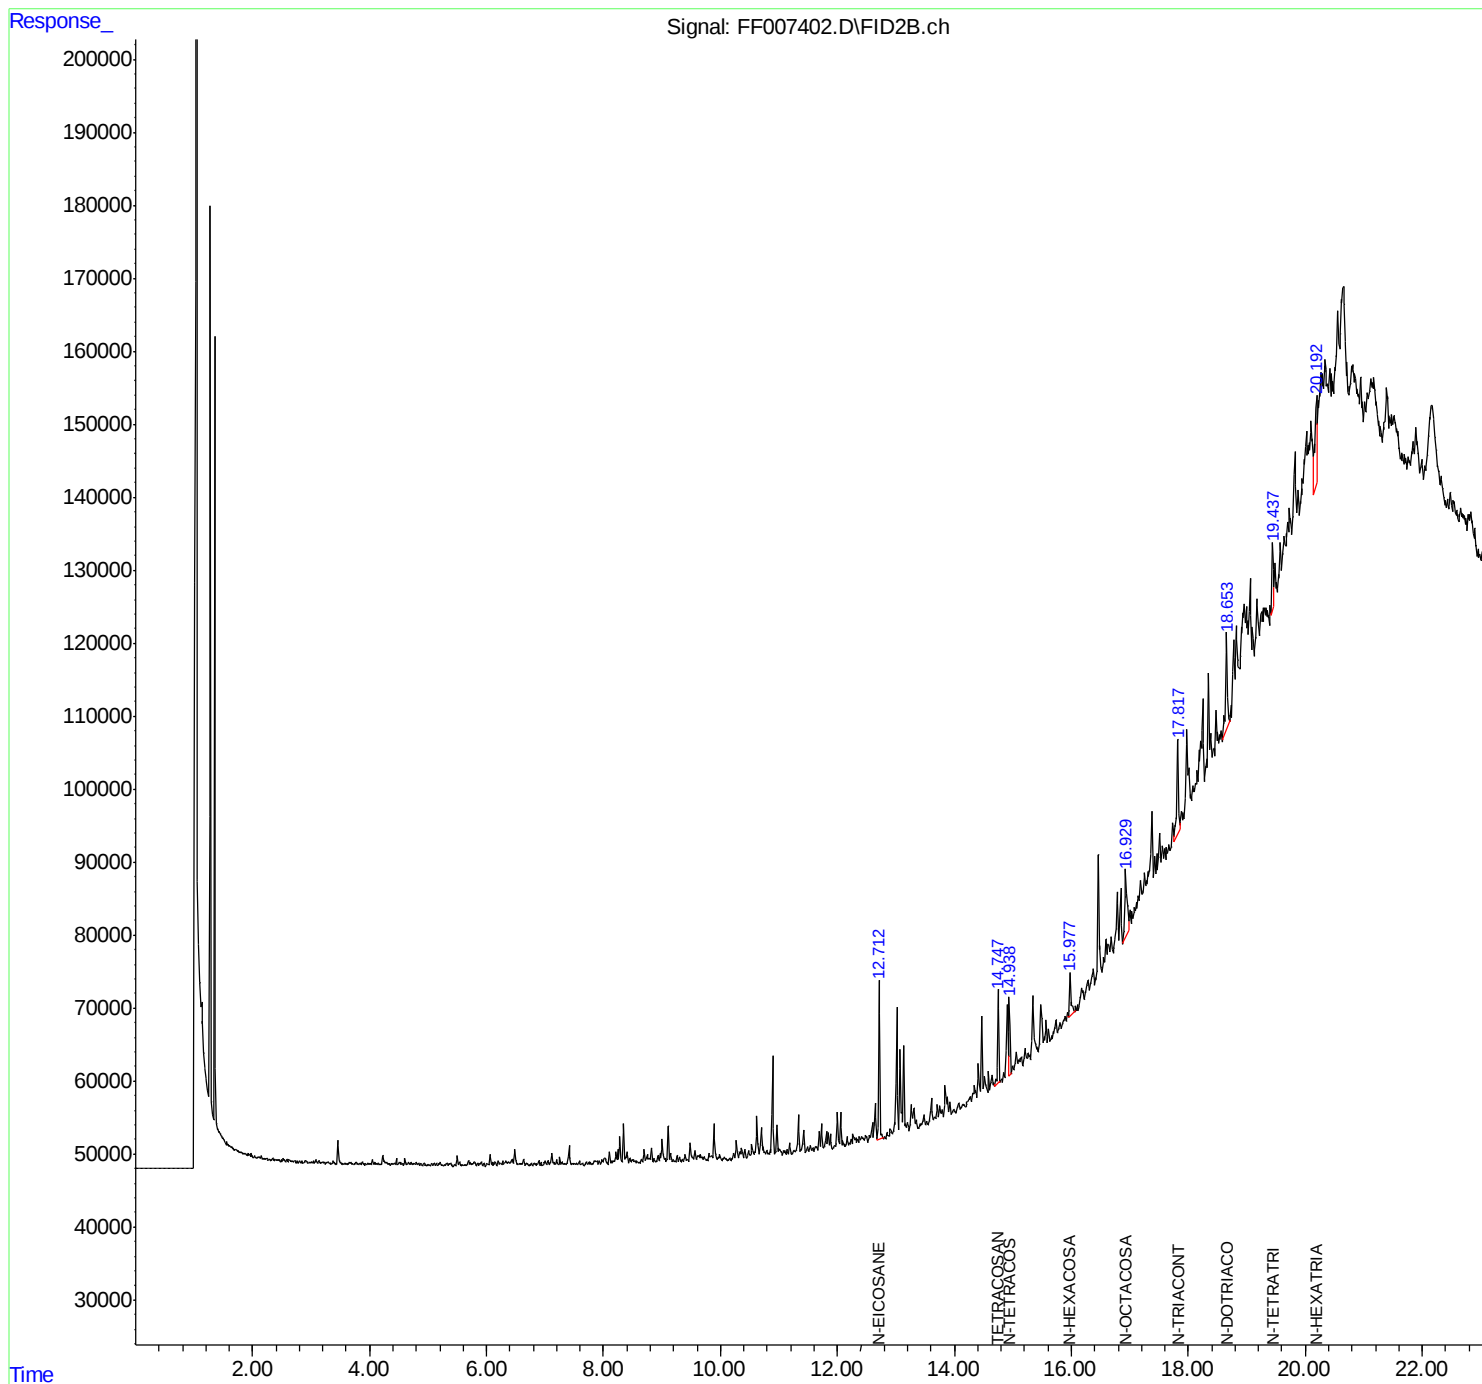


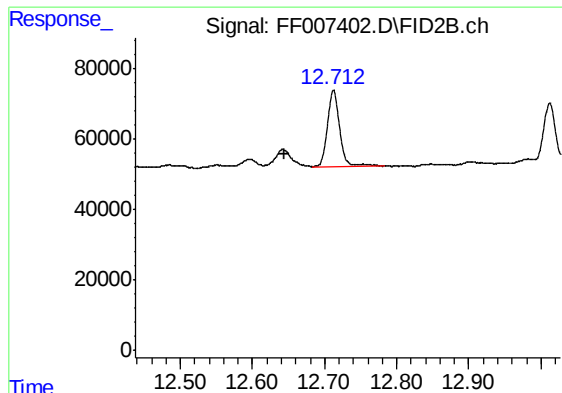

#7 N-EICOSANE


R.T.: 12.712 min
Delta R.T.: 0.068 min
Response: 257783
Conc: 1.67 ug/ml

Instrument :
FID_F
ClientSampleId :
EROC-BF-1E

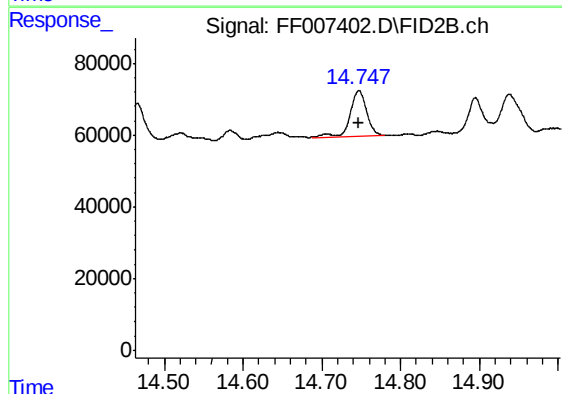


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min
Delta R.T.: 0.000 min
Response: 184992
Conc: 1.36 ug/ml

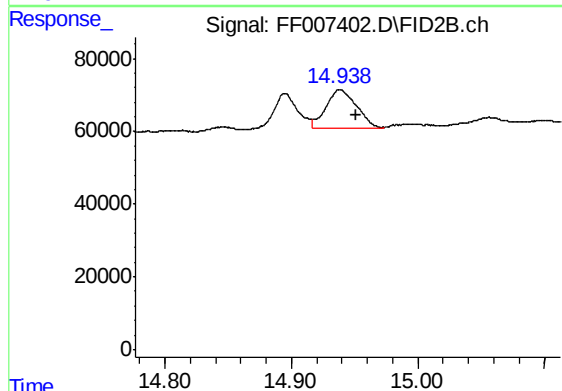


#10 N-TETRACOSANE

R.T.: 14.939 min
Delta R.T.: -0.013 min
Response: 177690
Conc: 1.13 ug/ml

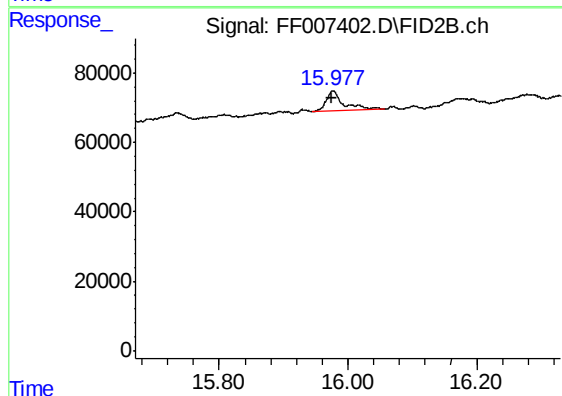

#11 N-HEXACOSANE


R.T.: 15.977 min
Delta R.T.: 0.002 min
Response: 110321
Conc: 0.70 ug/ml

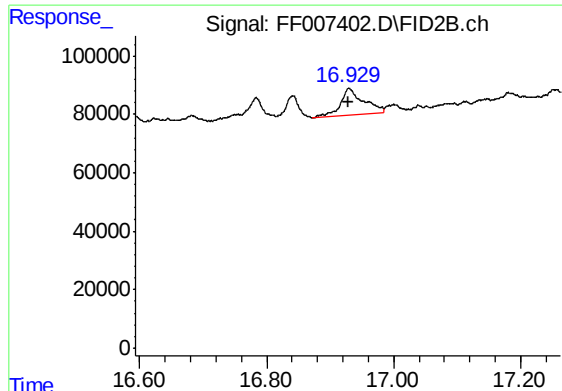

#12 N-OCTACOSANE


R.T.: 16.930 min
Delta R.T.: 0.002 min
Response: 227190
Conc: 1.45 ug/ml

Instrument :
FID_F
ClientSampleId :
EROC-BF-1E

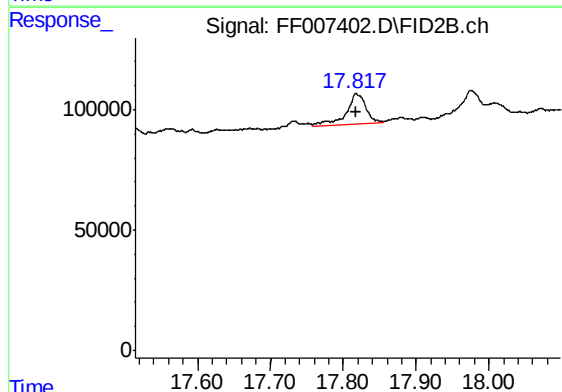


#13 N-TRIACONTANE

R.T.: 17.819 min
Delta R.T.: 0.001 min
Response: 252619
Conc: 1.61 ug/ml

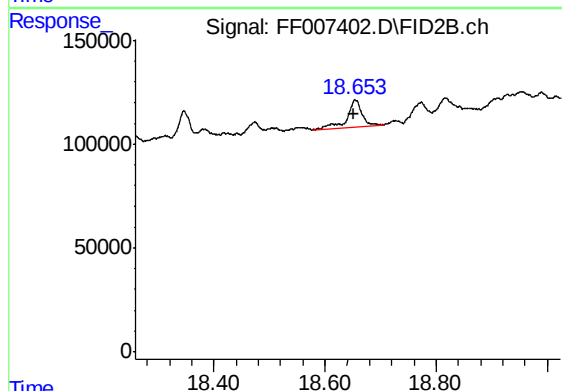


#14 N-DOTRIACONTANE

R.T.: 18.655 min
Delta R.T.: 0.002 min
Response: 237652
Conc: 1.60 ug/ml

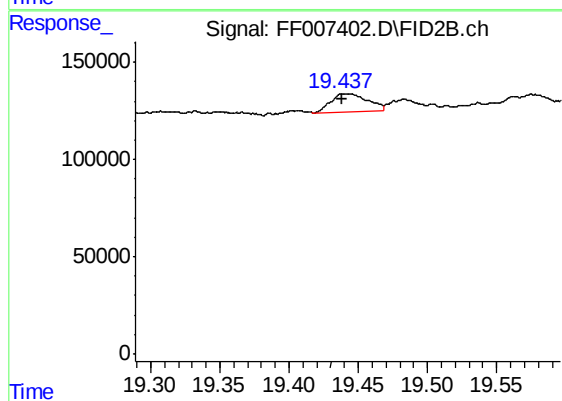

#15 N-TETRATRIACONTANE

R.T.: 19.442 min
Delta R.T.: 0.003 min
Response: 171168
Conc: 1.42 ug/ml

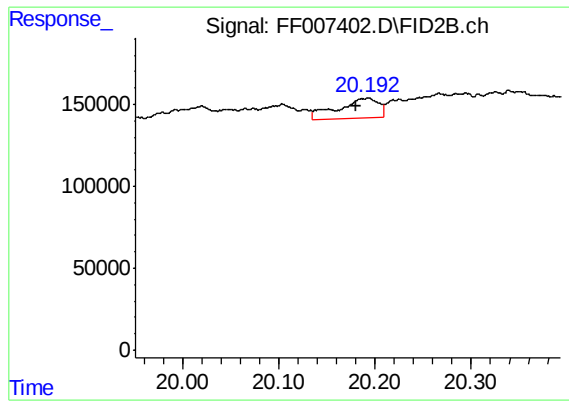

#16 N-HEXATRIACONTANE

R.T.: 20.191 min
Delta R.T.: 0.011 min
Response: 363365
Conc: 3.93 ug/ml

Instrument :
FID_F
ClientSampleId :
EROC-BF-1E