

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082120\
 Data File : FF007405.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2020 17:44
 Operator : DD\AJ
 Sample : L3734-04 20X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 EROC-BF-1C

Integration File: autoint1.e
 Quant Time: Aug 22 00:43:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	111790	0.819 ug/ml
Target Compounds			
7) N-EICOSANE	12.712f	135211	0.874 ug/ml
10) N-TETRACOSANE	14.938	105937	0.671 ug/ml
13) N-TRIACONTANE	17.819	143585	0.916 ug/ml
14) N-DOTRIACONTANE	18.656	152642	1.030 ug/ml
15) N-TETRATRIACONTANE	19.441	89617	0.741 ug/ml
16) N-HEXATRIACONTANE	20.217	271859	2.939 ug/ml
18) N-TETRACONTANE	21.923	472034	7.058 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082120\
Data File : FF007405.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2020 17:44
Operator : DD\AJ
Sample : L3734-04 20X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EROC-BF-1C

Integration File: autoint1.e
Quant Time: Aug 22 00:43:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

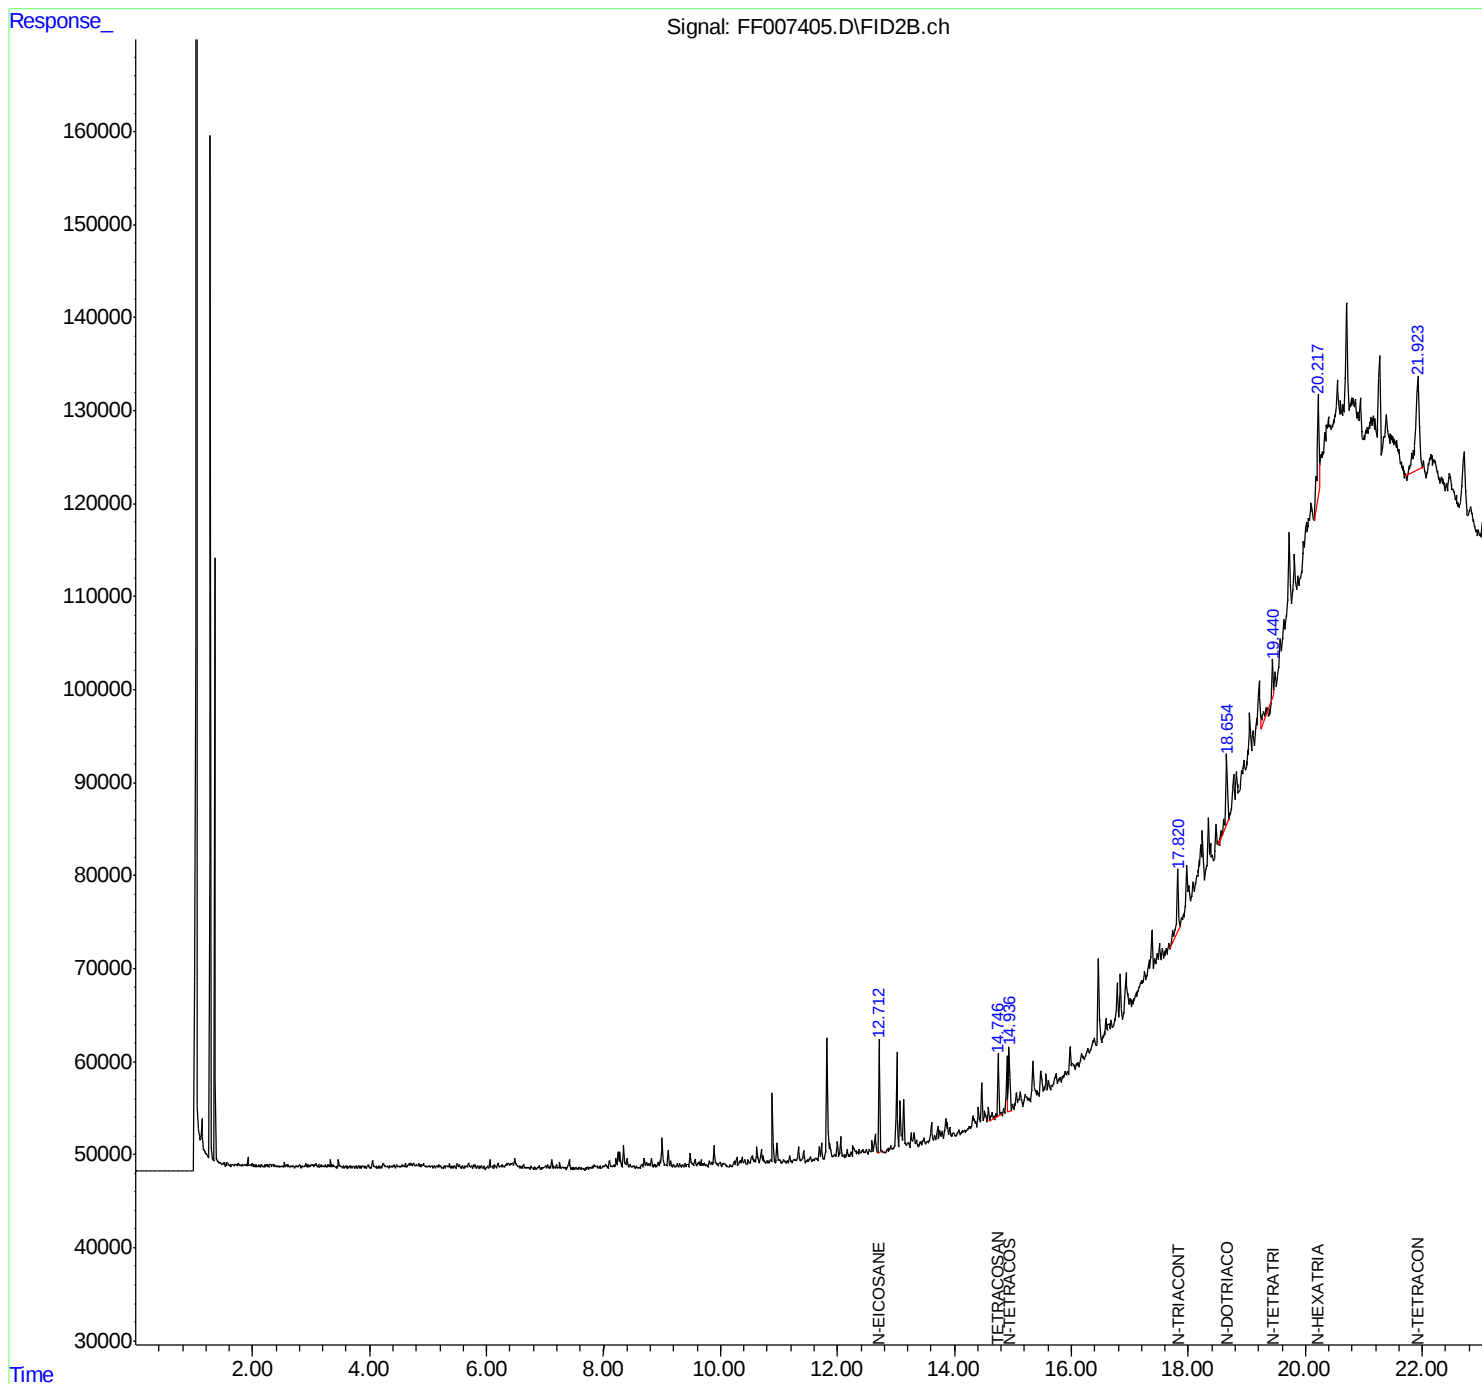


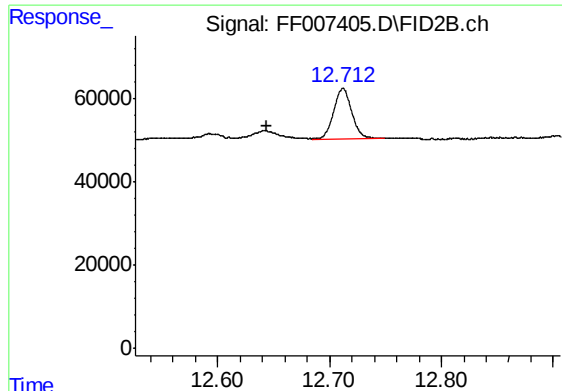

#7 N-EICOSANE


R.T.: 12.712 min
Delta R.T.: 0.068 min
Response: 135211
Conc: 0.87 ug/ml

Instrument :
FID_F
ClientSampleId :
EROC-BF-1C

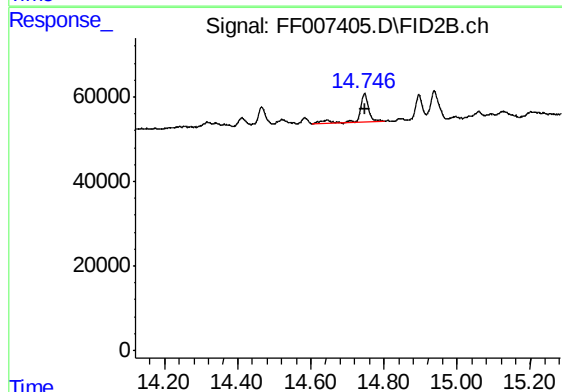


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min
Delta R.T.: -0.001 min
Response: 111790
Conc: 0.82 ug/ml

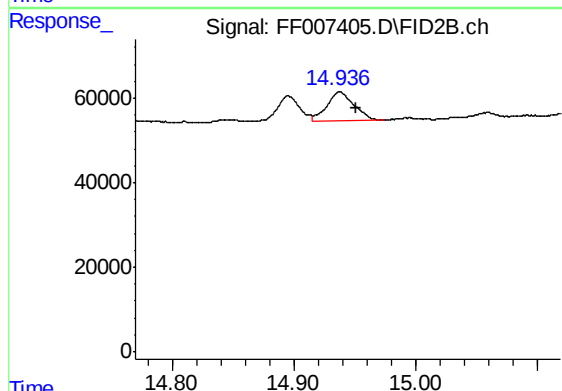


#10 N-TETRACOSANE

R.T.: 14.938 min
Delta R.T.: -0.014 min
Response: 105937
Conc: 0.67 ug/ml

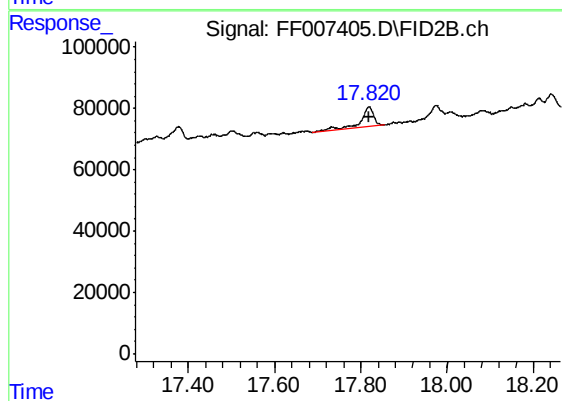

#13 N-TRIACONTANE


R.T.: 17.819 min
Delta R.T.: 0.001 min
Response: 143585
Conc: 0.92 ug/ml

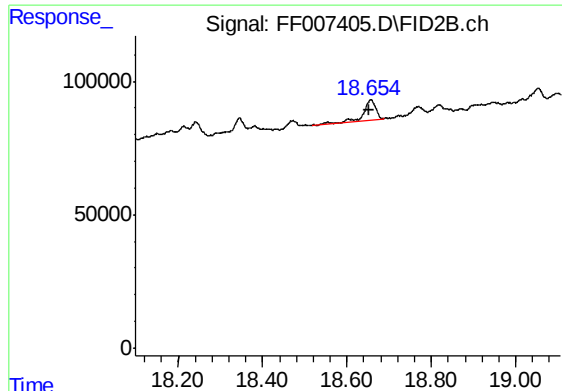

#14 N-DOTRIACONTANE


R.T.: 18.656 min
Delta R.T.: 0.004 min
Response: 152642
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :
EROC-BF-1C

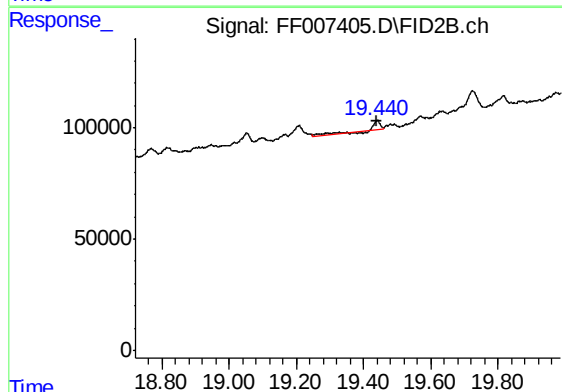


#15 N-TETRATRIACONTANE

R.T.: 19.441 min
Delta R.T.: 0.002 min
Response: 89617
Conc: 0.74 ug/ml

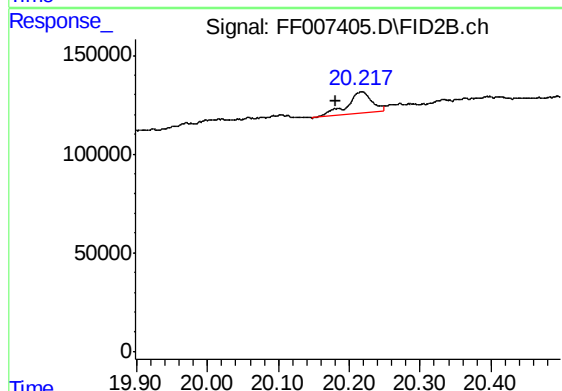

#16 N-HEXATRIACONTANE

R.T.: 20.217 min
Delta R.T.: 0.037 min
Response: 271859
Conc: 2.94 ug/ml

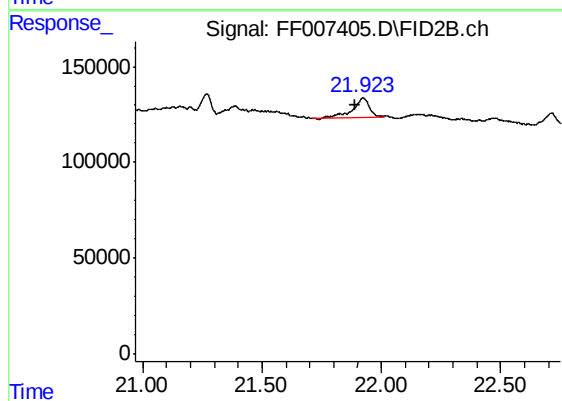

#18 N-TETRACONTANE

R.T.: 21.923 min
Delta R.T.: 0.036 min
Response: 472034
Conc: 7.06 ug/ml