

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082123AL\
 Data File : FF013228.D
 Signal(s) : FID2B.ch
 Acq On : 21 Aug 2023 09:35
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 22 01:32:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 10 16:05:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.870	19062	0.169 ug/ml
19) T n-Tetratriacontane (C34)	19.652	16234	0.153 ug/ml
20) T n-Hexatriacontane (C36)	20.390	21388	0.203 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082123AL\
Data File : FF013228.D
Signal(s) : FID2B.ch
Acq On : 21 Aug 2023 09:35
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:32:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

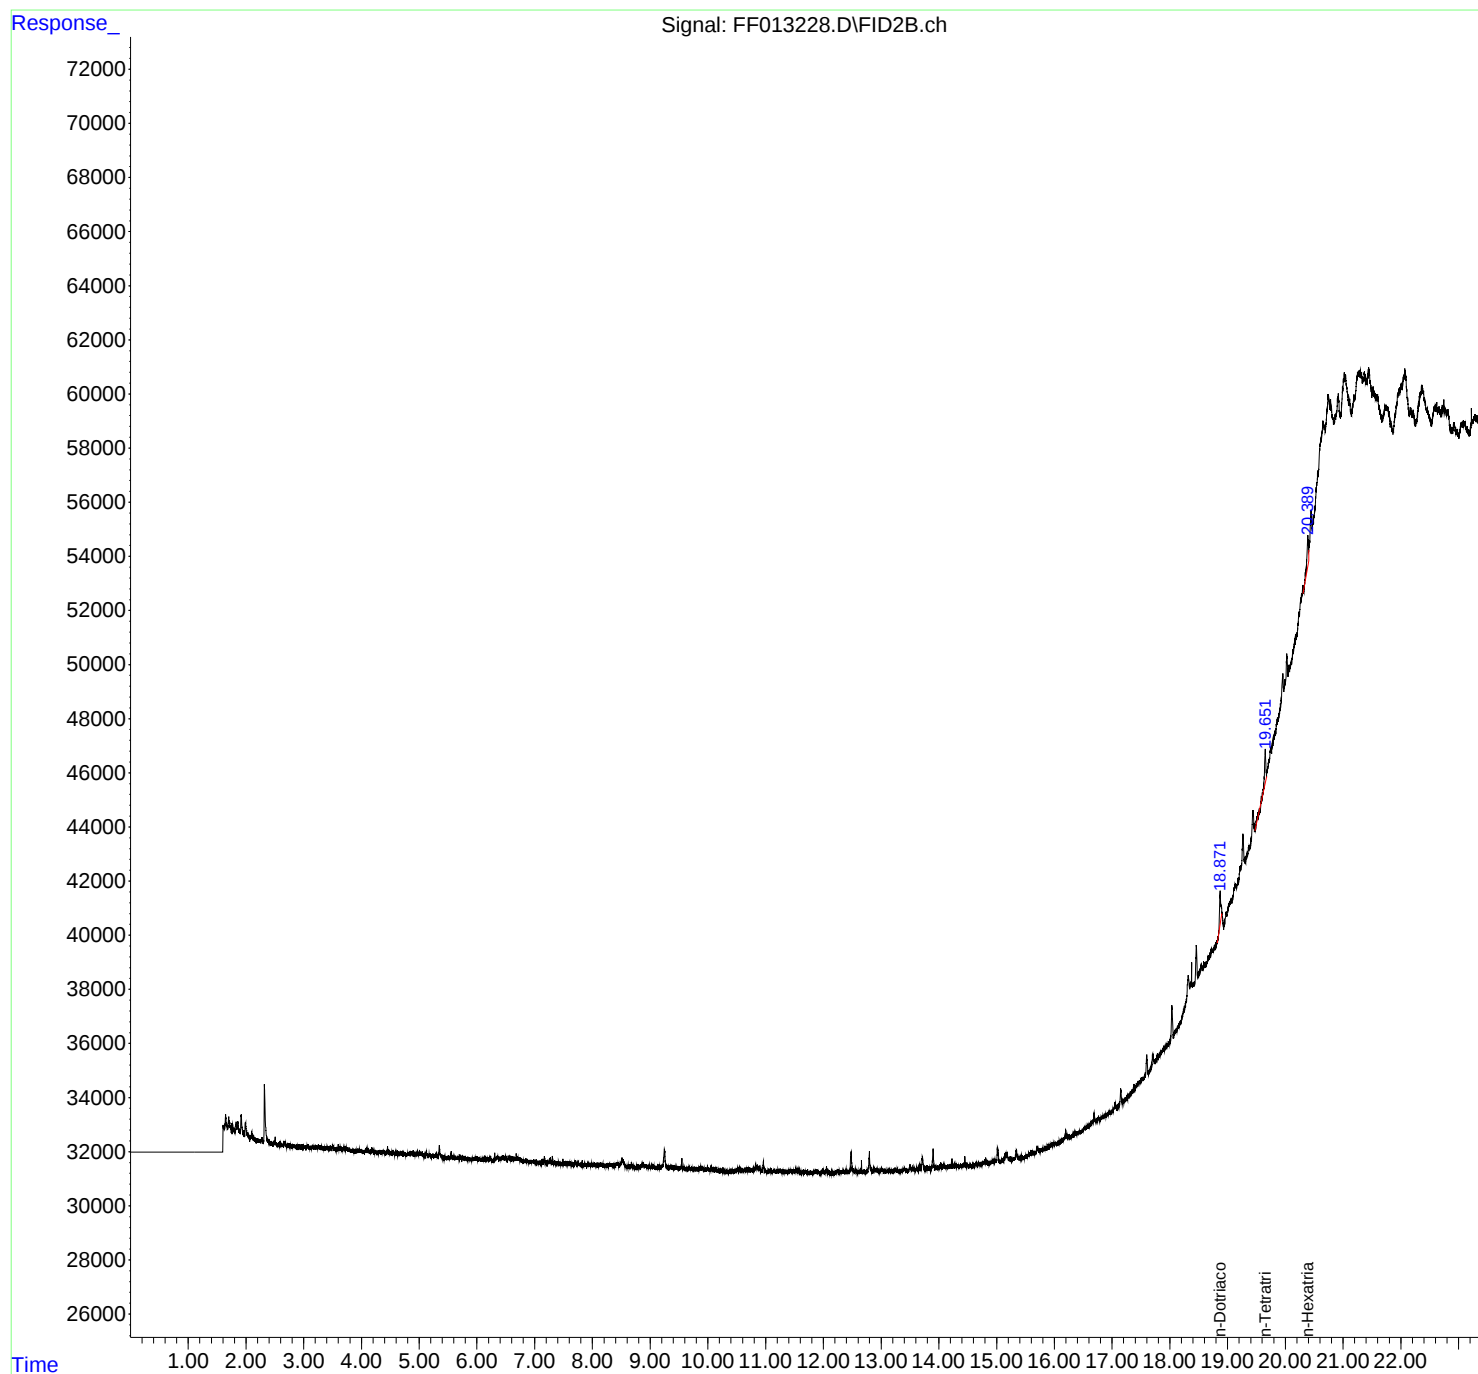


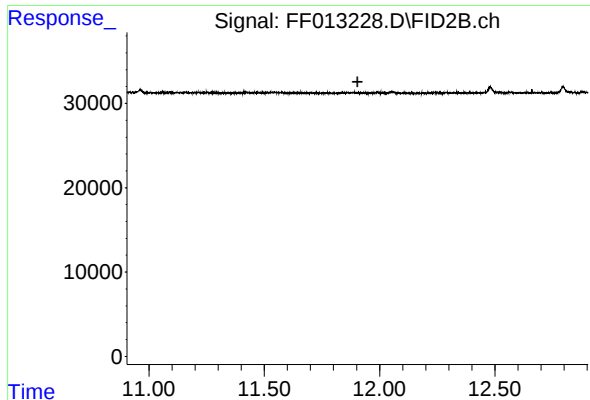

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.904 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

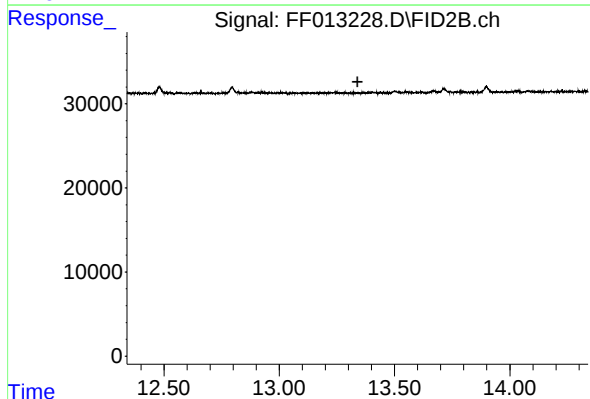


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.339 min
Response: 0
Conc: N.D.

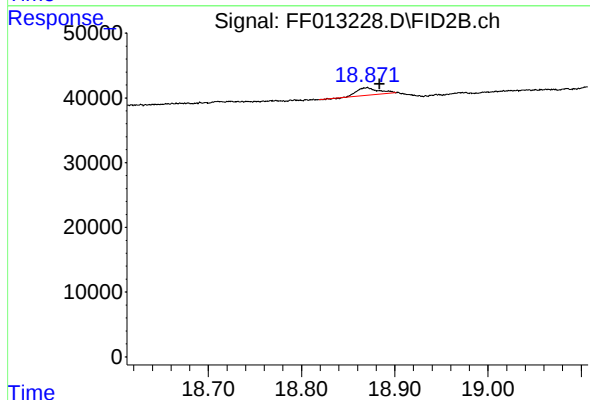


#18 n-Dotriacontane (C32)

R.T.: 18.870 min
Delta R.T.: -0.014 min
Response: 19062
Conc: 0.17 ug/ml

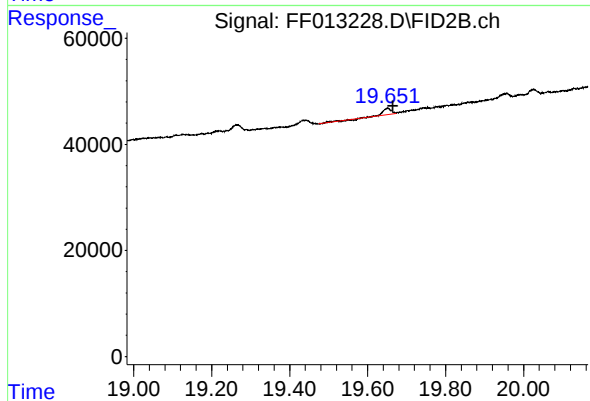

#19 n-Tetratriacontane (C34)

R.T.: 19.652 min
Delta R.T.: -0.014 min
Response: 16234
Conc: 0.15 ug/ml

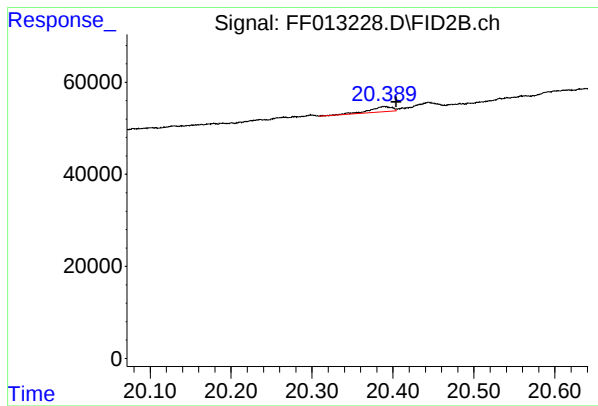

#20 n-Hexatriacontane (C36)

R.T.: 20.390 min
Delta R.T.: -0.014 min
Response: 21388
Conc: 0.20 ug/ml

Instrument :
FID_F
ClientSampleId :