

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
 Data File : FF001918.D
 Signal(s) : FID2B.ch
 Acq On : 22 Aug 2018 12:08
 Operator : AJ\SJ
 Sample : J4274-03 40X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 22 13:22:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.261f	506466	4.010 ug/ml
Target Compounds				
7)	N-EICOSANE	12.192	153546	1.030 ug/ml
8)	N-DOCOSANE	13.437	494373	3.385 ug/ml
10)	N-TETRACOSANE	14.491	3030427	21.243 ug/ml
12)	N-OCTACOSANE	16.509	593935	4.236 ug/ml
13)	N-TRIACONTANE	17.358	29334	0.212 ug/ml
14)	N-DOTRIACONTANE	18.195	724358	5.552 ug/ml
15)	N-TETRATRIACONTANE	18.967	133388	1.104 ug/ml
16)	N-HEXATRIACONTANE	19.690	334016	3.002 ug/ml
18)	N-TETRACONTANE	21.288f	41731	0.419 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
Data File : FF001918.D
Signal(s) : FID2B.ch
Acq On : 22 Aug 2018 12:08
Operator : AJ\SJ
Sample : J4274-03 40X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 22 13:22:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

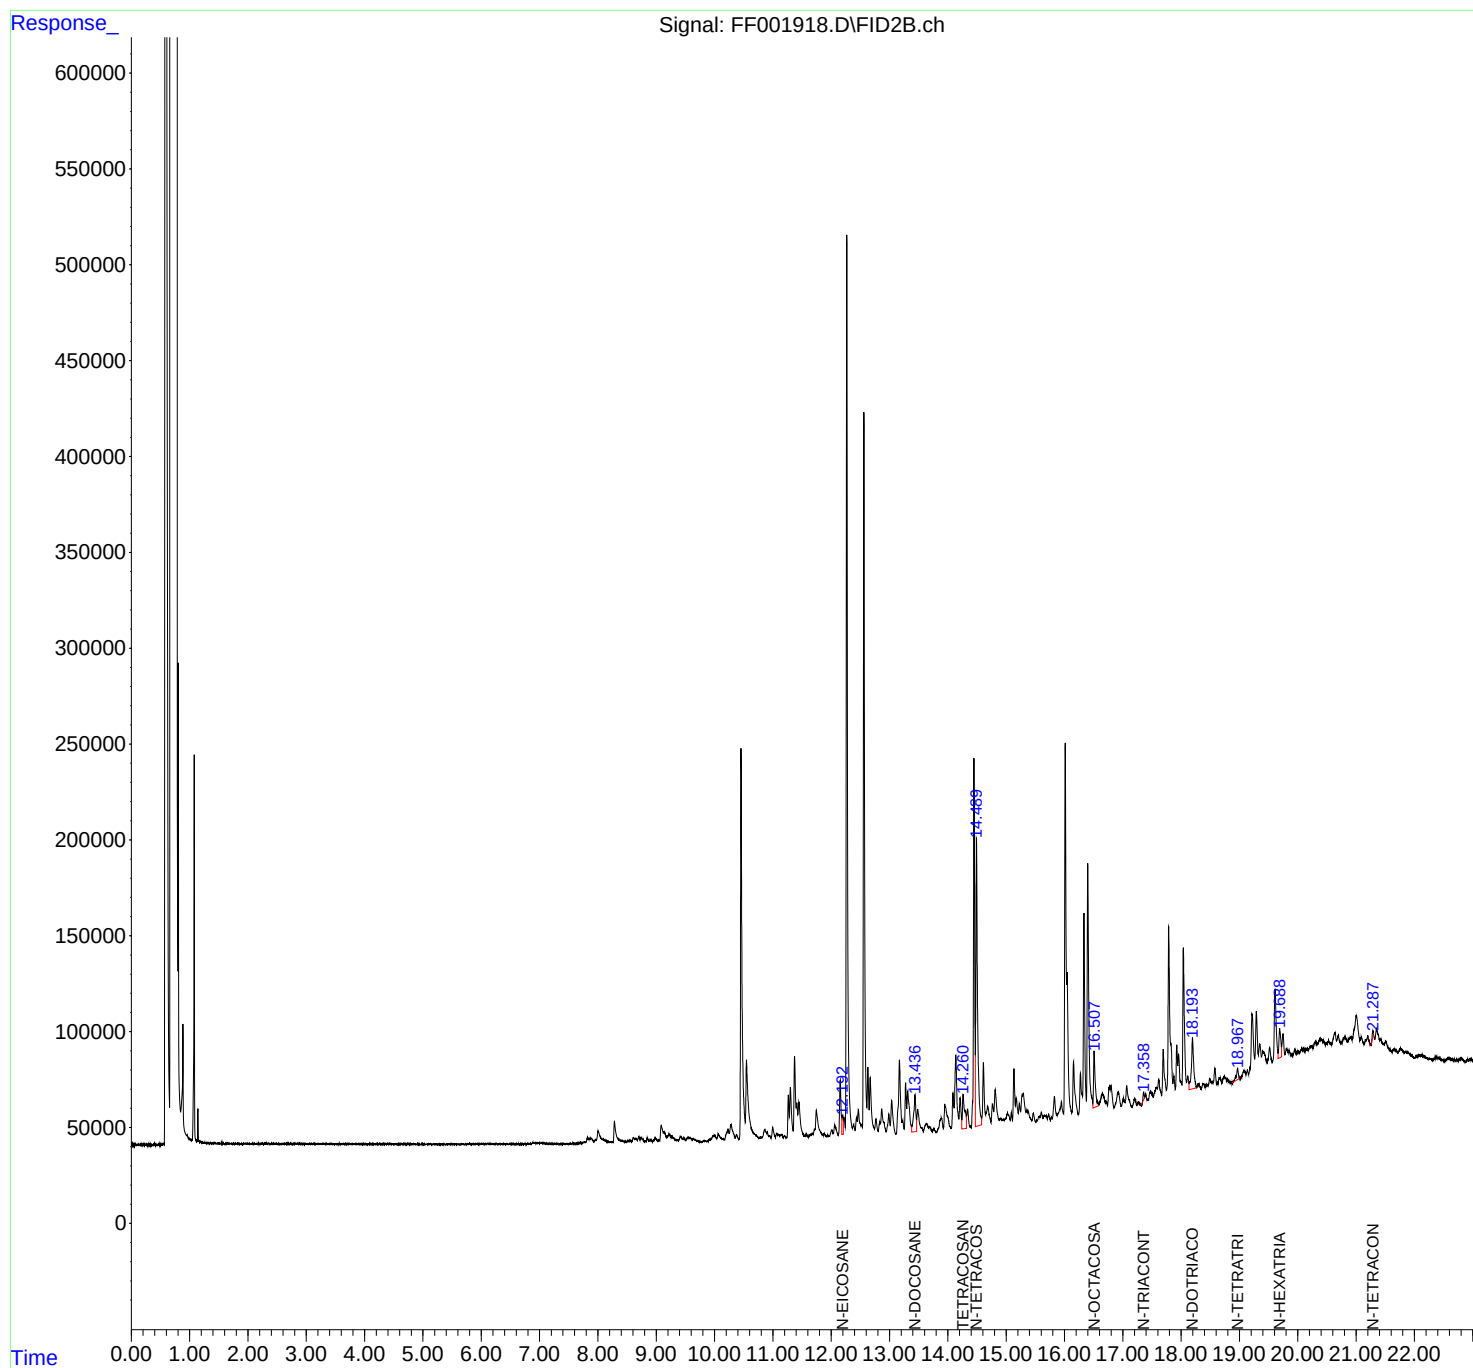

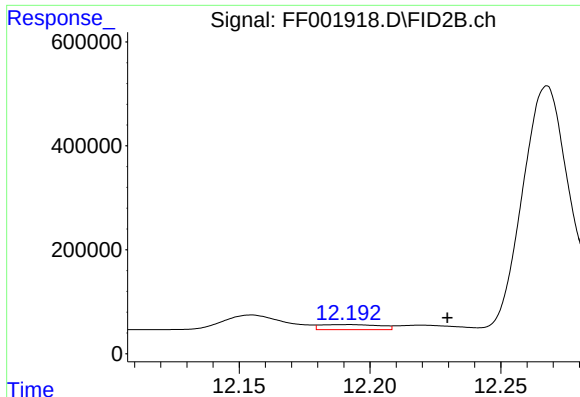


#7 N-EICOSANE

R.T.: 12.192 min
Delta R.T.: -0.038 min
Response: 153546
Conc: 1.03 ug/ml

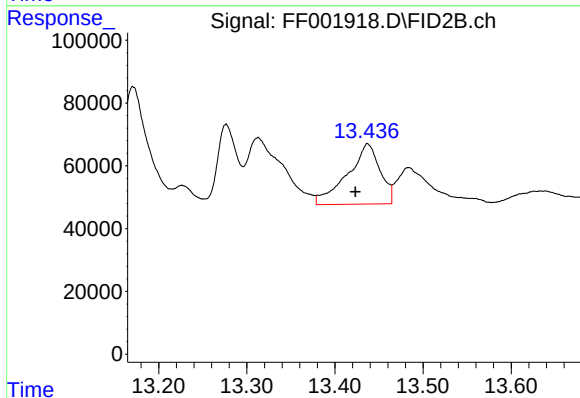


#8 N-DOCOSANE

R.T.: 13.437 min
Delta R.T.: 0.014 min
Response: 494373
Conc: 3.38 ug/ml

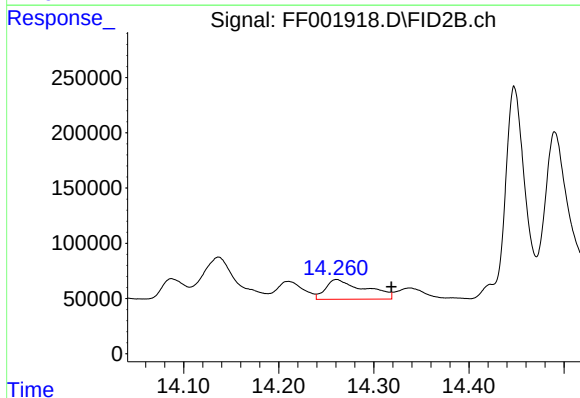


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.261 min
Delta R.T.: -0.057 min
Response: 506466
Conc: 4.01 ug/ml

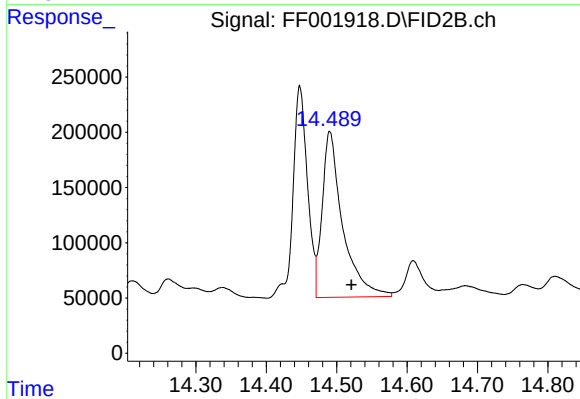


#10 N-TETRACOSANE

R.T.: 14.491 min
Delta R.T.: -0.030 min
Response: 3030427
Conc: 21.24 ug/ml

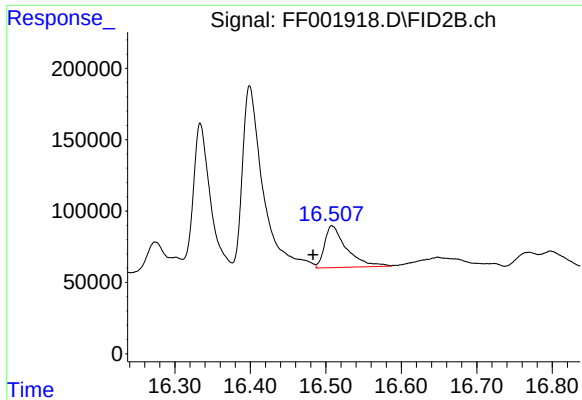


#12 N-OCTACOSANE

R.T.: 16.509 min
Delta R.T.: 0.025 min
Response: 593935
Conc: 4.24 ug/ml

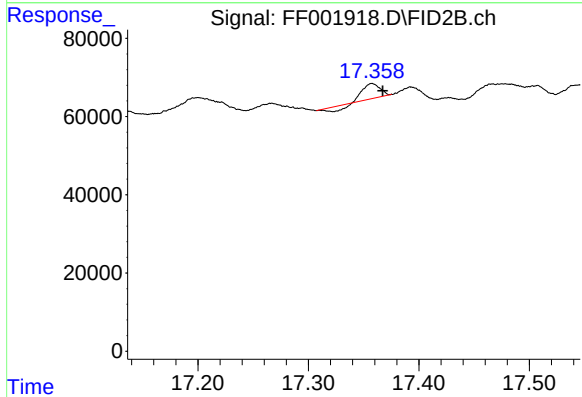


#13 N-TRIACONTANE

R.T.: 17.358 min
Delta R.T.: -0.010 min
Response: 29334
Conc: 0.21 ug/ml

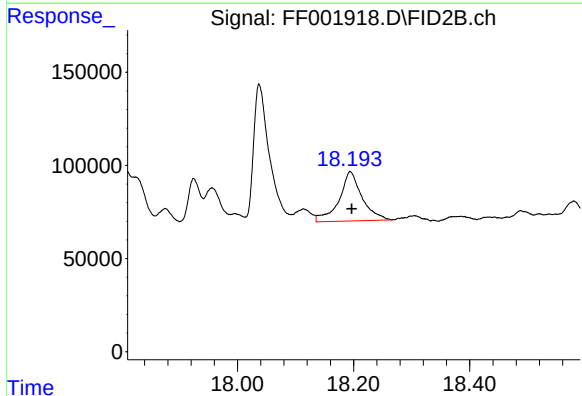


#14 N-DOTRIACONTANE

R.T.: 18.195 min
Delta R.T.: -0.002 min
Response: 724358
Conc: 5.55 ug/ml

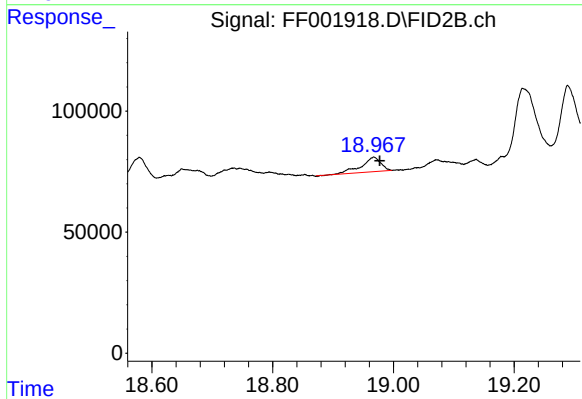


#15 N-TETRATRIACONTANE

R.T.: 18.967 min
Delta R.T.: -0.010 min
Response: 133388
Conc: 1.10 ug/ml

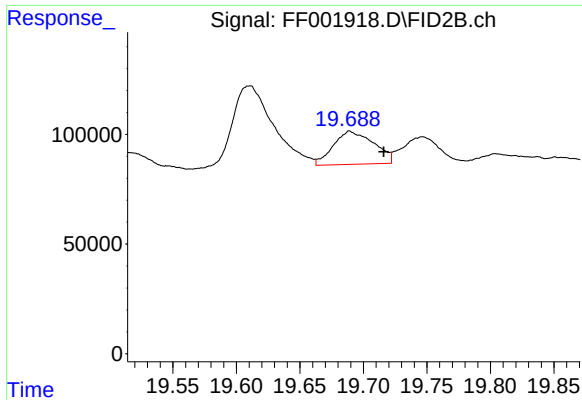

#16 N-HEXATRIACONTANE

R.T.: 19.690 min
Delta R.T.: -0.027 min
Response: 334016
Conc: 3.00 ug/ml

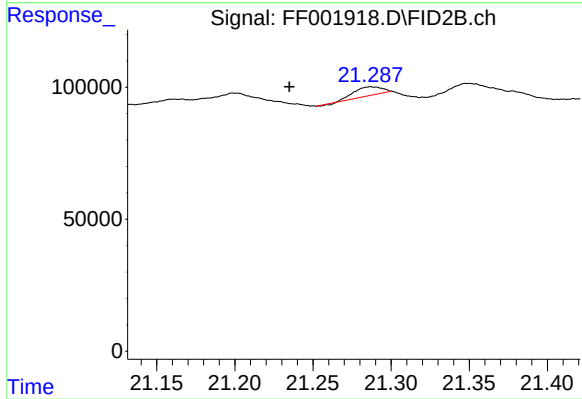

#18 N-TETRACONTANE

R.T.: 21.288 min
Delta R.T.: 0.053 min
Response: 41731
Conc: 0.42 ug/ml