

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
 Data File : FF001923.D
 Signal(s) : FID2B.ch
 Acq On : 22 Aug 2018 14:47
 Operator : AJ\SJ
 Sample : J4276-03 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 23 05:29:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.307	229190	1.815 ug/ml
Target Compounds				
7)	N-EICOSANE	12.218	201786	1.354 ug/ml
8)	N-DOCOSANE	13.440	175317	1.200 ug/ml
10)	N-TETRACOSANE	14.501	1120268	7.853 ug/ml
12)	N-OCTACOSANE	16.475	276536	1.972 ug/ml
13)	N-TRIACONTANE	17.362	320055	2.312 ug/ml
14)	N-DOTRIACONTANE	18.195	410958	3.150 ug/ml
15)	N-TETRATRIACONTANE	18.977	371422	3.073 ug/ml
16)	N-HEXATRIACONTANE	19.715	340363	3.059 ug/ml
17)	N-OCTATRIACONTANE	20.418	85893	0.862 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
Data File : FF001923.D
Signal(s) : FID2B.ch
Acq On : 22 Aug 2018 14:47
Operator : AJ\SJ
Sample : J4276-03 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 23 05:29:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

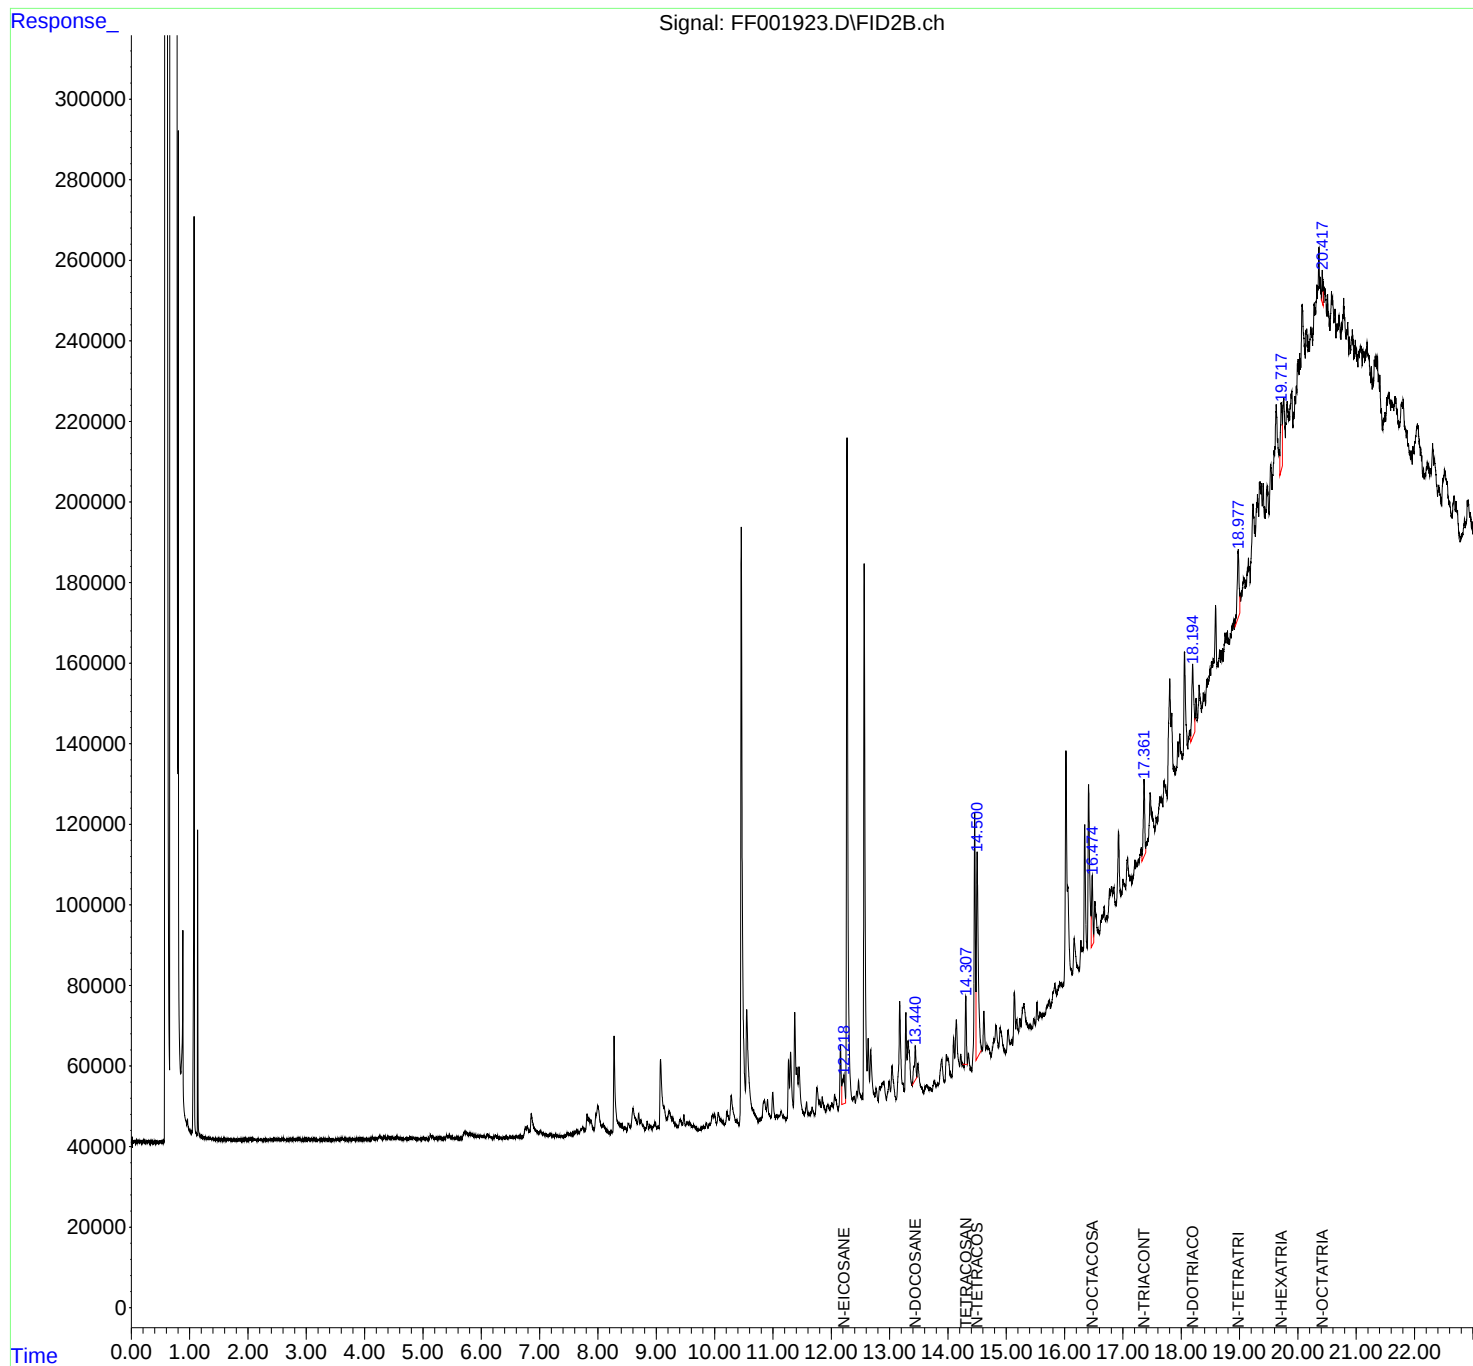

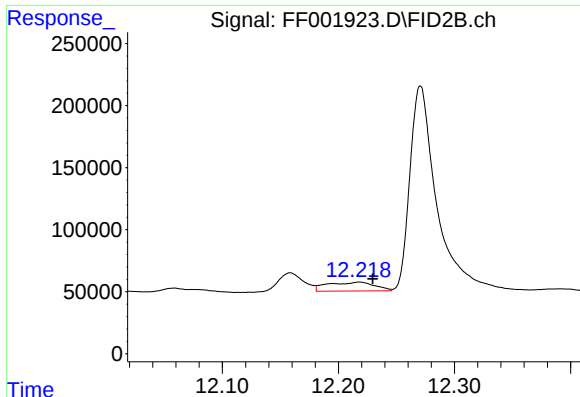


#7 N-EICOSANE

R.T.: 12.218 min
Delta R.T.: -0.012 min
Response: 201786
Conc: 1.35 ug/ml

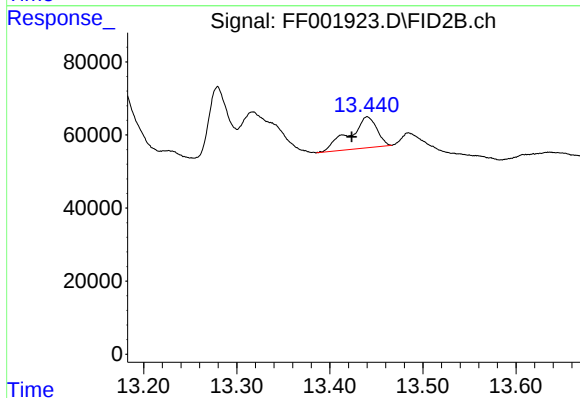


#8 N-DOCOSANE

R.T.: 13.440 min
Delta R.T.: 0.017 min
Response: 175317
Conc: 1.20 ug/ml

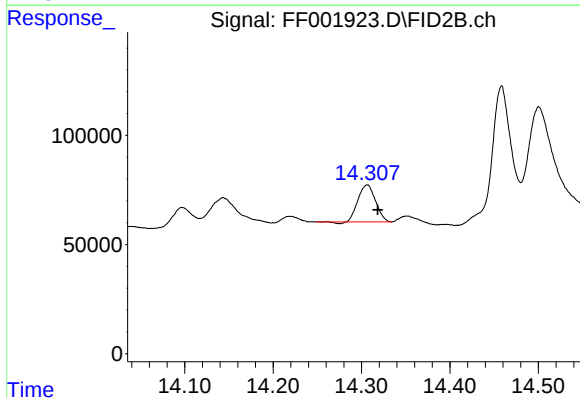


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.307 min
Delta R.T.: -0.012 min
Response: 229190
Conc: 1.81 ug/ml

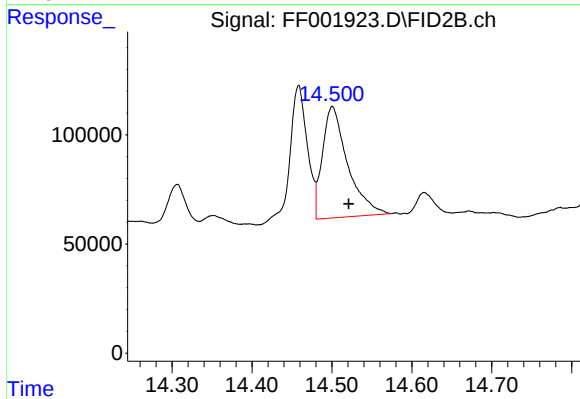


#10 N-TETRACOSANE

R.T.: 14.501 min
Delta R.T.: -0.020 min
Response: 1120268
Conc: 7.85 ug/ml

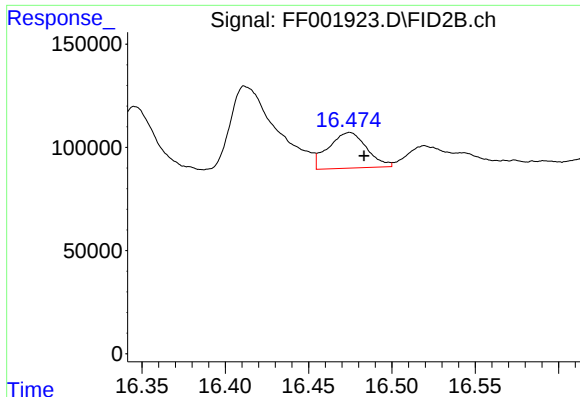


#12 N-OCTACOSANE

R.T.: 16.475 min
Delta R.T.: -0.009 min
Response: 276536
Conc: 1.97 ug/ml

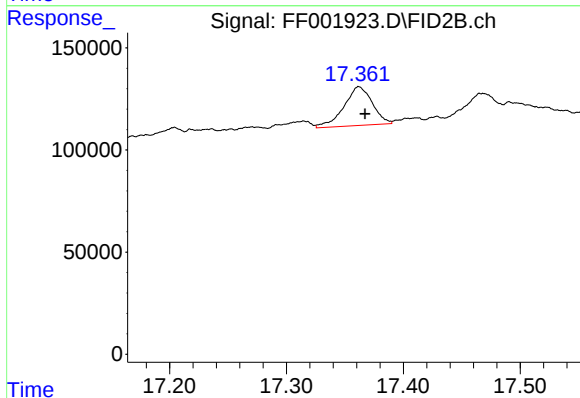


#13 N-TRIACONTANE

R.T.: 17.362 min
Delta R.T.: -0.005 min
Response: 320055
Conc: 2.31 ug/ml

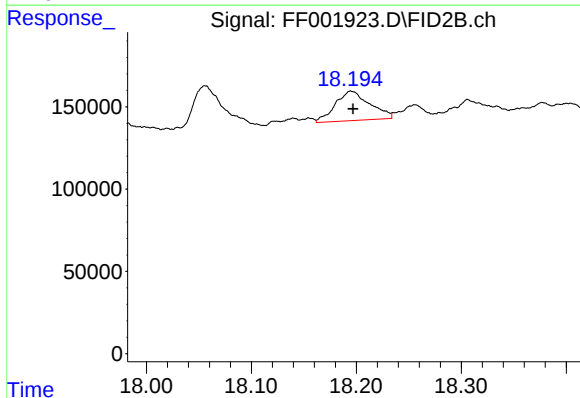


#14 N-DOTRIACONTANE

R.T.: 18.195 min
Delta R.T.: -0.002 min
Response: 410958
Conc: 3.15 ug/ml

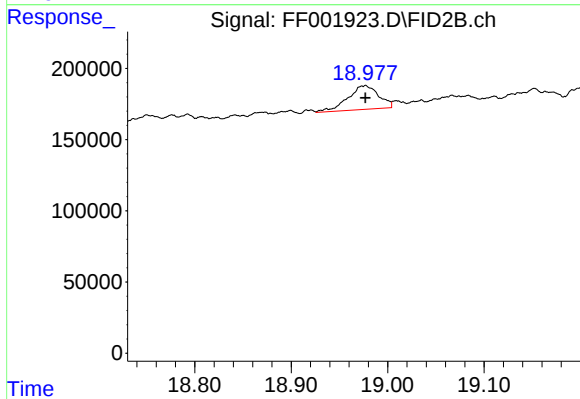


#15 N-TETRATRIACONTANE

R.T.: 18.977 min
Delta R.T.: 0.000 min
Response: 371422
Conc: 3.07 ug/ml

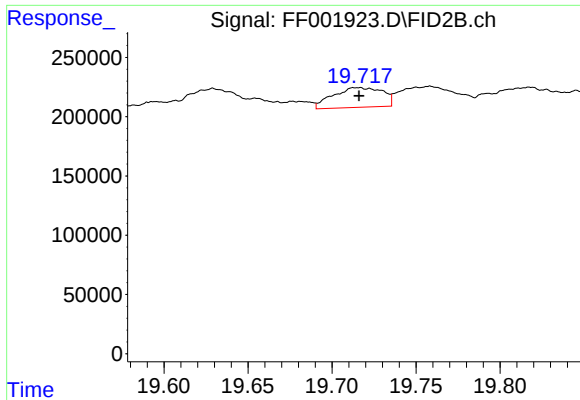

#16 N-HEXATRIACONTANE

R.T.: 19.715 min
Delta R.T.: -0.001 min
Response: 340363
Conc: 3.06 ug/ml

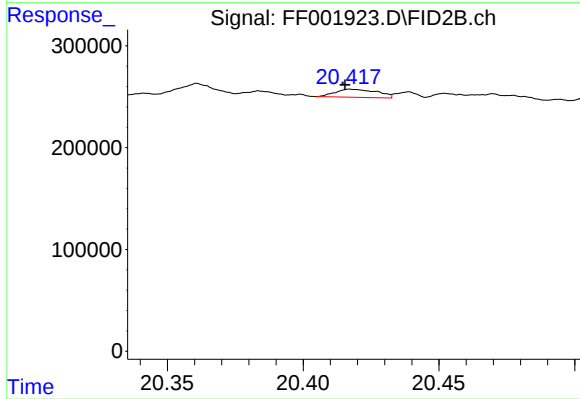

#17 N-OCTATRIACONTANE

R.T.: 20.418 min
Delta R.T.: 0.002 min
Response: 85893
Conc: 0.86 ug/ml