

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
Data File : FF001928.D
Signal(s) : FID2B.ch
Acq On : 22 Aug 2018 17:20
Operator : AJ\SJ
Sample : J4278-11 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 23 05:30:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.306	166966	1.322 ug/ml
Target Compounds				
12)	N-OCTACOSANE	16.473	112038	0.799 ug/ml
14)	N-DOTRIACONTANE	18.191	149217	1.144 ug/ml
15)	N-TETRATRIACONTANE	18.974	169215	1.400 ug/ml
16)	N-HEXATRIACONTANE	19.714	85728	0.770 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
Data File : FF001928.D
Signal(s) : FID2B.ch
Acq On : 22 Aug 2018 17:20
Operator : AJ\SJ
Sample : J4278-11 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 23 05:30:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

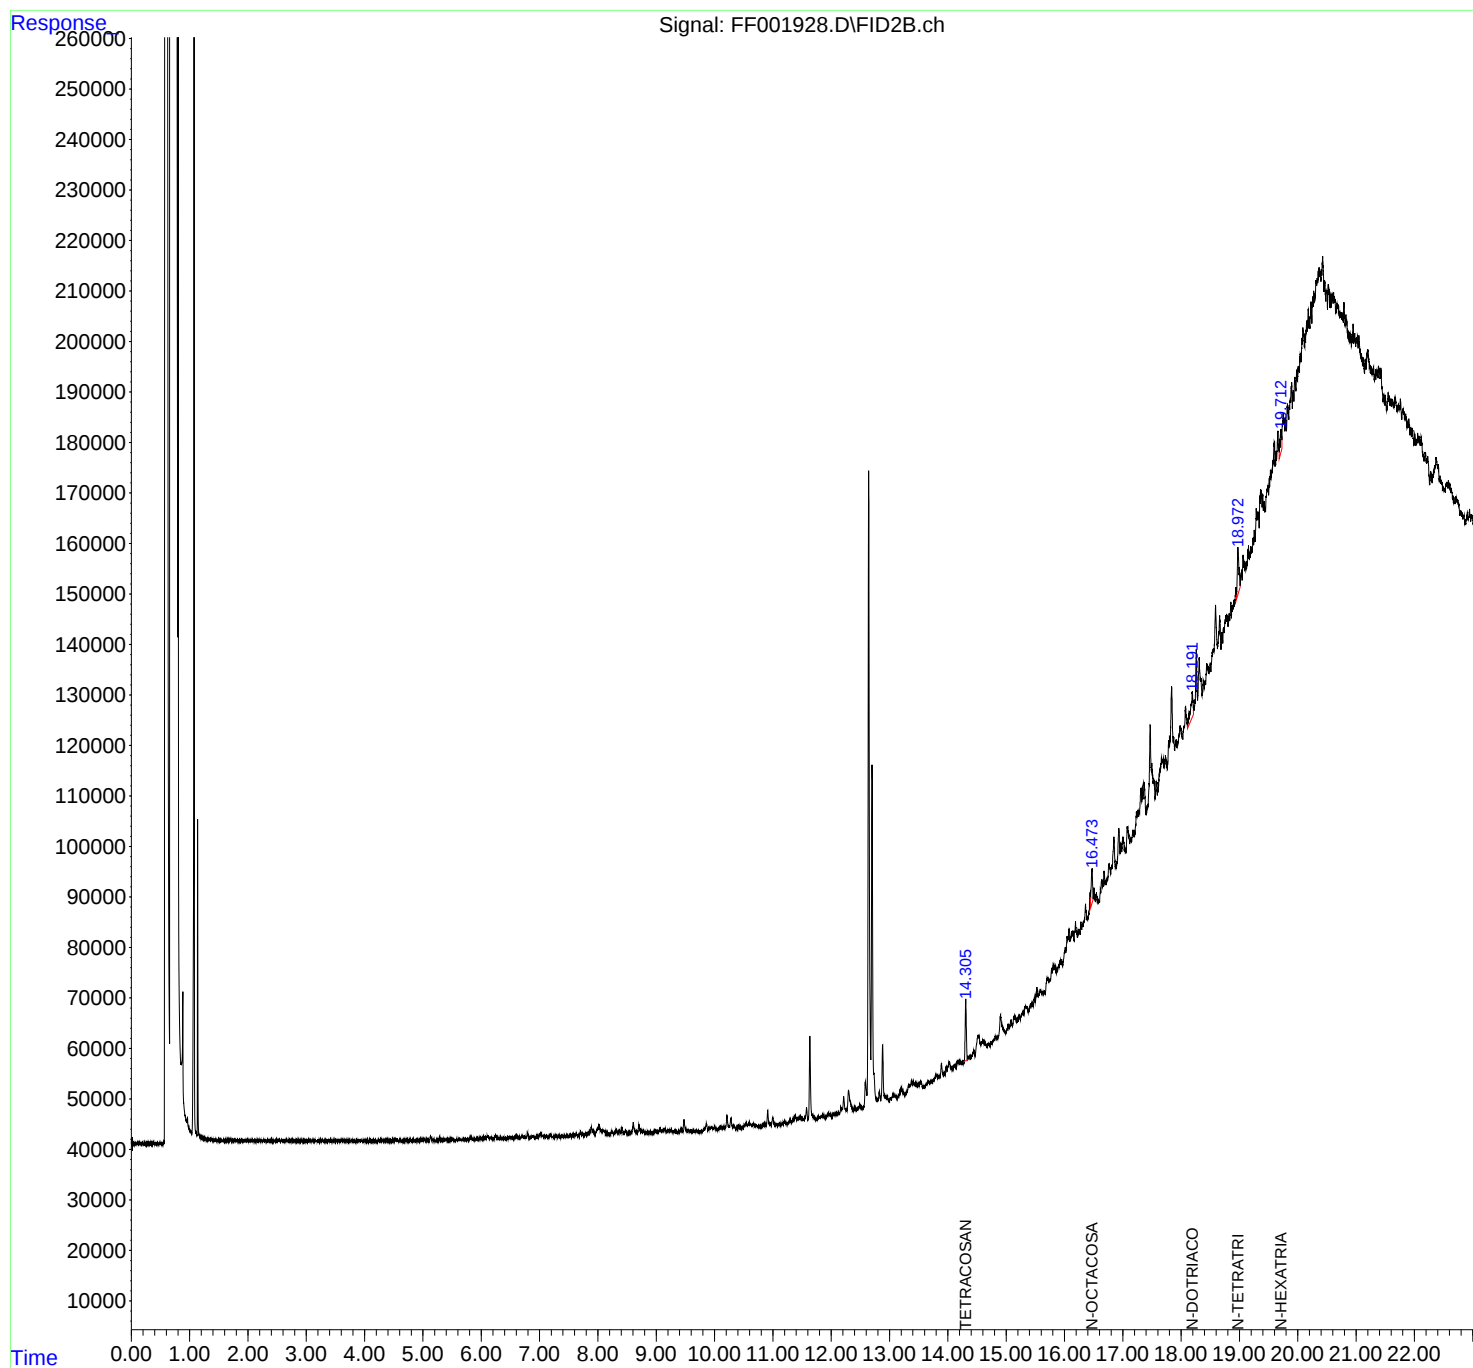

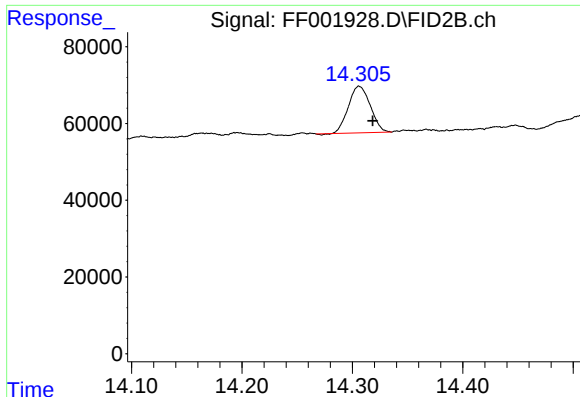


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.306 min
Delta R.T.: -0.012 min
Response: 166966
Conc: 1.32 ug/ml

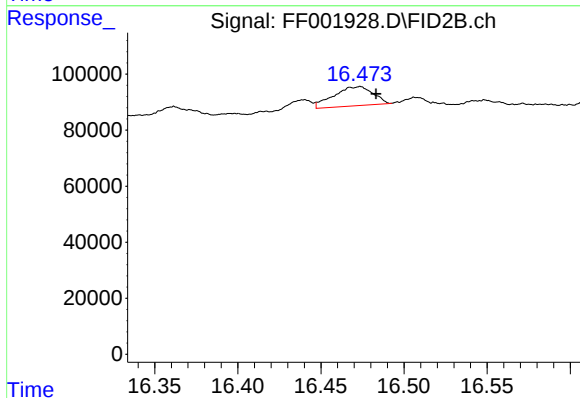


#12 N-OCTACOSANE

R.T.: 16.473 min
Delta R.T.: -0.010 min
Response: 112038
Conc: 0.80 ug/ml

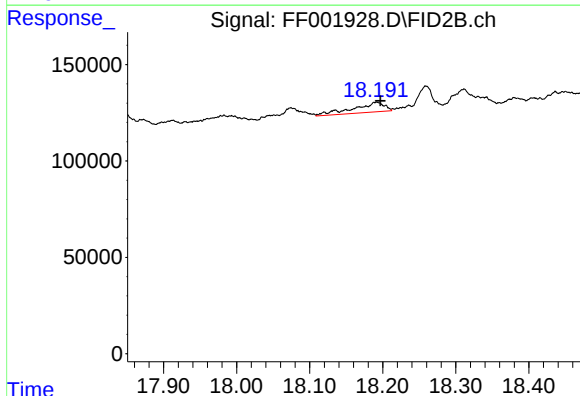


#14 N-DOTRIACONTANE

R.T.: 18.191 min
Delta R.T.: -0.005 min
Response: 149217
Conc: 1.14 ug/ml

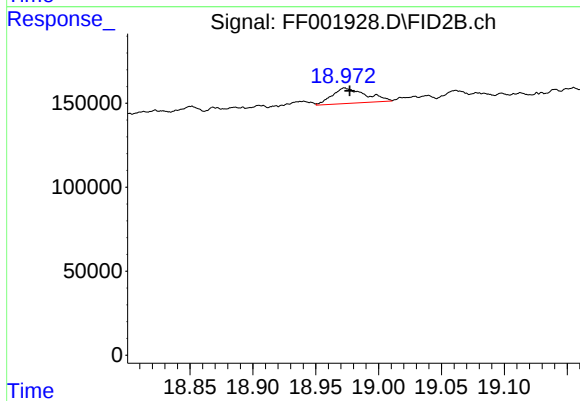

#15 N-TETRATRIACONTANE

R.T.: 18.974 min
Delta R.T.: -0.003 min
Response: 169215
Conc: 1.40 ug/ml

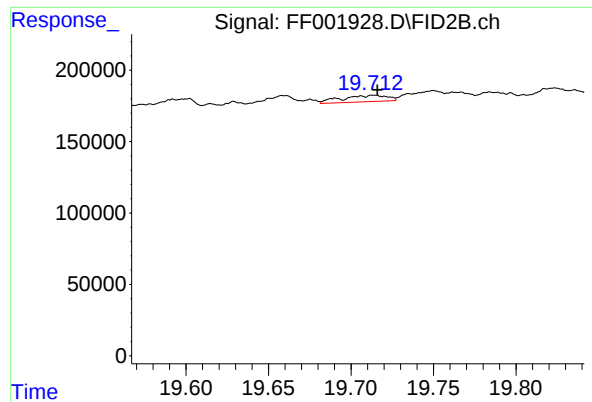

#16 N-HEXATRIACONTANE

R.T.: 19.714 min
Delta R.T.: -0.002 min
Response: 85728
Conc: 0.77 ug/ml