

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
 Data File : FF001915.D
 Signal(s) : FID2B.ch
 Acq On : 22 Aug 2018 10:36
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 22 13:22:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.306	6807299	53.897 ug/ml
Target Compounds			
2) N-DECANE	4.091	7377421	50.588 ug/ml
3) N-DODECANE	6.098	7713648	51.748 ug/ml
4) N-TETRADECANE	7.882	7866168	52.191 ug/ml
5) N-HEXADECANE	9.474	7926841	52.950 ug/ml
6) N-OCTADECANE	10.911	7951171	52.753 ug/ml
7) N-EICOSANE	12.215	7866523	52.780 ug/ml
8) N-DOCOSANE	13.408	7785054	53.298 ug/ml
10) N-TETRACOSANE	14.508	7653576	53.652 ug/ml
11) N-HEXACOSANE	15.526	7553797	53.625 ug/ml
12) N-OCTACOSANE	16.473	7467319	53.255 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082218\
Data File : FF001915.D
Signal(s) : FID2B.ch
Acq On : 22 Aug 2018 10:36
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 22 13:22:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

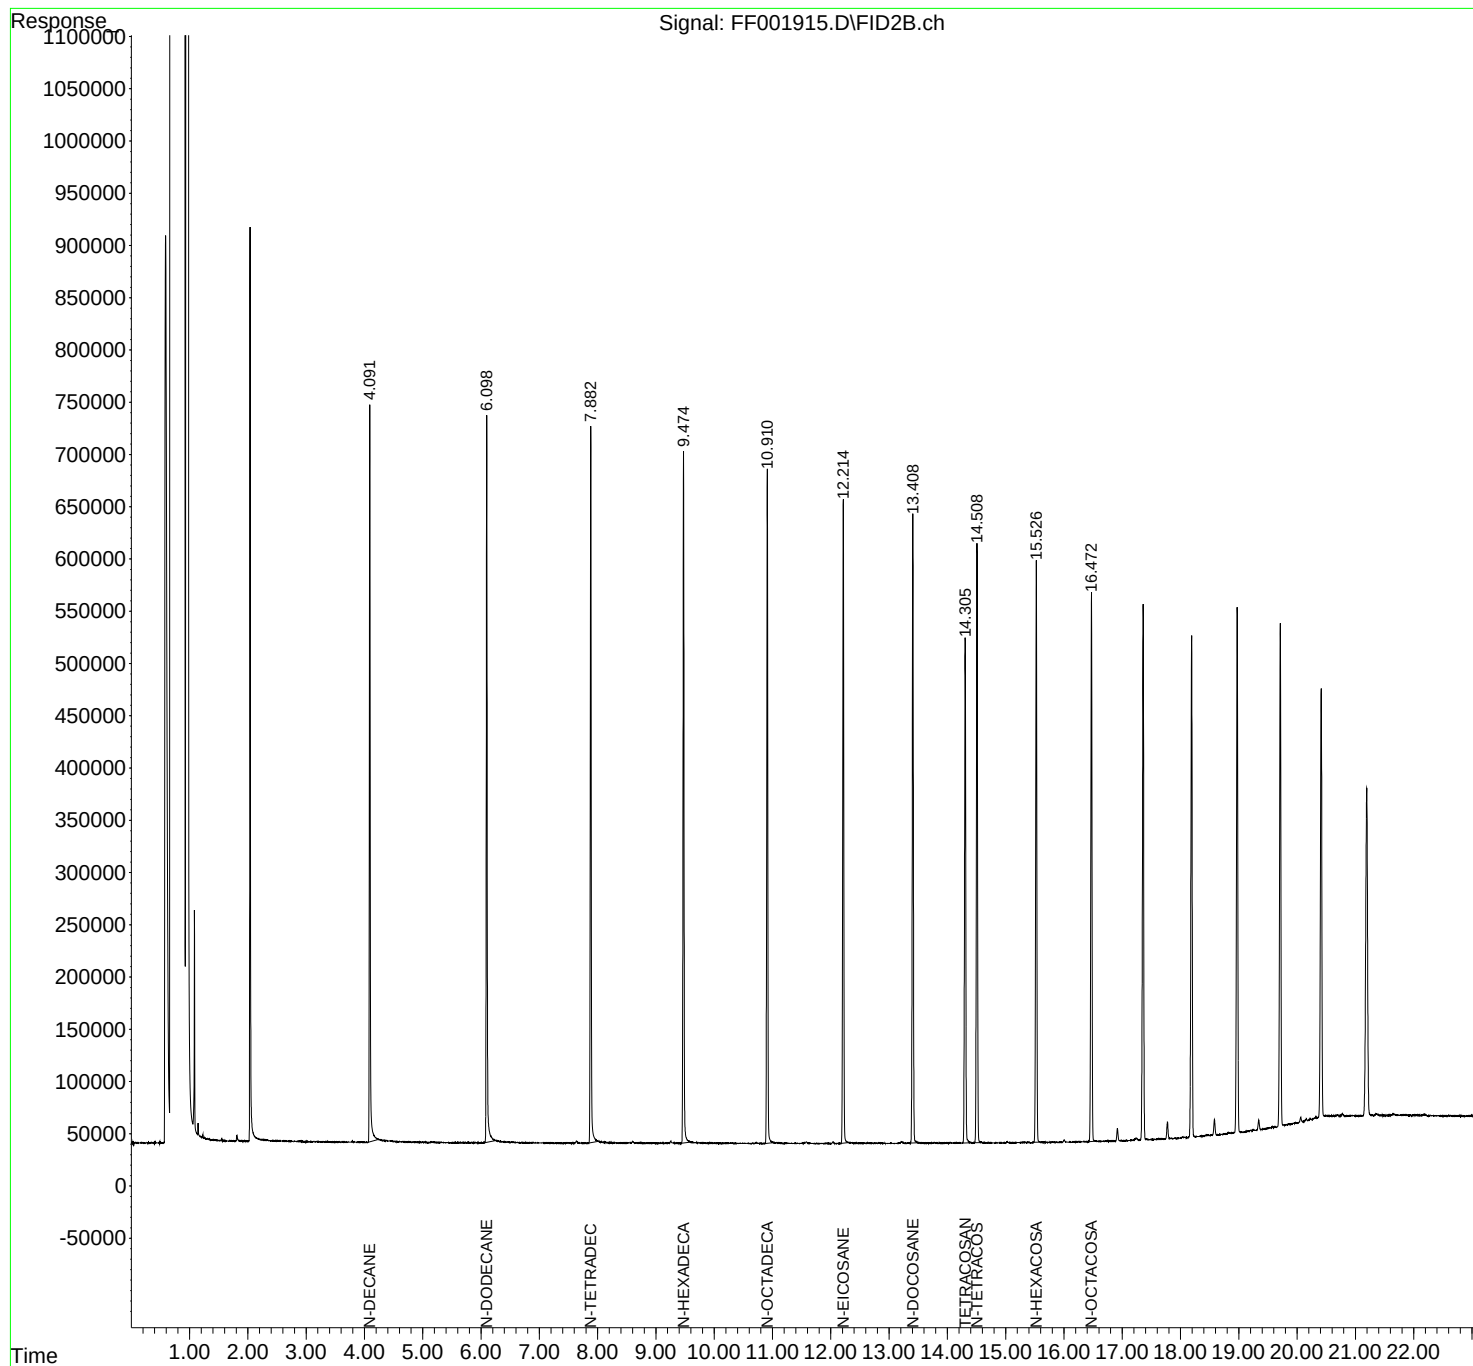

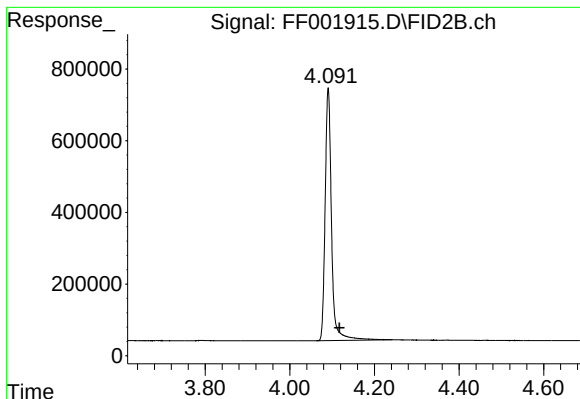


#2 N-DECANE

R.T.: 4.091 min
Delta R.T.: -0.026 min
Response: 7377421
Conc: 50.59 ug/ml

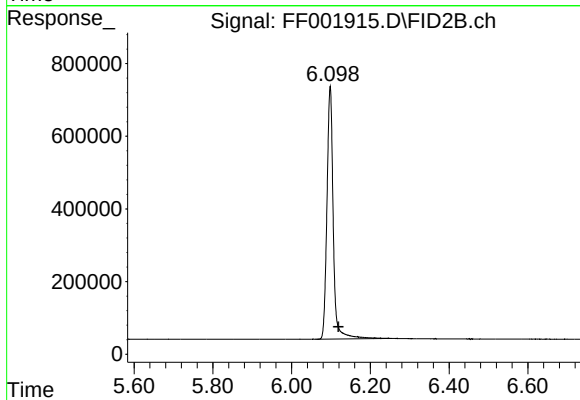


#3 N-DODECANE

R.T.: 6.098 min
Delta R.T.: -0.021 min
Response: 7713648
Conc: 51.75 ug/ml

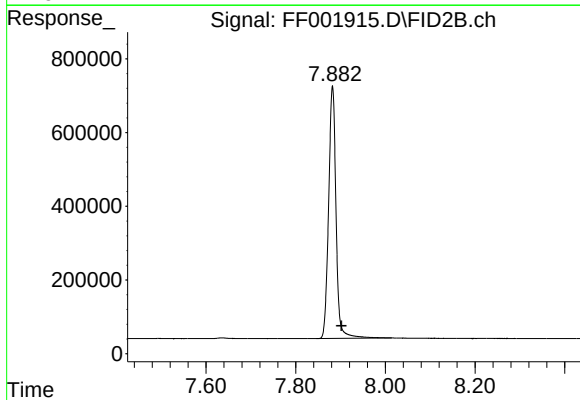


#4 N-TETRADECANE

R.T.: 7.882 min
Delta R.T.: -0.020 min
Response: 7866168
Conc: 52.19 ug/ml

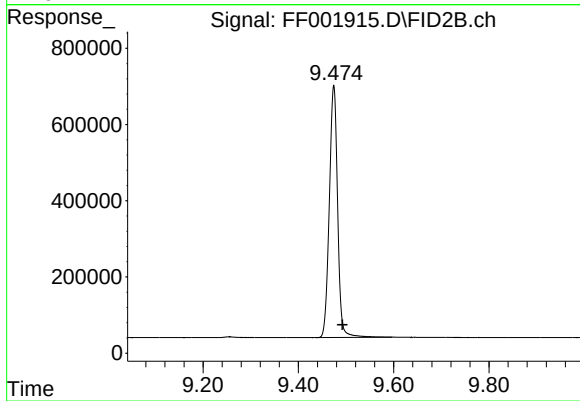


#5 N-HEXADECANE

R.T.: 9.474 min
Delta R.T.: -0.018 min
Response: 7926841
Conc: 52.95 ug/ml

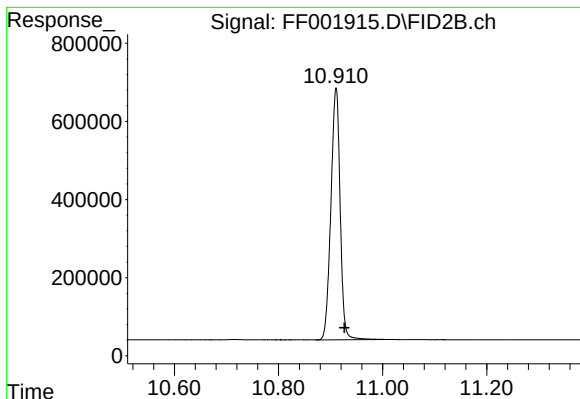


#6 N-OCTADECANE

R.T.: 10.911 min
Delta R.T.: -0.016 min
Response: 7951171
Conc: 52.75 ug/ml

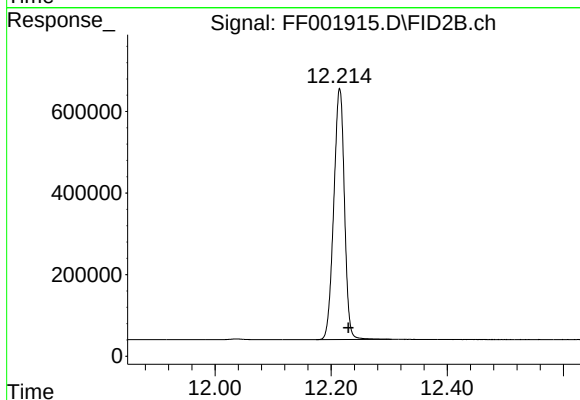


#7 N-EICOSANE

R.T.: 12.215 min
Delta R.T.: -0.015 min
Response: 7866523
Conc: 52.78 ug/ml

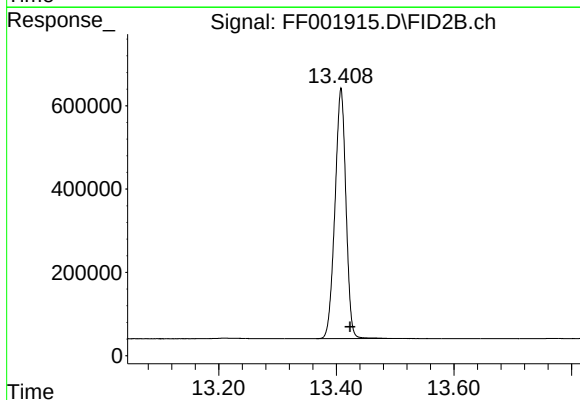


#8 N-DOCOSANE

R.T.: 13.408 min
Delta R.T.: -0.015 min
Response: 7785054
Conc: 53.30 ug/ml

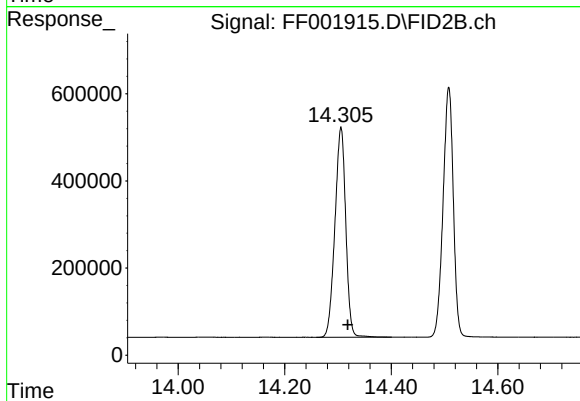


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.306 min
Delta R.T.: -0.013 min
Response: 6807299
Conc: 53.90 ug/ml

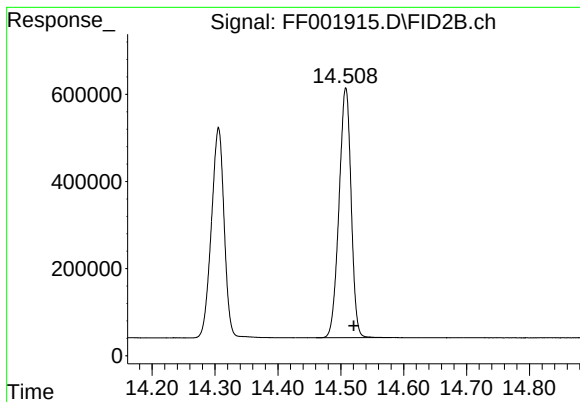


#10 N-TETRACOSANE

R.T.: 14.508 min
Delta R.T.: -0.013 min
Response: 7653576
Conc: 53.65 ug/ml

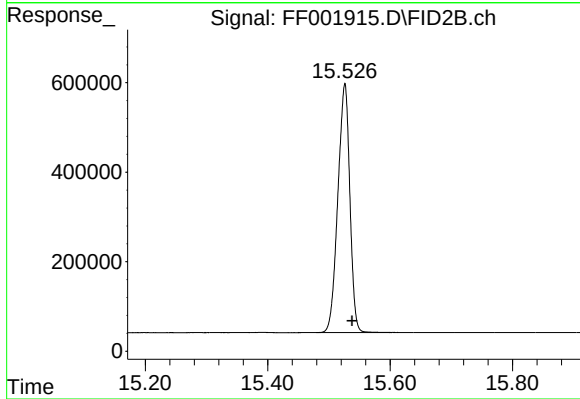

#11 N-HEXACOSANE

R.T.: 15.526 min
Delta R.T.: -0.012 min
Response: 7553797
Conc: 53.62 ug/ml

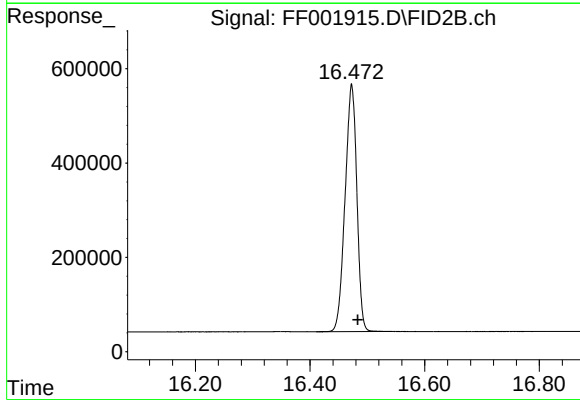

#12 N-OCTACOSANE

R.T.: 16.473 min
Delta R.T.: -0.011 min
Response: 7467319
Conc: 53.26 ug/ml