

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082222AL\
Data File : FF011291.D
Signal(s) : FID2B.ch
Acq On : 22 Aug 2022 22:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 23 03:05:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 03:03:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	16.849	30579	0.296 ug/ml
18) T	n-Dotriacontane (C32)	17.679	47376	0.560 ug/ml
19) T	n-Tetratriacontane (C34)	18.458	36186	0.585 ug/ml
20) T	n-Hexatriacontane (C36)	19.196	26433	0.565 ug/ml
21) T	n-Octatriacontane (C38)	19.900	29668	0.738 ug/ml
22) T	n-Tetracontane (C40)	20.718	58009	1.514 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082222AL\
Data File : FF011291.D
Signal(s) : FID2B.ch
Acq On : 22 Aug 2022 22:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 23 03:05:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 03:03:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

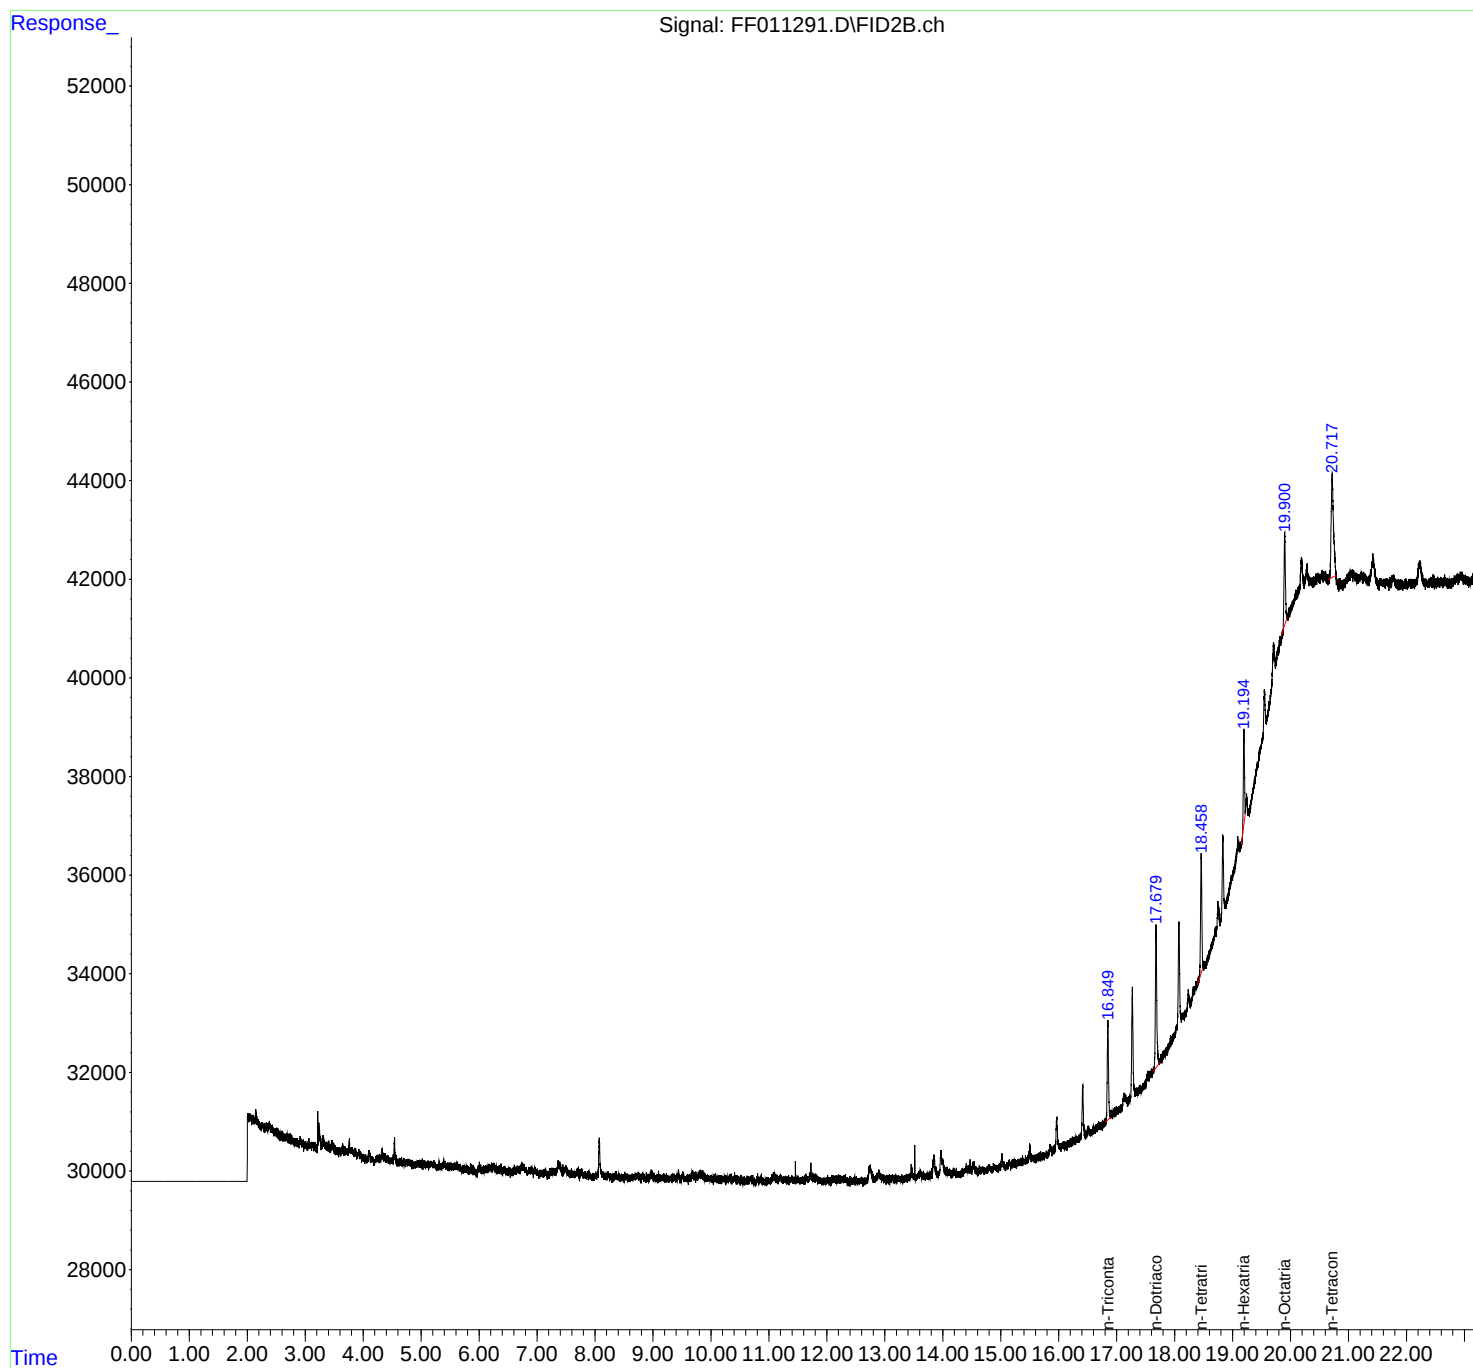


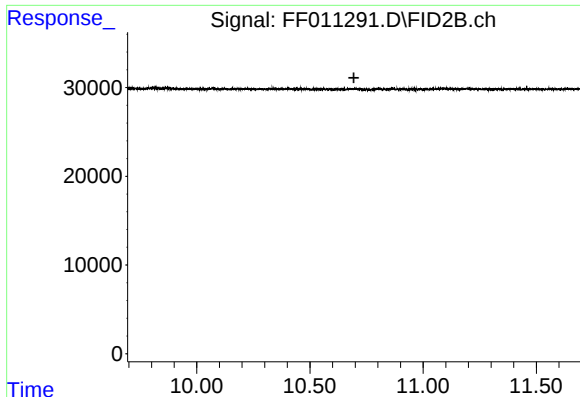

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.694 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

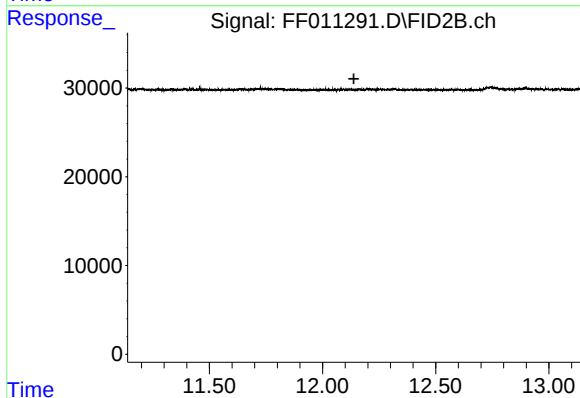


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.138 min
Response: 0
Conc: N.D.

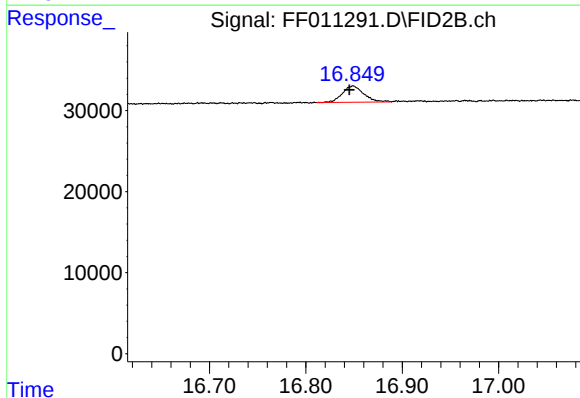


#17 n-Tricontane (C30)

R.T.: 16.849 min
Delta R.T.: 0.004 min
Response: 30579
Conc: 0.30 ug/ml

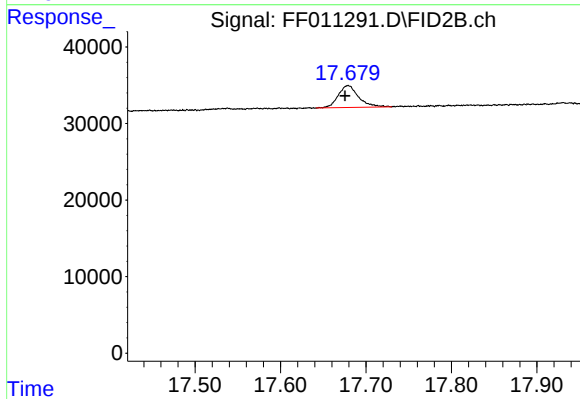

#18 n-Dotriacontane (C32)


R.T.: 17.679 min
Delta R.T.: 0.003 min
Response: 47376
Conc: 0.56 ug/ml

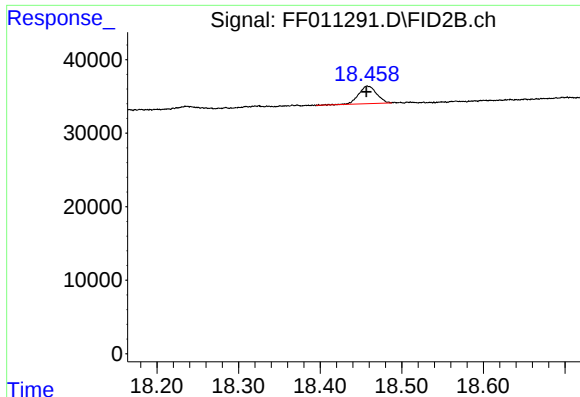

#19 n-Tetratriacontane (C34)


R.T.: 18.458 min
Delta R.T.: 0.000 min
Response: 36186
Conc: 0.58 ug/ml

Instrument :
FID_F
ClientSampleId :

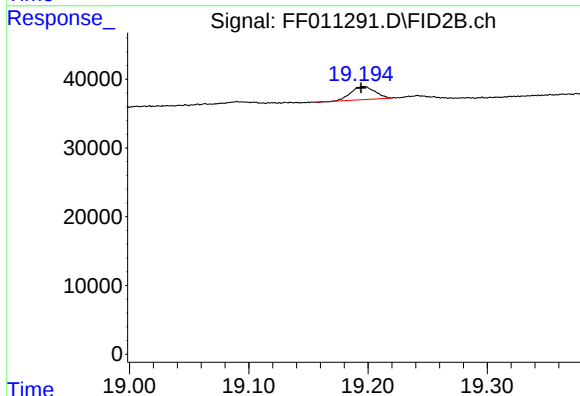


#20 n-Hexatriacontane (C36)

R.T.: 19.196 min
Delta R.T.: 0.002 min
Response: 26433
Conc: 0.56 ug/ml

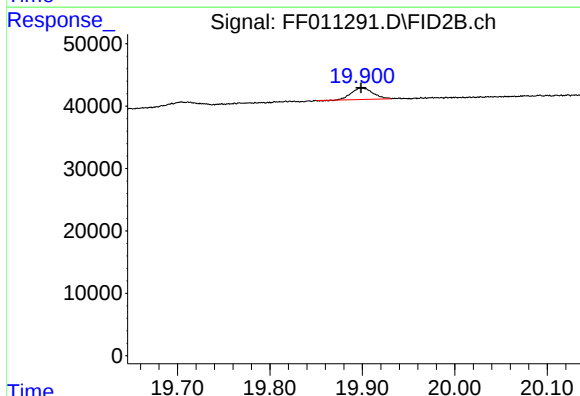

#21 n-Octatriacontane (C38)

R.T.: 19.900 min
Delta R.T.: 0.001 min
Response: 29668
Conc: 0.74 ug/ml

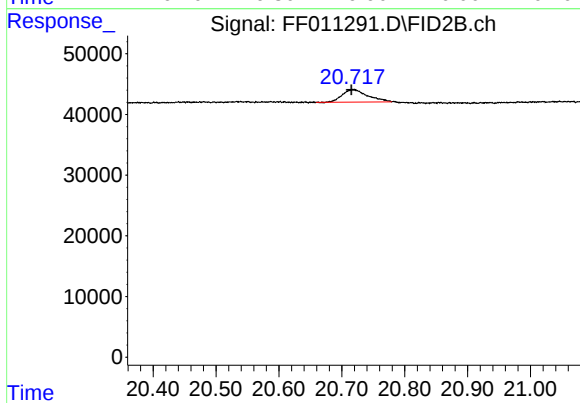

#22 n-Tetracontane (C40)

R.T.: 20.718 min
Delta R.T.: 0.003 min
Response: 58009
Conc: 1.51 ug/ml