

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082323AL\
 Data File : FF013300.D
 Signal(s) : FID2B.ch
 Acq On : 23 Aug 2023 08:27
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 24 01:08:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 10 16:05:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.846	122427	1.116 ug/ml
11) T n-Heneicosane (C21)	13.482	130015	1.183 ug/ml
13) T n-Docosane (C22)	14.072	125333	1.142 ug/ml
14) T n-Tetracosane (C24)	15.177	63179	0.575 ug/ml
15) T n-Hexacosane (C26)	16.199	69459	0.636 ug/ml
16) T n-Octacosane (C28)	17.148	82330	0.763 ug/ml
17) T n-Tricontane (C30)	18.036	89530	0.819 ug/ml
18) T n-Dotriacontane (C32)	18.864	172801	1.530 ug/ml
19) T n-Tetratriacontane (C34)	19.651	84814	0.798 ug/ml
20) T n-Hexatriacontane (C36)	20.390	144583	1.372 ug/ml
22) T n-Tetracontane (C40)	22.005	23468	0.236 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082323AL\
Data File : FF013300.D
Signal(s) : FID2B.ch
Acq On : 23 Aug 2023 08:27
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 24 01:08:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

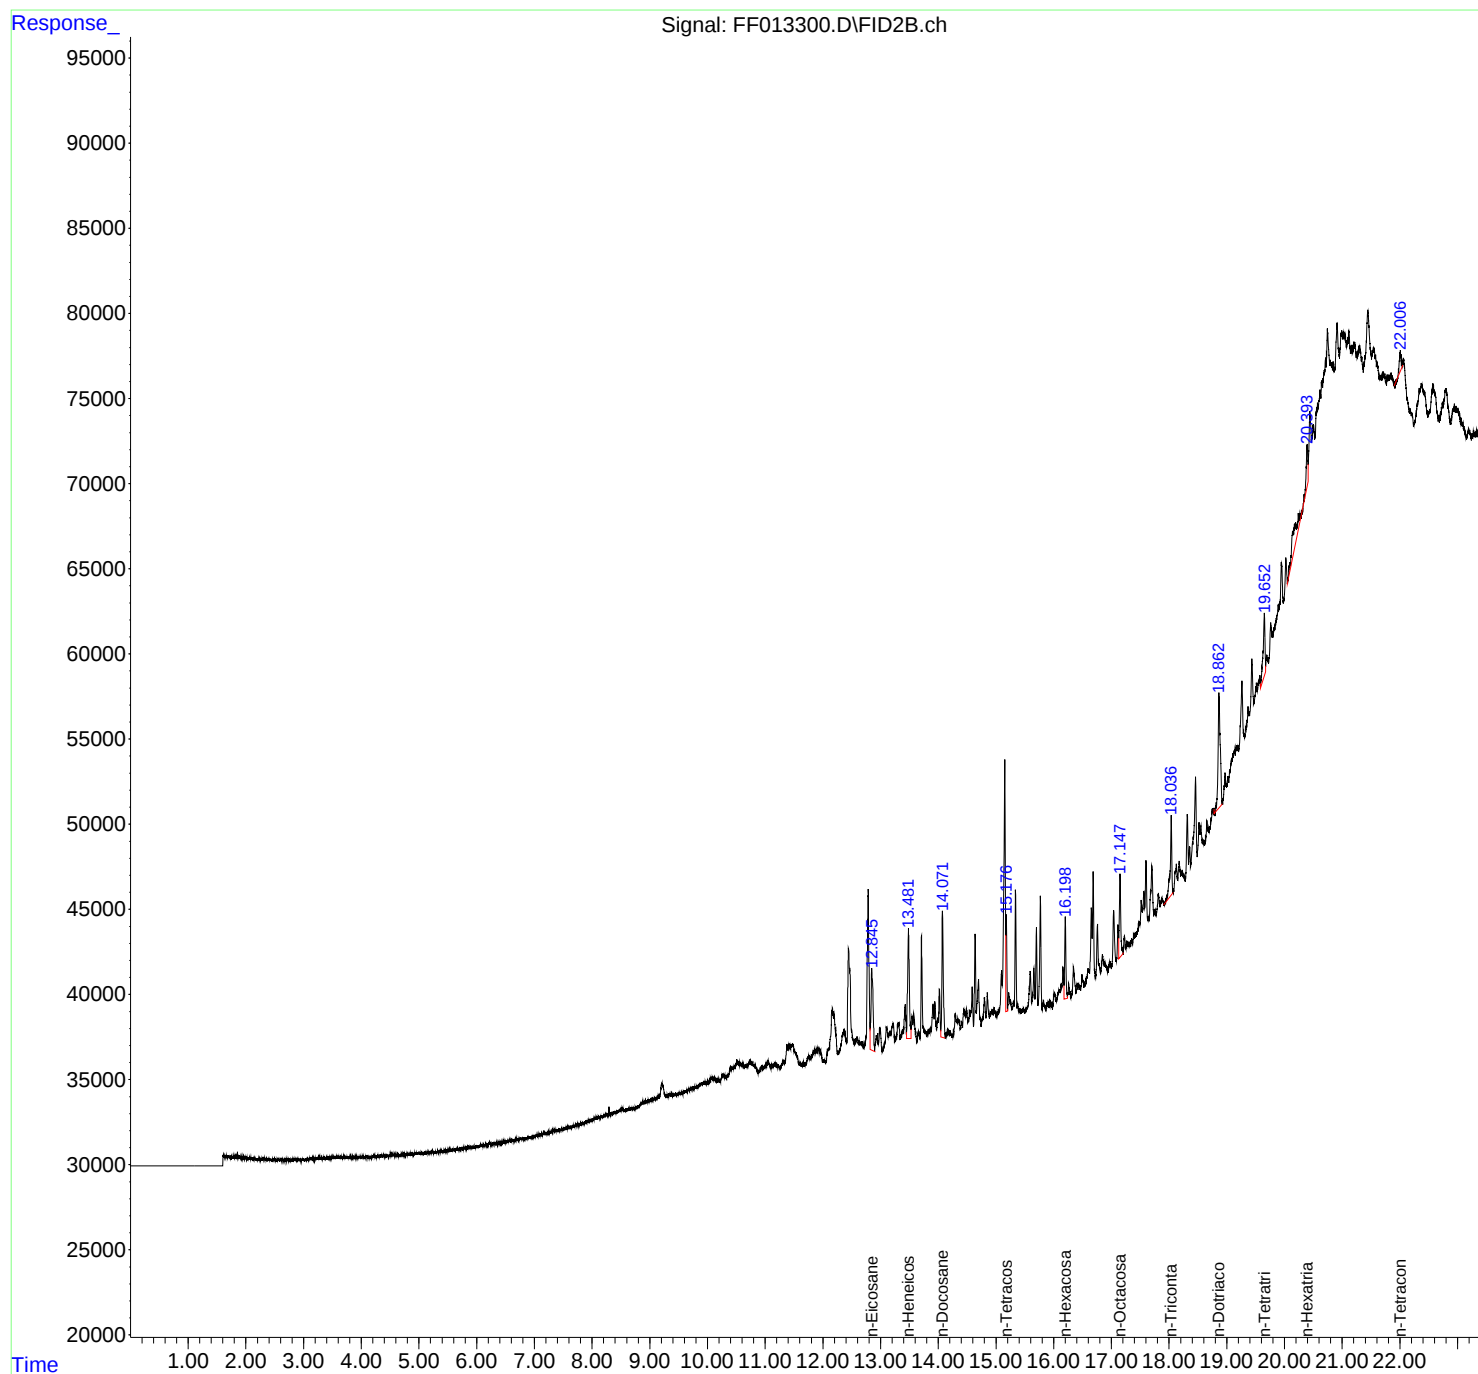


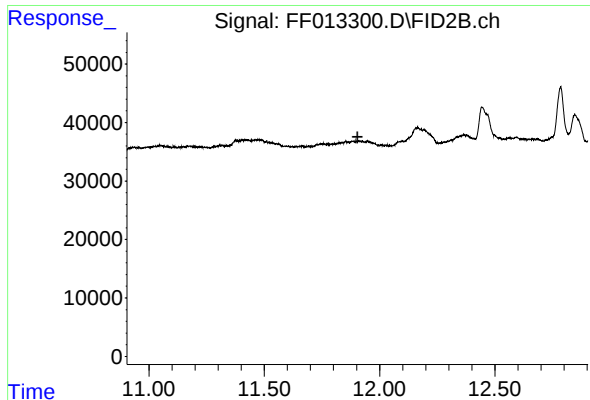

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.904 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

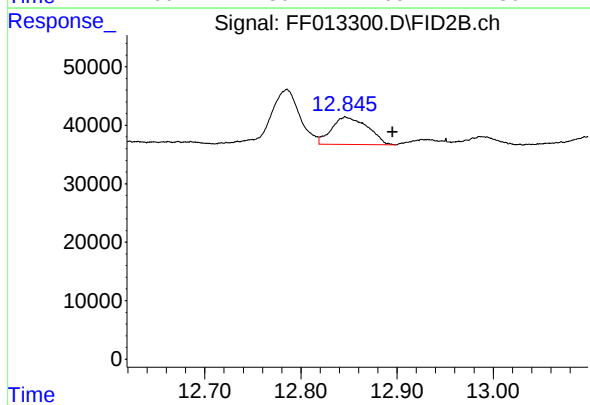


#10 n-Eicosane (C20)

R.T.: 12.846 min
Delta R.T.: -0.049 min
Response: 122427
Conc: 1.12 ug/ml

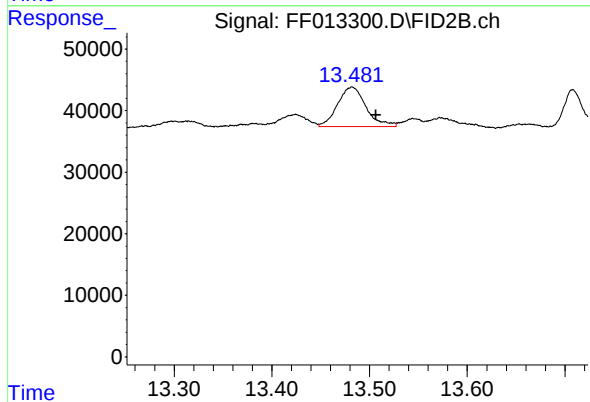


#11 n-Heneicosane (C21)

R.T.: 13.482 min
Delta R.T.: -0.024 min
Response: 130015
Conc: 1.18 ug/ml

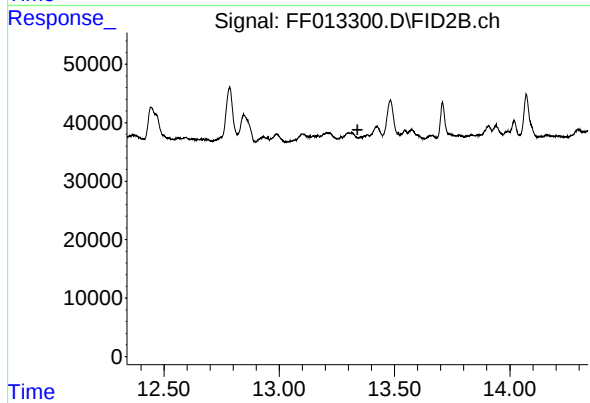

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.339 min
Response: 0
Conc: N.D.

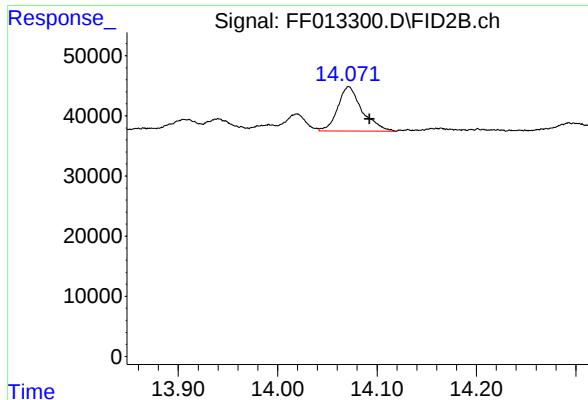

#13 n-Docosane (C22)


R.T.: 14.072 min
Delta R.T.: -0.021 min
Response: 125333
Conc: 1.14 ug/ml

Instrument :
FID_F
ClientSampleId :

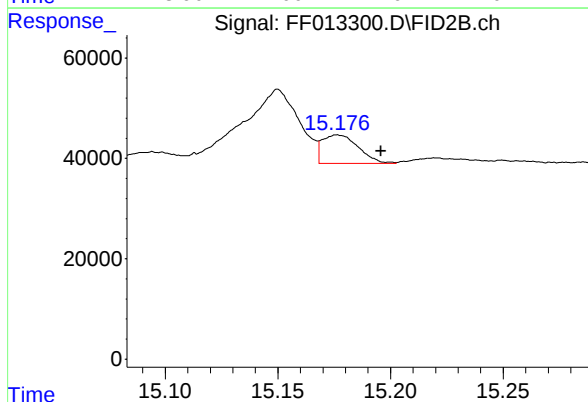


#14 n-Tetracosane (C24)

R.T.: 15.177 min
Delta R.T.: -0.019 min
Response: 63179
Conc: 0.58 ug/ml

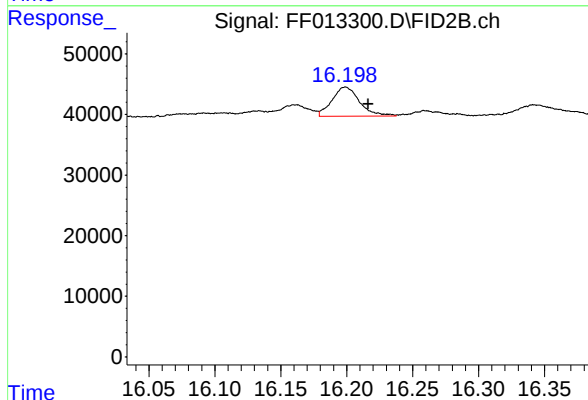


#15 n-Hexacosane (C26)

R.T.: 16.199 min
Delta R.T.: -0.018 min
Response: 69459
Conc: 0.64 ug/ml

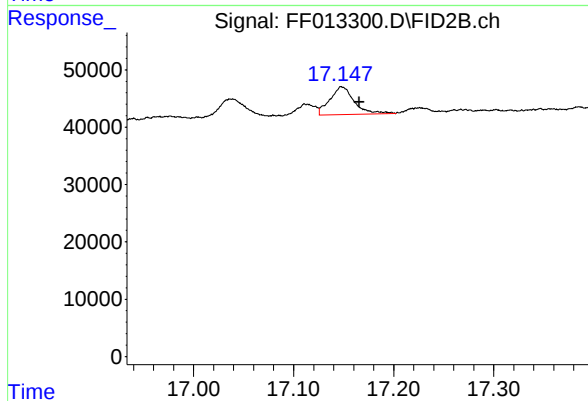

#16 n-Octacosane (C28)


R.T.: 17.148 min
Delta R.T.: -0.018 min
Response: 82330
Conc: 0.76 ug/ml

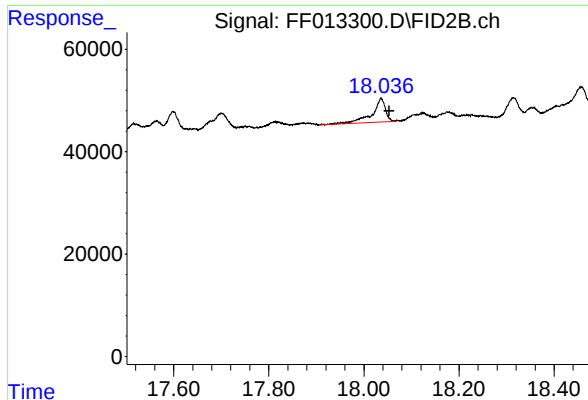

#17 n-Tricontane (C30)


R.T.: 18.036 min
Delta R.T.: -0.017 min
Response: 89530
Conc: 0.82 ug/ml

Instrument :
FID_F
ClientSampleId :

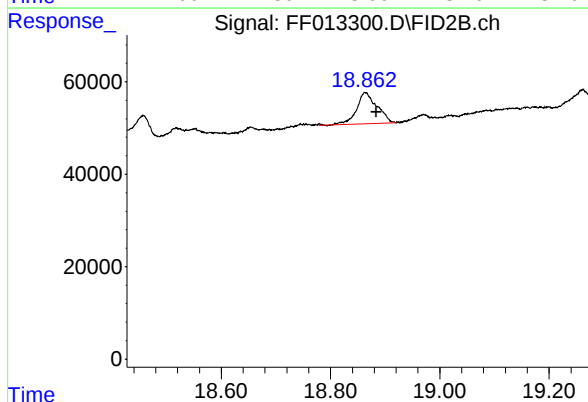


#18 n-Dotriacontane (C32)

R.T.: 18.864 min
Delta R.T.: -0.020 min
Response: 172801
Conc: 1.53 ug/ml

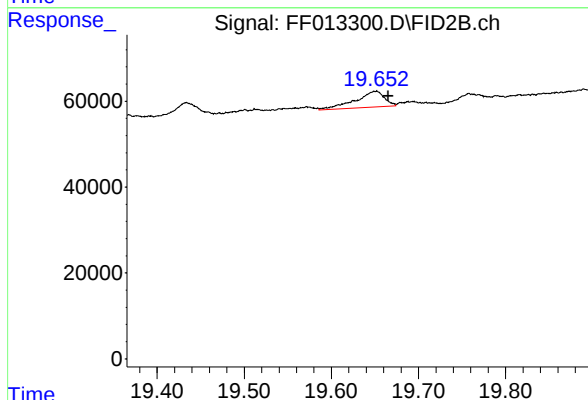


#19 n-Tetratriacontane (C34)

R.T.: 19.651 min
Delta R.T.: -0.015 min
Response: 84814
Conc: 0.80 ug/ml

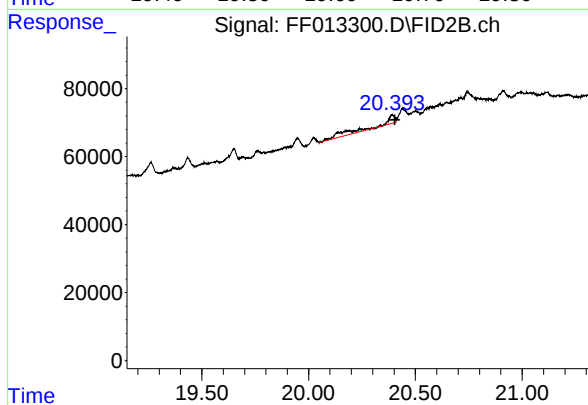

#20 n-Hexatriacontane (C36)

R.T.: 20.390 min
Delta R.T.: -0.014 min
Response: 144583
Conc: 1.37 ug/ml

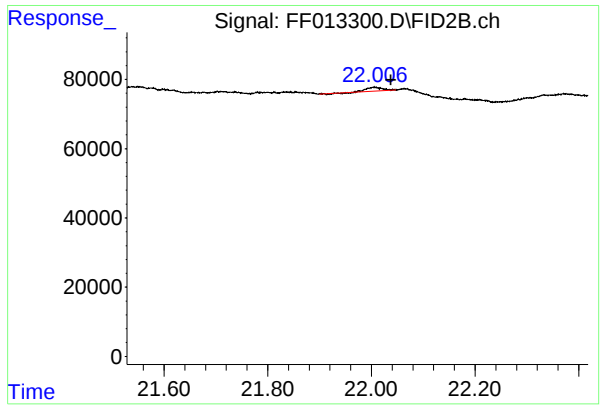

#22 n-Tetracontane (C40)

R.T.: 22.005 min

Delta R.T.: -0.033 min

Response: 23468

Conc: 0.24 ug/ml

Instrument :

FID_F

ClientSampleId :