

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082323AL\
Data File : FF013301.D
Signal(s) : FID2B.ch
Acq On : 23 Aug 2023 08:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 24 01:09:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
16) T	n-Octacosane (C28)	17.150	26114	0.242 ug/ml
17) T	n-Tricontane (C30)	18.038	116432	1.065 ug/ml
18) T	n-Dotriacontane (C32)	18.869	195000	1.726 ug/ml
19) T	n-Tetratriacontane (C34)	19.651	165330	1.556 ug/ml
20) T	n-Hexatriacontane (C36)	20.391	323034	3.065 ug/ml
21) T	n-Octatriacontane (C38)	21.119	50493	0.500 ug/ml
22) T	n-Tetracontane (C40)	22.012	183657	1.848 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082323AL\
Data File : FF013301.D
Signal(s) : FID2B.ch
Acq On : 23 Aug 2023 08:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 24 01:09:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

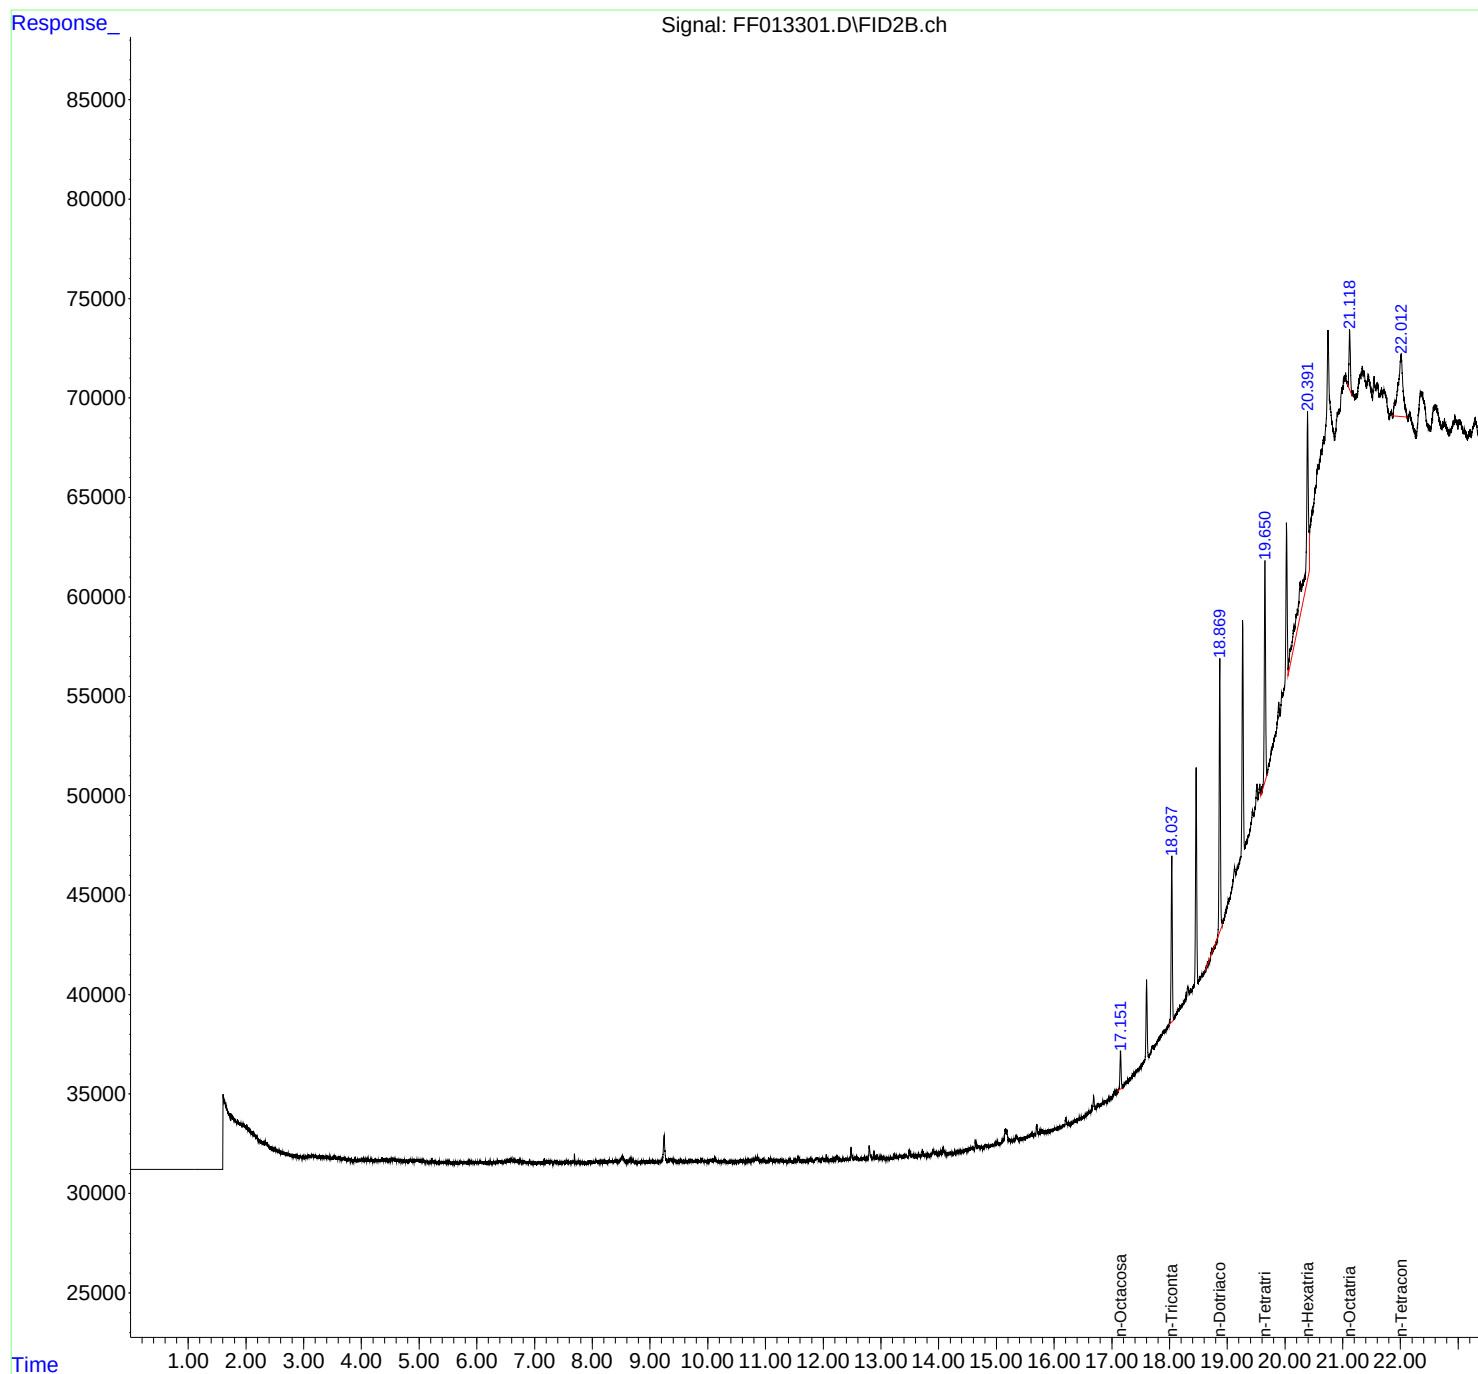


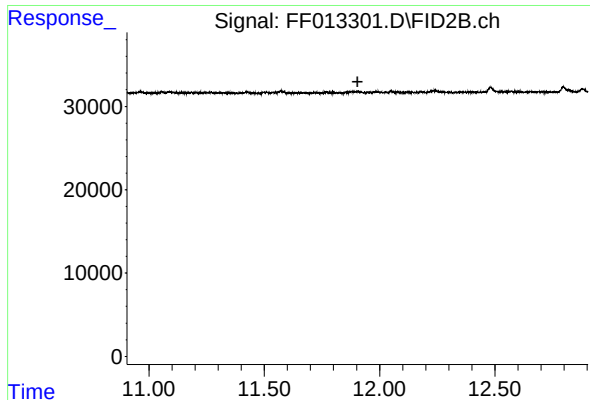

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.904 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

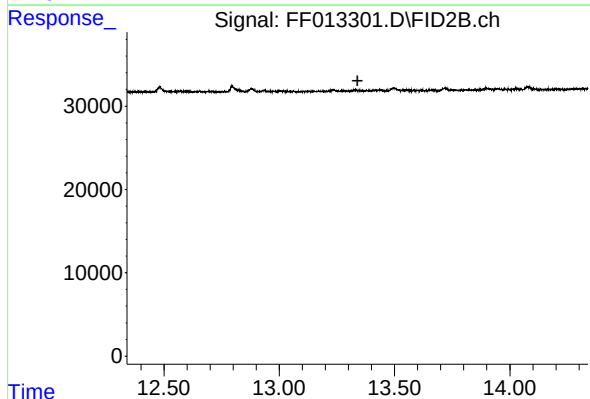


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.339 min
Response: 0
Conc: N.D.

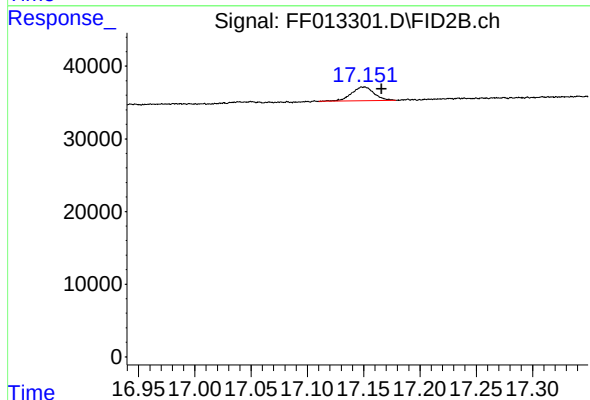


#16 n-Octacosane (C28)

R.T.: 17.150 min
Delta R.T.: -0.016 min
Response: 26114
Conc: 0.24 ug/ml

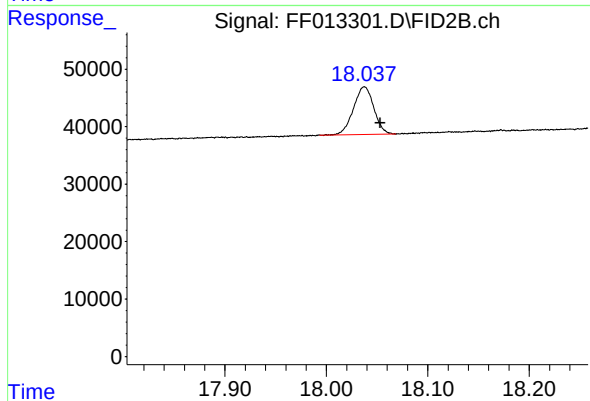

#17 n-Tricontane (C30)


R.T.: 18.038 min
Delta R.T.: -0.015 min
Response: 116432
Conc: 1.06 ug/ml

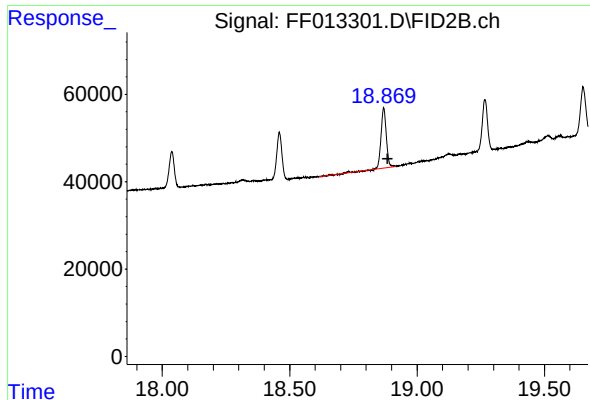

#18 n-Dotriacontane (C32)


R.T.: 18.869 min
Delta R.T.: -0.015 min
Response: 195000
Conc: 1.73 ug/ml

Instrument :
FID_F
ClientSampleId :

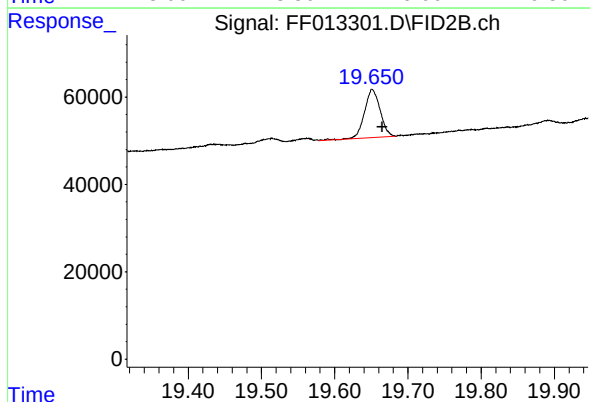


#19 n-Tetratriacontane (C34)

R.T.: 19.651 min
Delta R.T.: -0.014 min
Response: 165330
Conc: 1.56 ug/ml

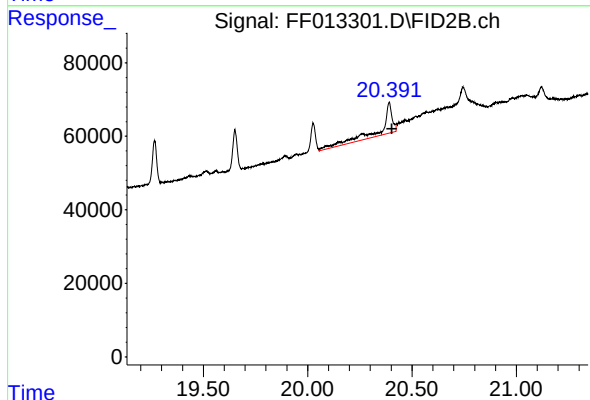


#20 n-Hexatriacontane (C36)

R.T.: 20.391 min
Delta R.T.: -0.013 min
Response: 323034
Conc: 3.06 ug/ml

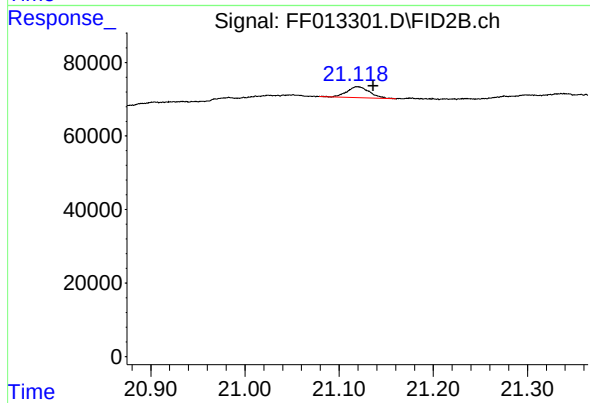

#21 n-Octatriacontane (C38)

R.T.: 21.119 min
Delta R.T.: -0.017 min
Response: 50493
Conc: 0.50 ug/ml

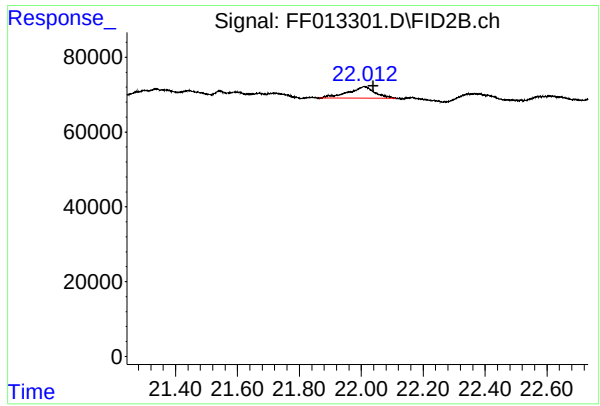

#22 n-Tetracontane (C40)

R.T.: 22.012 min
Delta R.T.: -0.026 min
Response: 183657
Conc: 1.85 ug/ml

Instrument :

FID_F

ClientSampleId :