

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082323AL\  
 Data File : FF013327.D  
 Signal(s) : FID2B.ch  
 Acq On : 24 Aug 2023 00:38  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Aug 24 01:12:59 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH 081023.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Aug 10 16:05:52 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                    |                         | R.T.   | Response | Conc Units  |
|-----------------------------|-------------------------|--------|----------|-------------|
| -----                       |                         |        |          |             |
| System Monitoring Compounds |                         |        |          |             |
| Target Compounds            |                         |        |          |             |
| 17) T                       | n-Tricontane (C30)      | 18.044 | 11874    | 0.109 ug/ml |
| 18) T                       | n-Dotriacontane (C32)   | 18.874 | 136528   | 1.209 ug/ml |
| 20) T                       | n-Hexatriacontane (C36) | 20.408 | 636649   | 6.040 ug/ml |
| 22) T                       | n-Tetracontane (C40)    | 22.025 | 339605   | 3.417 ug/ml |
| -----                       |                         |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF082323AL\  
Data File : FF013327.D  
Signal(s) : FID2B.ch  
Acq On : 24 Aug 2023 00:38  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 24 01:12:59 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH 081023.M  
Quant Title : GC Extractables  
QLast Update : Thu Aug 10 16:05:52 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

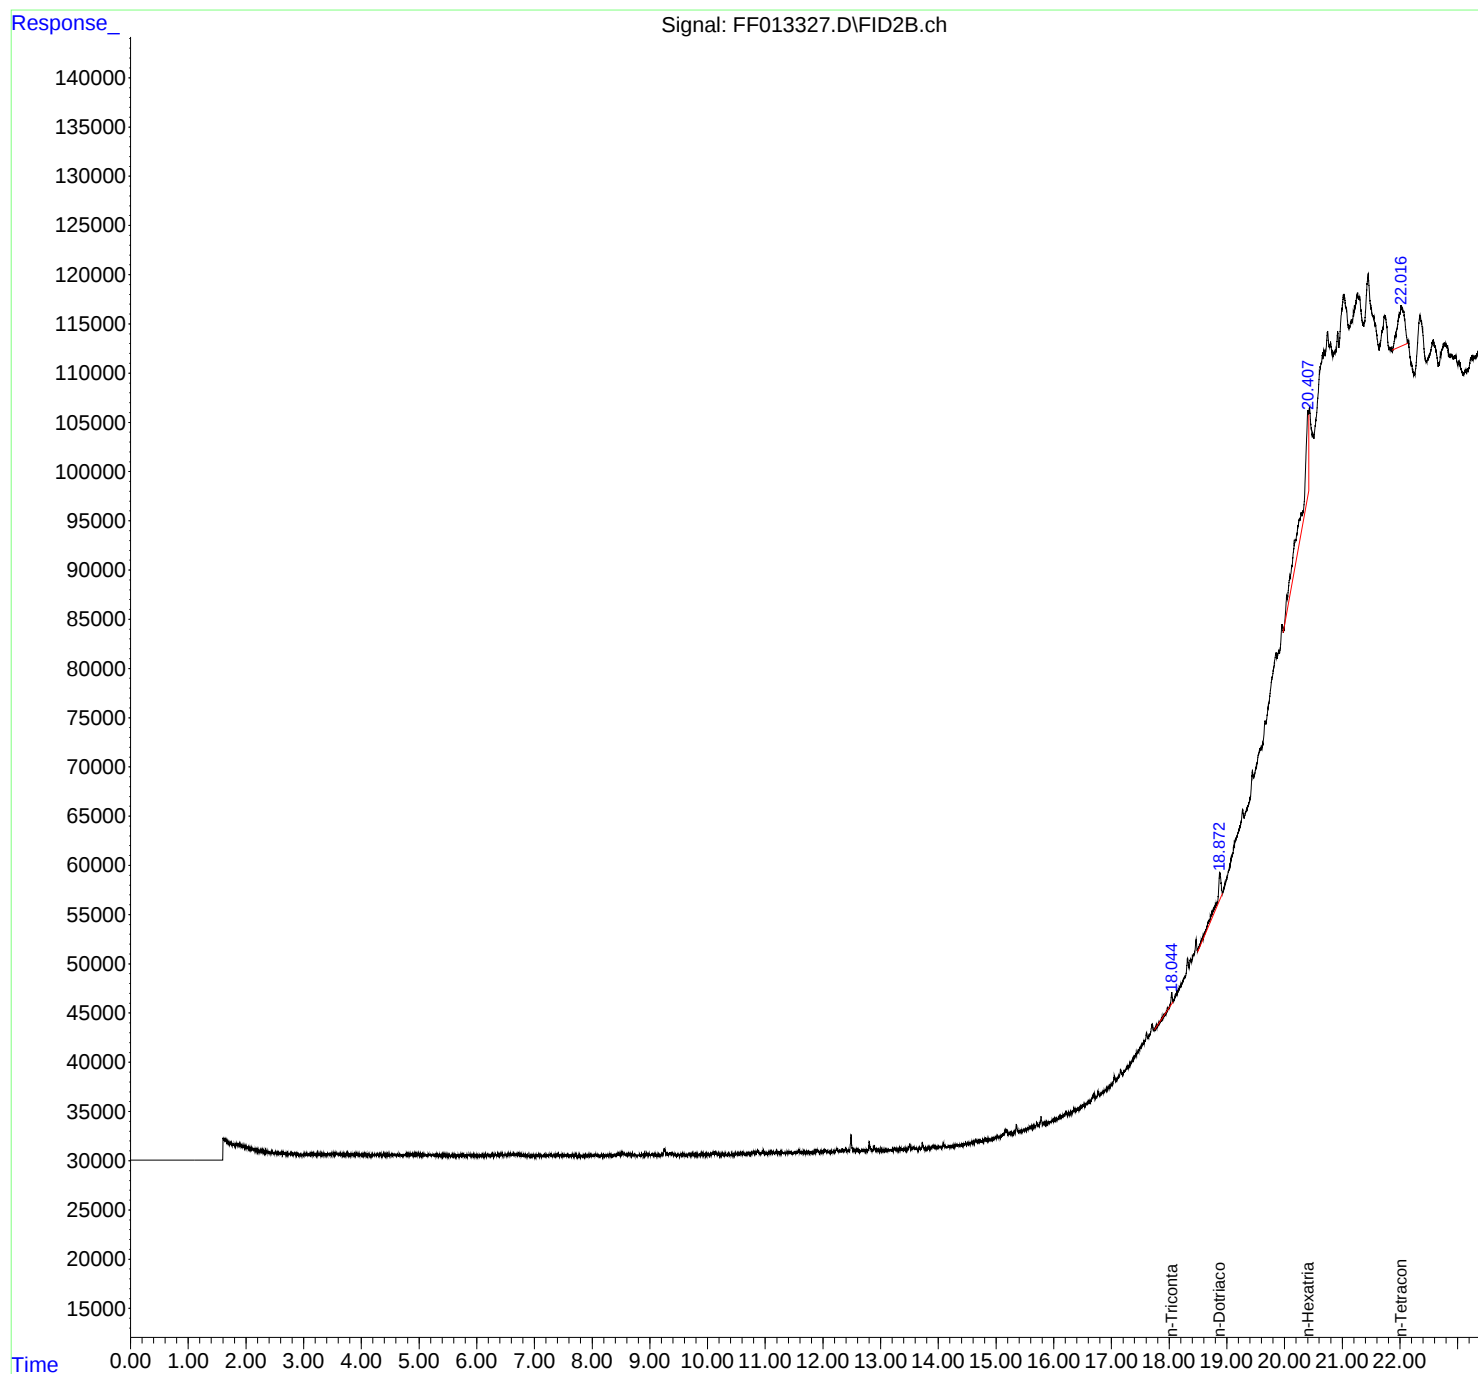


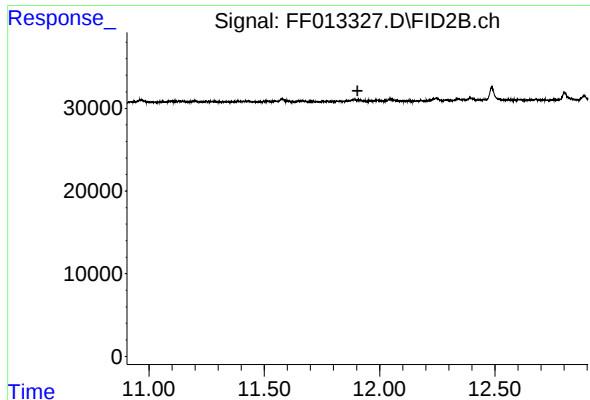

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min  
Exp R.T.: 11.904 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_F  
ClientSampleId :

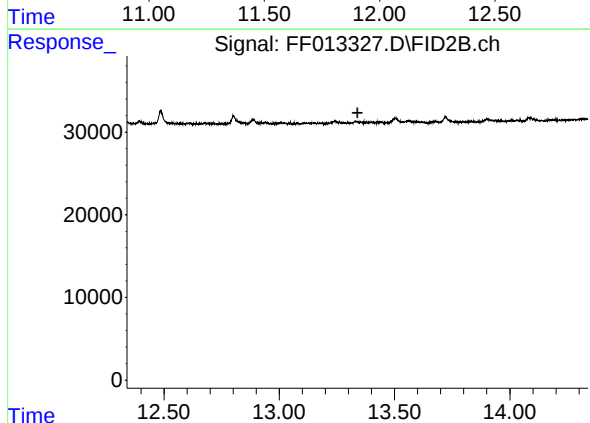


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min  
Exp R.T.: 13.339 min  
Response: 0  
Conc: N.D.

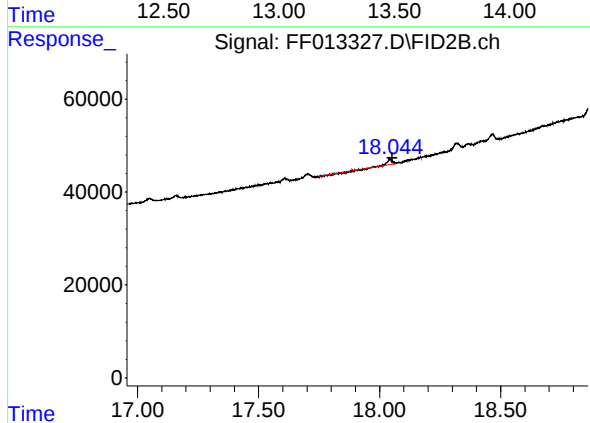


#17 n-Tricontane (C30)

R.T.: 18.044 min  
Delta R.T.: -0.009 min  
Response: 11874  
Conc: 0.11 ug/ml

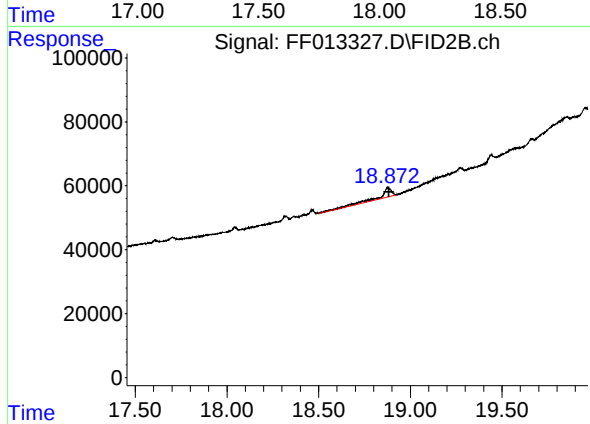

#18 n-Dotriacontane (C32)

R.T.: 18.874 min  
Delta R.T.: -0.010 min  
Response: 136528  
Conc: 1.21 ug/ml

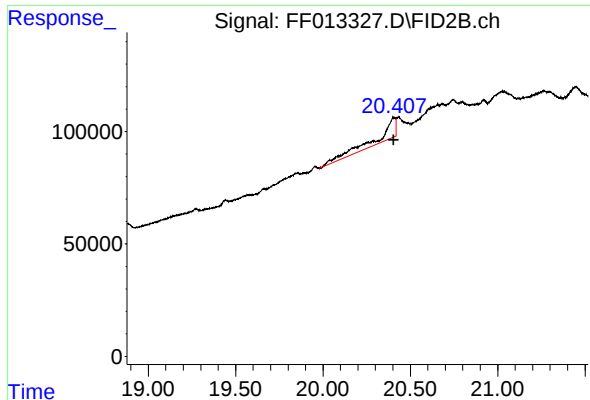


#20 n-Hexatriacontane (C36)

R.T.: 20.408 min  
Delta R.T.: 0.004 min  
Response: 636649  
Conc: 6.04 ug/ml

Instrument :

FID\_F

ClientSampleId :

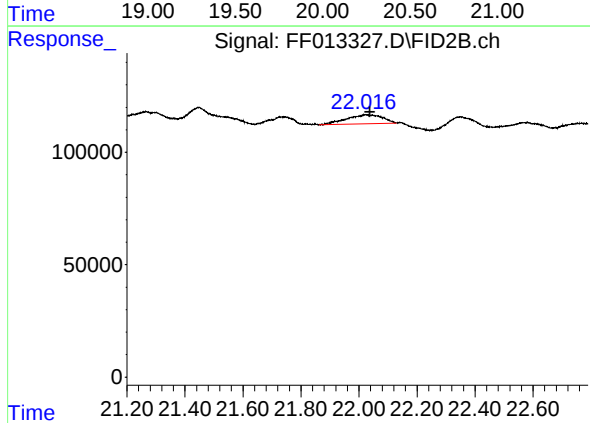

#22 n-Tetracontane (C40)

R.T.: 22.025 min  
Delta R.T.: -0.013 min  
Response: 339605  
Conc: 3.42 ug/ml