

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082419\
Data File : FF005330.D
Signal(s) : FID2B.ch
Acq On : 24 Aug 2019 14:24
Operator : DD\AJ
Sample : K4510-06
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 26 01:20:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.639	1506678	13.681 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.237	318606	2.214 ug/ml
12)	N-OCTACOSANE	16.822	165323	1.324 ug/ml
13)	N-TRIACONTANE	17.714	208579	1.636 ug/ml
14)	N-DOTRIACONTANE	18.551	124038	0.996 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082419\
Data File : FF005330.D
Signal(s) : FID2B.ch
Acq On : 24 Aug 2019 14:24
Operator : DD\AJ
Sample : K4510-06
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 26 01:20:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

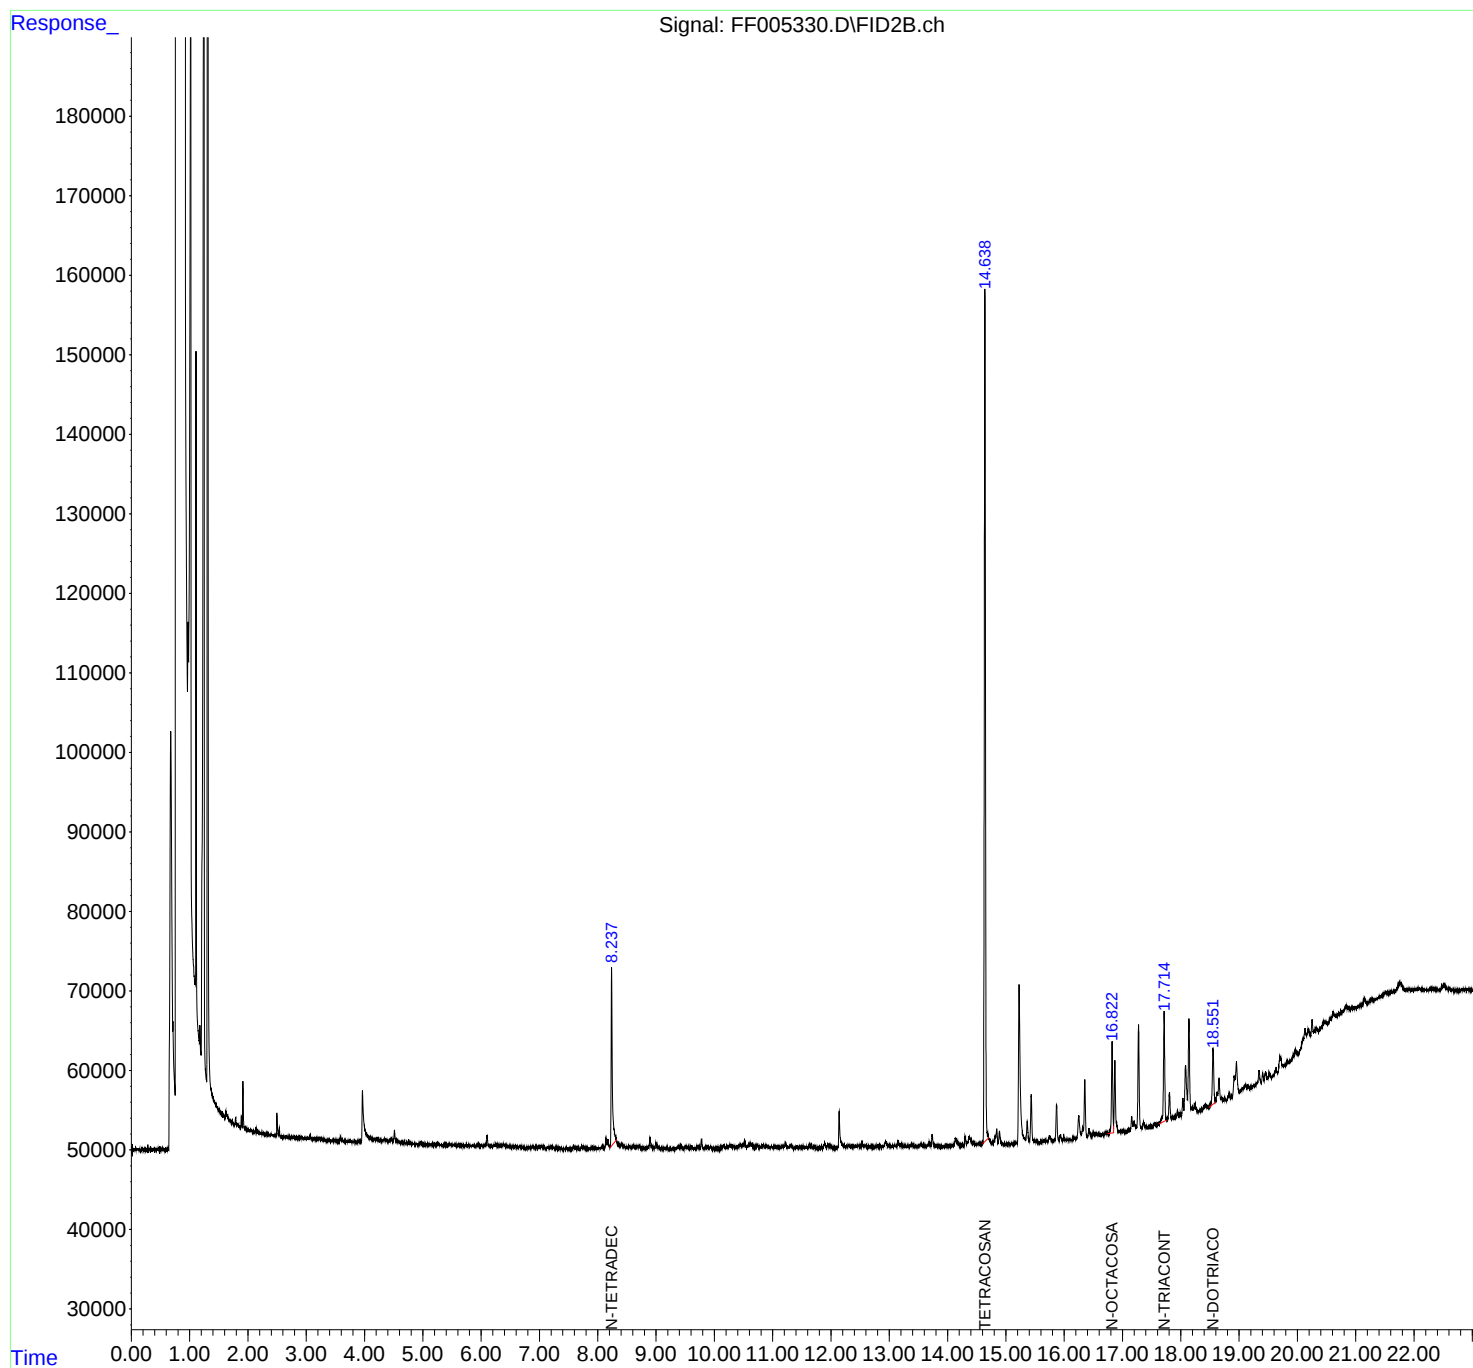

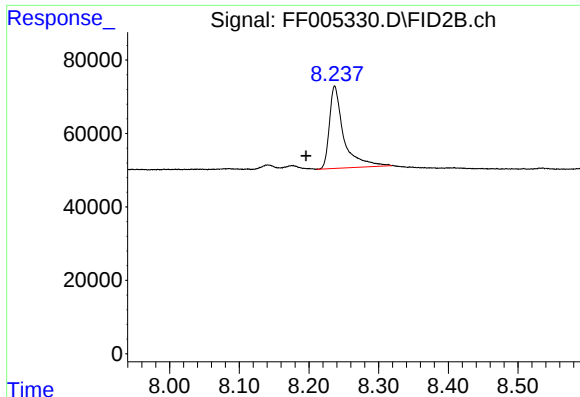


#4 N-TETRADECANE

R.T.: 8.237 min
Delta R.T.: 0.041 min
Response: 318606
Conc: 2.21 ug/ml

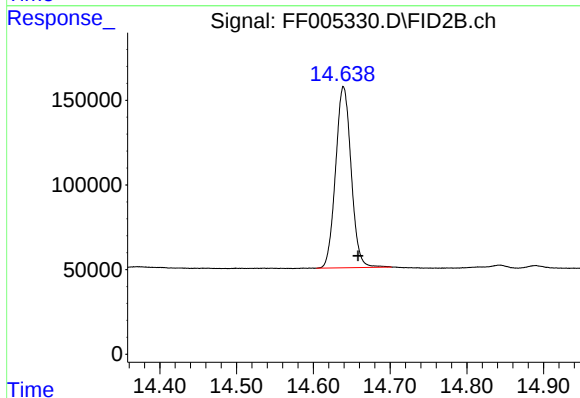


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.639 min
Delta R.T.: -0.019 min
Response: 1506678
Conc: 13.68 ug/ml

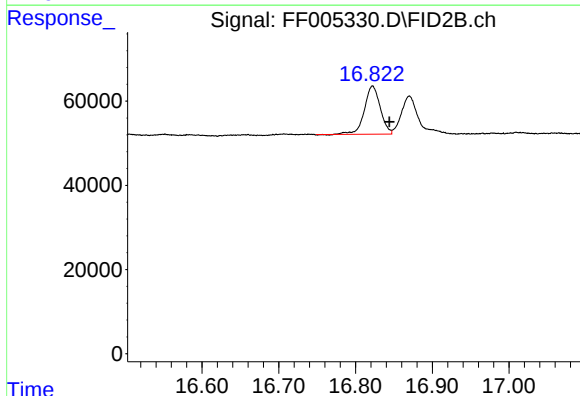


#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.022 min
Response: 165323
Conc: 1.32 ug/ml

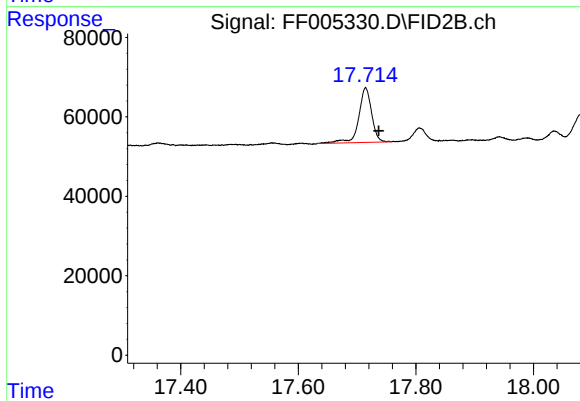

#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.023 min
Response: 208579
Conc: 1.64 ug/ml

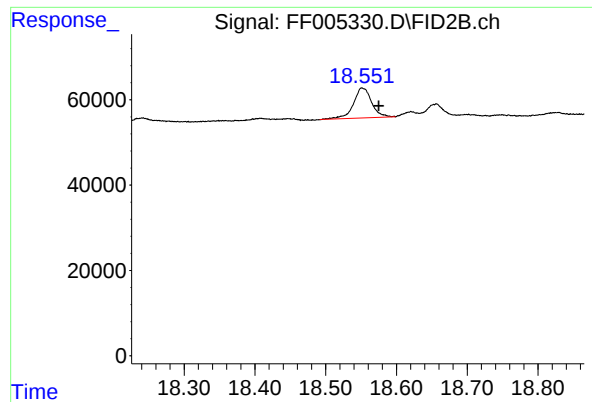

#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: -0.024 min
Response: 124038
Conc: 1.00 ug/ml