

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082419\
Data File : FF005332.D
Signal(s) : FID2B.ch
Acq On : 24 Aug 2019 15:24
Operator : DD\AJ
Sample : K4510-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 26 01:20:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.639	1465765	13.310 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.237	425650	2.957 ug/ml
12)	N-OCTACOSANE	16.822	167713	1.343 ug/ml
13)	N-TRIACONTANE	17.716	230021	1.804 ug/ml
14)	N-DOTRIACONTANE	18.554	168709	1.355 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082419\
Data File : FF005332.D
Signal(s) : FID2B.ch
Acq On : 24 Aug 2019 15:24
Operator : DD\AJ
Sample : K4510-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 26 01:20:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

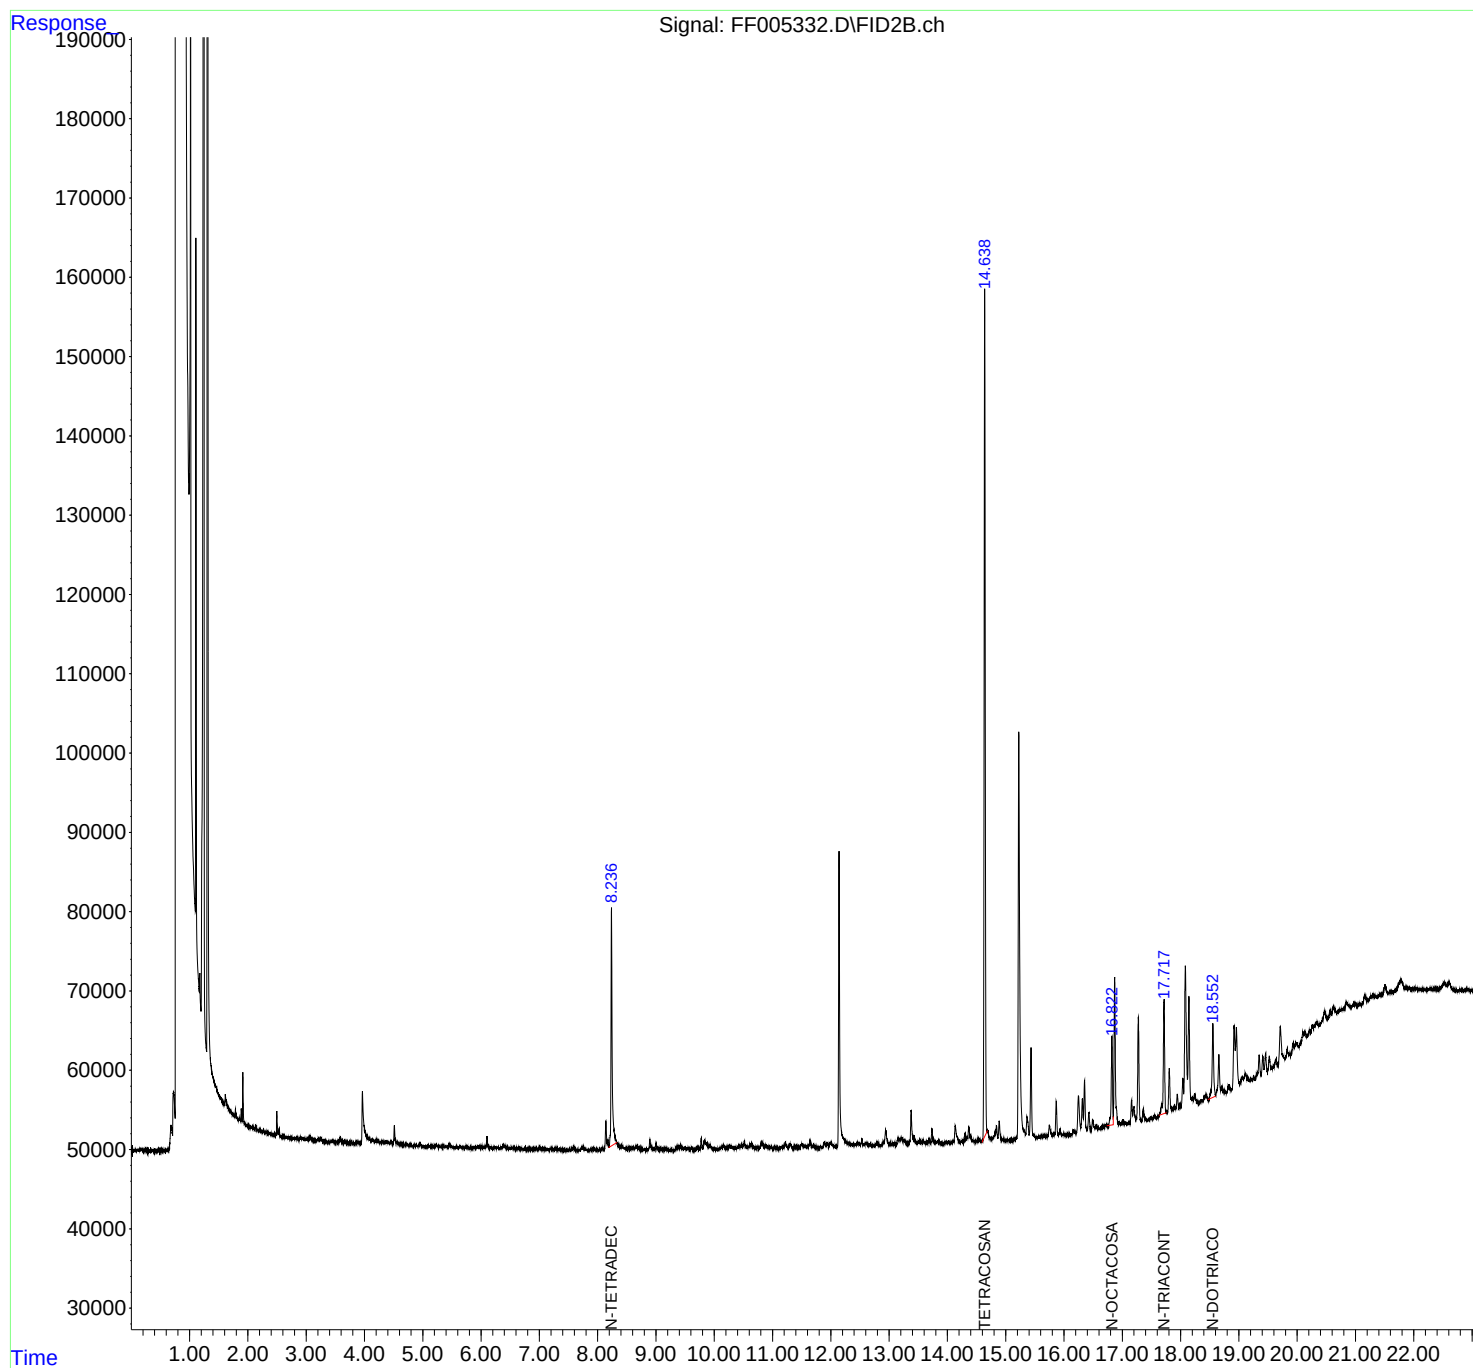

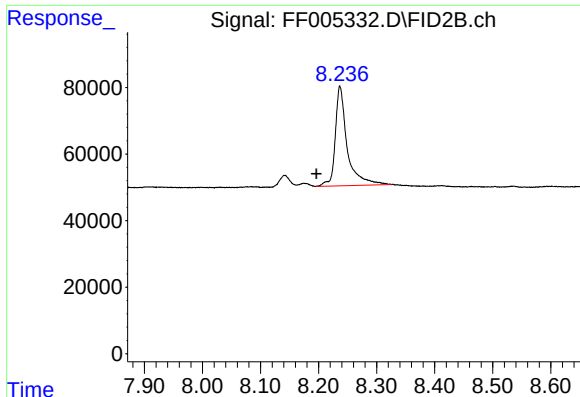


#4 N-TETRADECANE

R.T.: 8.237 min
Delta R.T.: 0.041 min
Response: 425650
Conc: 2.96 ug/ml

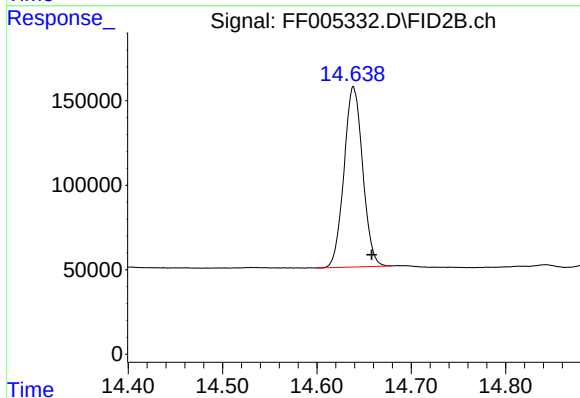


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.639 min
Delta R.T.: -0.020 min
Response: 1465765
Conc: 13.31 ug/ml

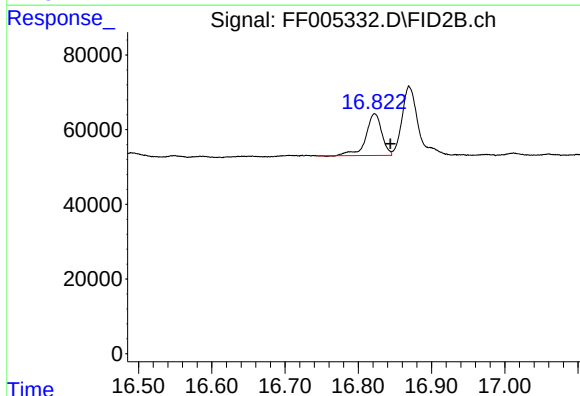


#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.022 min
Response: 167713
Conc: 1.34 ug/ml

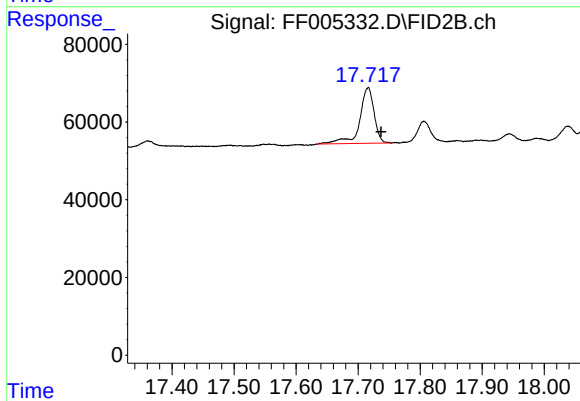

#13 N-TRIACONTANE

R.T.: 17.716 min
Delta R.T.: -0.021 min
Response: 230021
Conc: 1.80 ug/ml

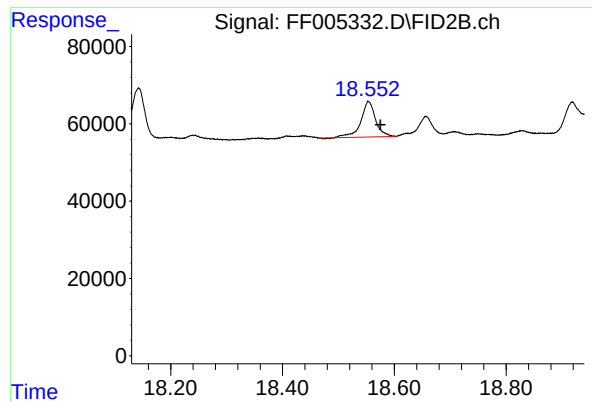

#14 N-DOTRIACONTANE

R.T.: 18.554 min
Delta R.T.: -0.021 min
Response: 168709
Conc: 1.36 ug/ml