

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082423AL\
 Data File : FF013329.D
 Signal(s) : FID2B.ch
 Acq On : 24 Aug 2023 07:59
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 25 01:40:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 10 16:05:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11) T	n-Heneicosane (C21)	13.487	115888	1.055 ug/ml
13) T	n-Docosane (C22)	14.074	118509	1.079 ug/ml
14) T	n-Tetracosane (C24)	15.154	77925	0.709 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082423AL\
Data File : FF013329.D
Signal(s) : FID2B.ch
Acq On : 24 Aug 2023 07:59
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 25 01:40:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 081023.M
Quant Title : GC Extractables
QLast Update : Thu Aug 10 16:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

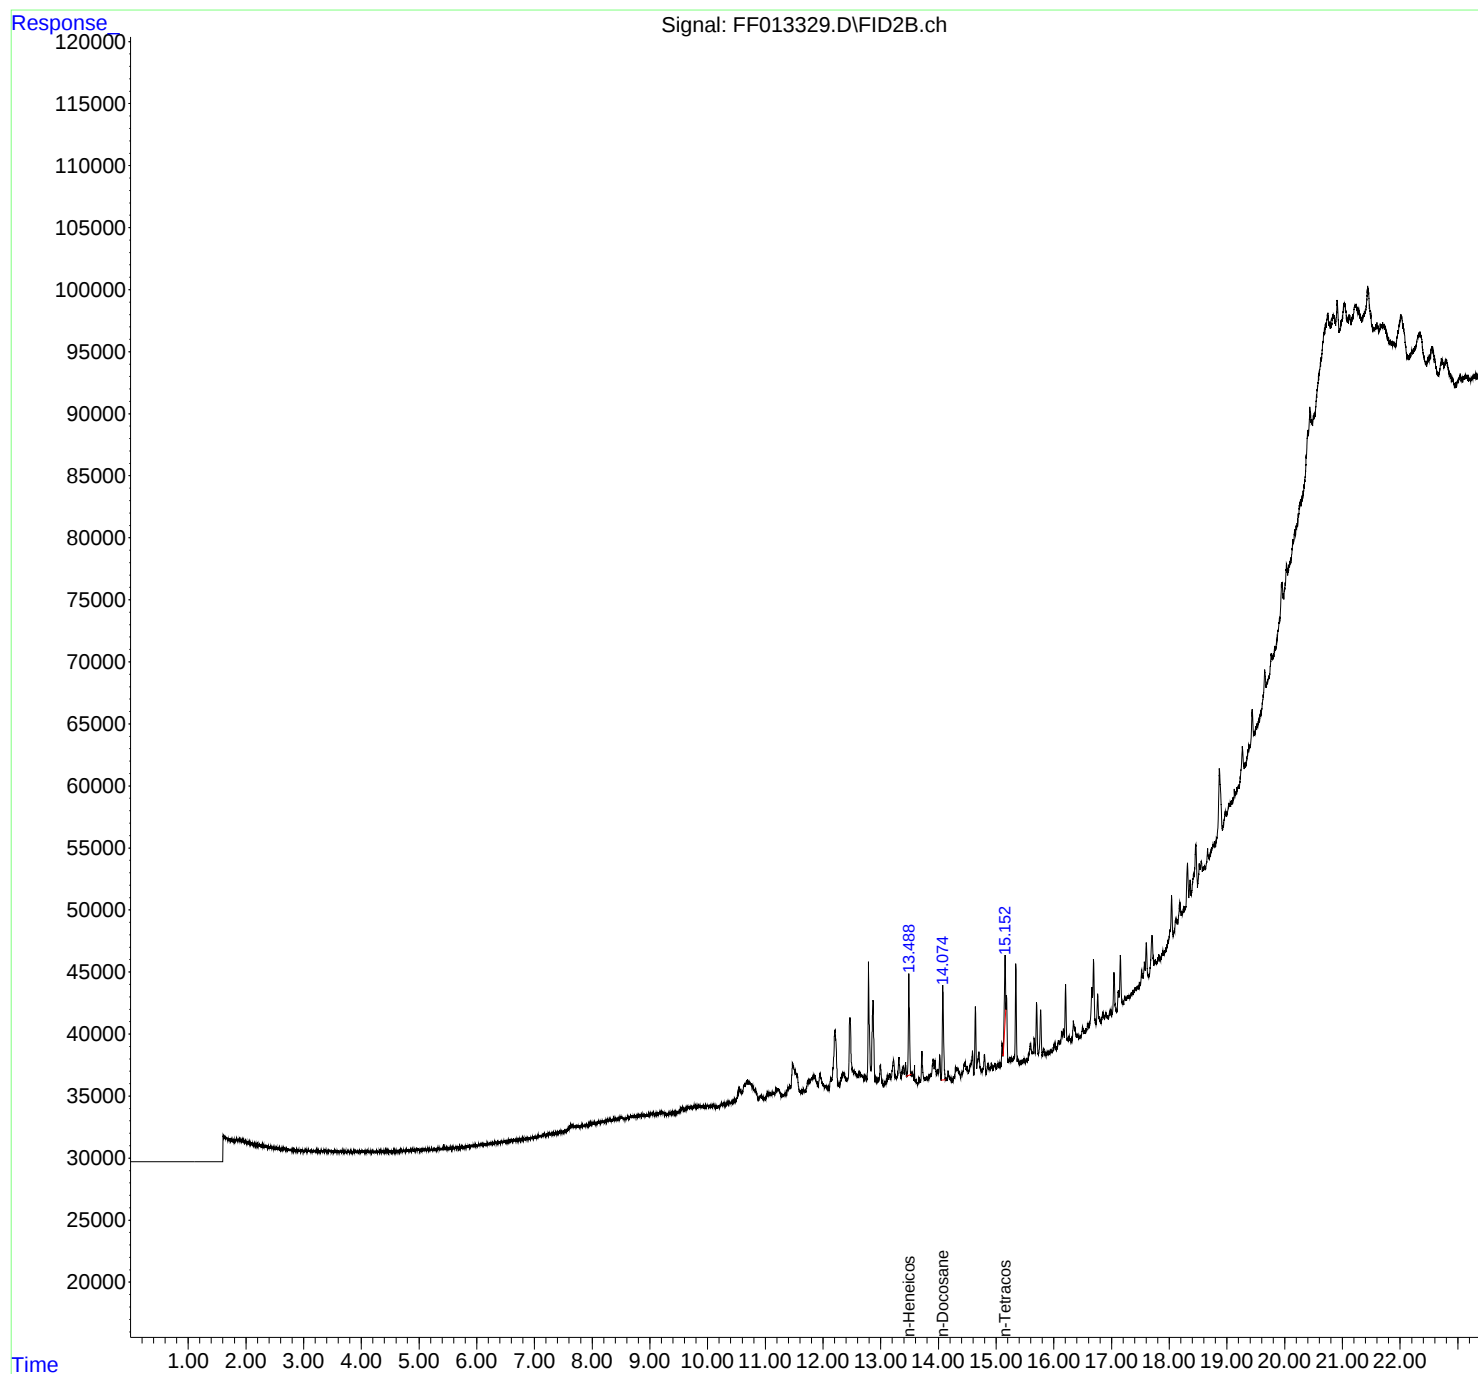


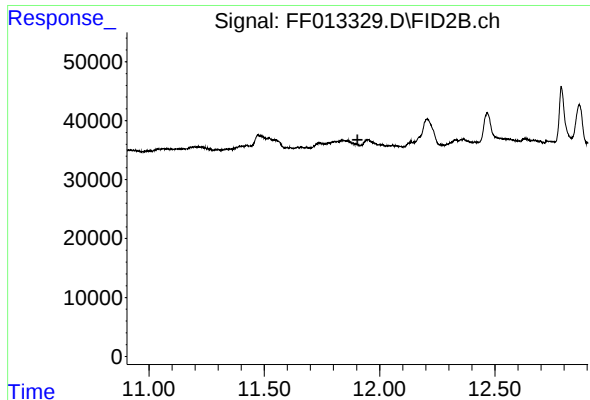

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.904 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

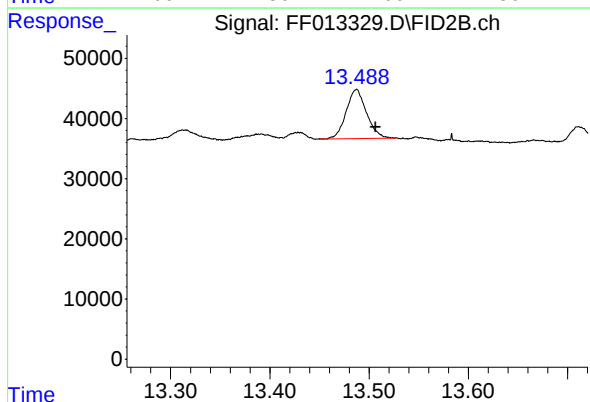


#11 n-Heneicosane (C21)

R.T.: 13.487 min
Delta R.T.: -0.019 min
Response: 115888
Conc: 1.05 ug/ml

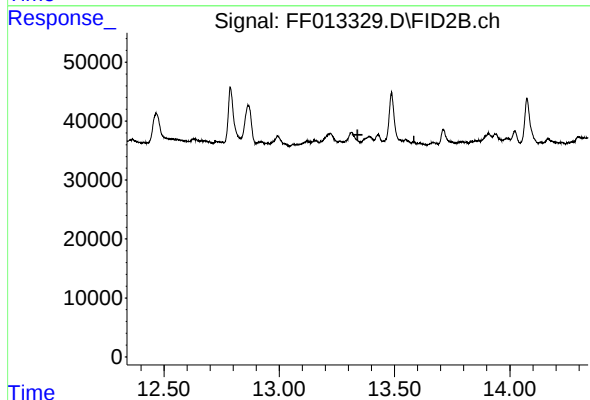


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.339 min
Response: 0
Conc: N.D.

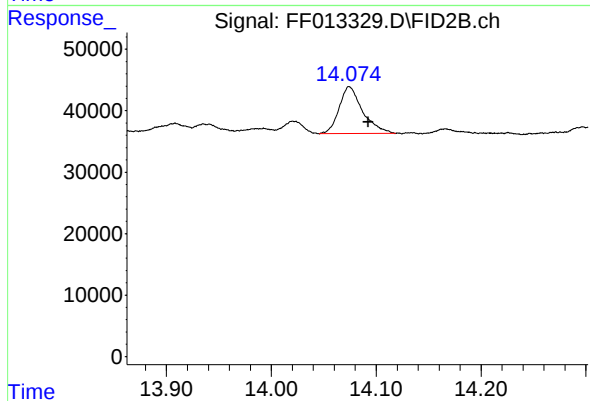

#13 n-Docosane (C22)

R.T.: 14.074 min
Delta R.T.: -0.018 min
Response: 118509
Conc: 1.08 ug/ml

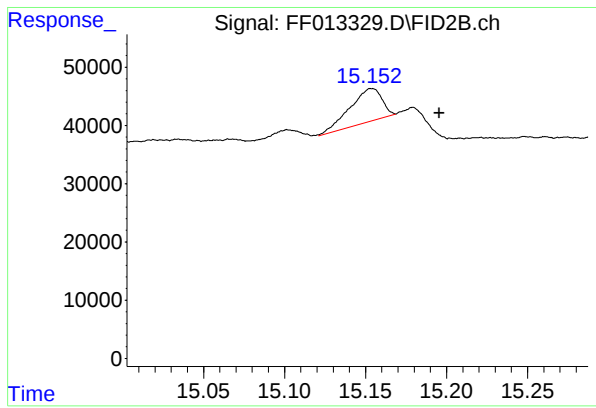

#14 n-Tetracosane (C24)

R.T.: 15.154 min

Delta R.T.: -0.042 min

Response: 77925

Conc: 0.71 ug/ml

Instrument :

FID_F

ClientSampleId :