

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082522\
Data File : FF011296.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2022 14:10
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 25 18:42:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.521	3191548	25.354 ug/ml
12)	N-OCTACOSANE	16.960	3093828	25.629 ug/ml
13)	N-TRIACONTANE	17.844	157288	1.317 ug/ml
14)	N-DOTRIACONTANE	18.673	227288	1.924 ug/ml
15)	N-TETRATRIACONTANE	19.454	219337	1.966 ug/ml
16)	N-HEXATRIACONTANE	20.193	192132	1.890 ug/ml
17)	N-OCTATRIACONTANE	20.898	261935	2.618 ug/ml
18)	N-TETRACONTANE	21.714	505599	4.614 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082522\
Data File : FF011296.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2022 14:10
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 25 18:42:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

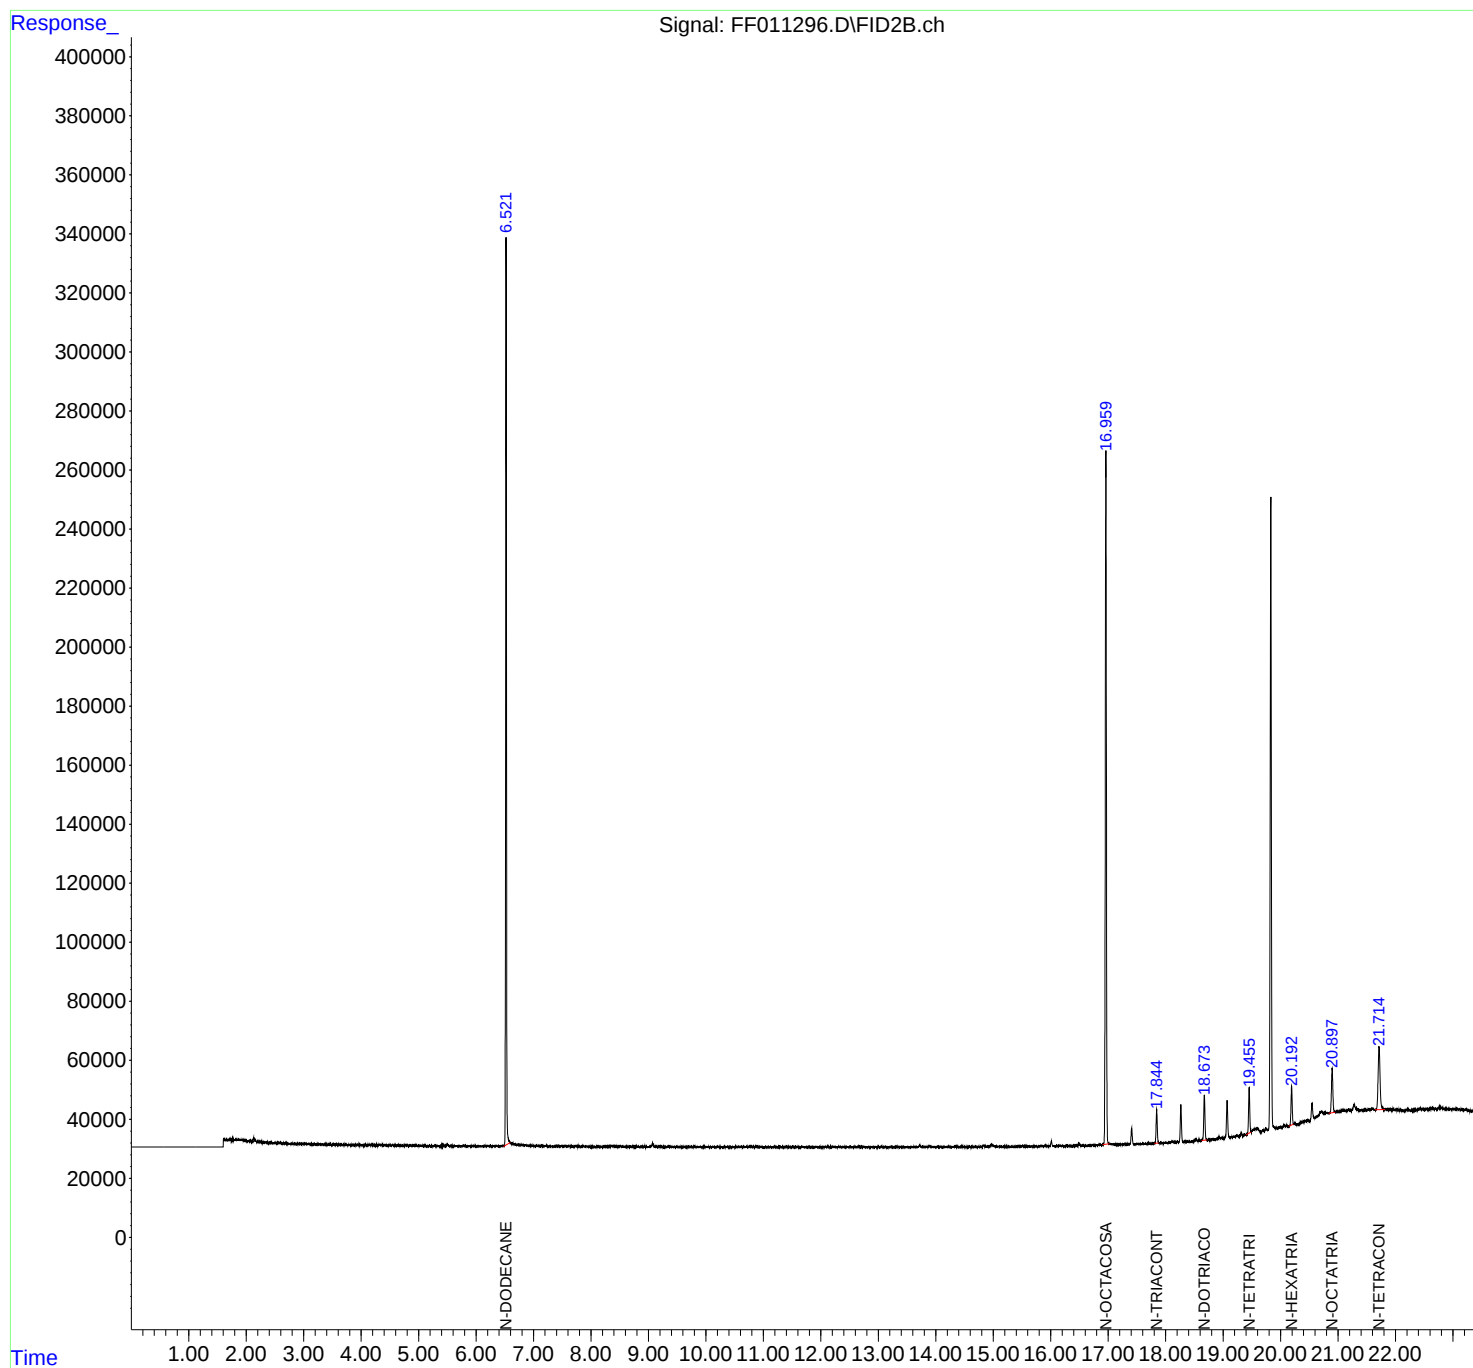


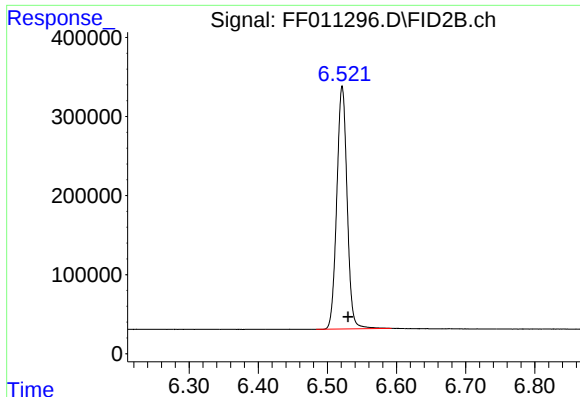

#3 N-DODECANE


R.T.: 6.521 min
Delta R.T.: -0.008 min
Response: 3191548
Conc: 25.35 ug/ml

Instrument :
FID_F
ClientSampleId :

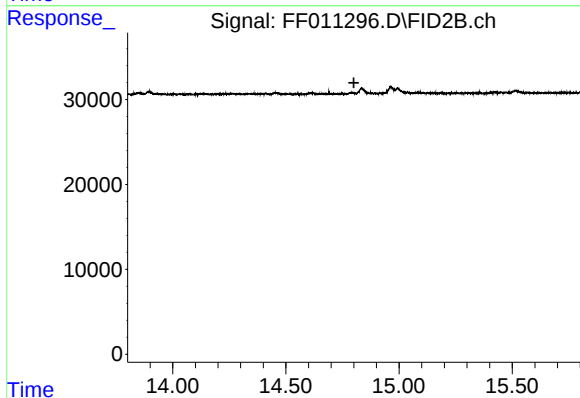


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.801 min
Response: 0
Conc: N.D.

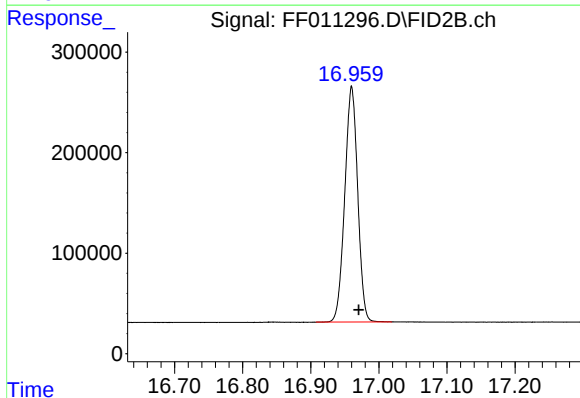


#12 N-OCTACOSANE

R.T.: 16.960 min
Delta R.T.: -0.011 min
Response: 3093828
Conc: 25.63 ug/ml

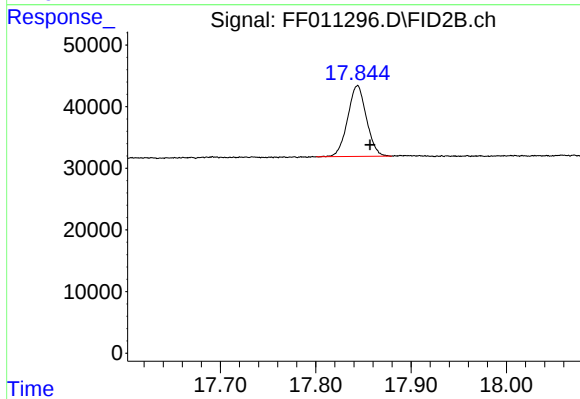

#13 N-TRIACONTANE


R.T.: 17.844 min
Delta R.T.: -0.013 min
Response: 157288
Conc: 1.32 ug/ml

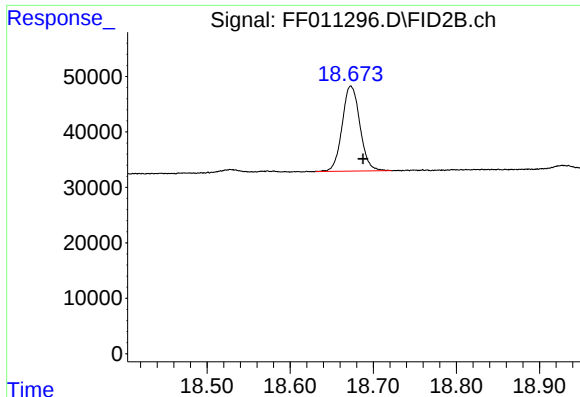

#14 N-DOTRIACONTANE


R.T.: 18.673 min
Delta R.T.: -0.015 min
Response: 227288
Conc: 1.92 ug/ml

Instrument :
FID_F
ClientSampleId :

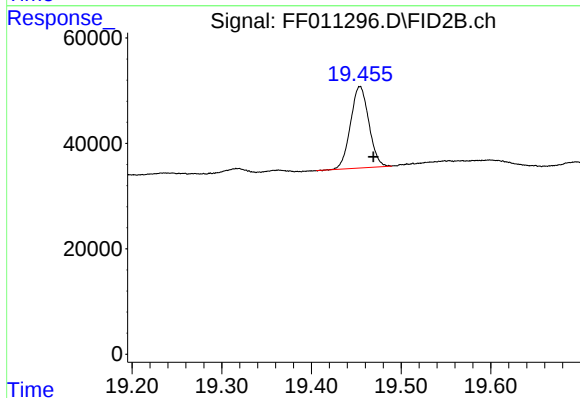


#15 N-TETRATRIACONTANE

R.T.: 19.454 min
Delta R.T.: -0.015 min
Response: 219337
Conc: 1.97 ug/ml

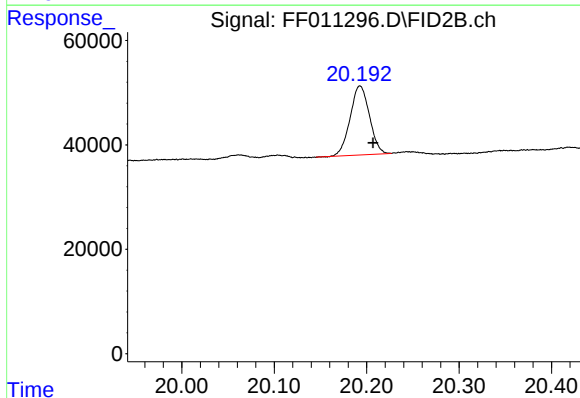


#16 N-HEXATRIACONTANE

R.T.: 20.193 min
Delta R.T.: -0.014 min
Response: 192132
Conc: 1.89 ug/ml

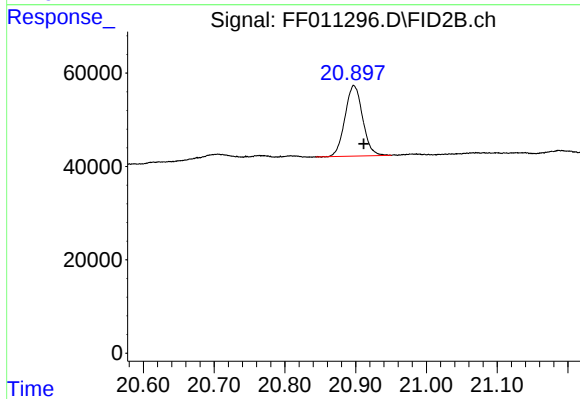

#17 N-OCTATRIACONTANE

R.T.: 20.898 min
Delta R.T.: -0.014 min
Response: 261935
Conc: 2.62 ug/ml

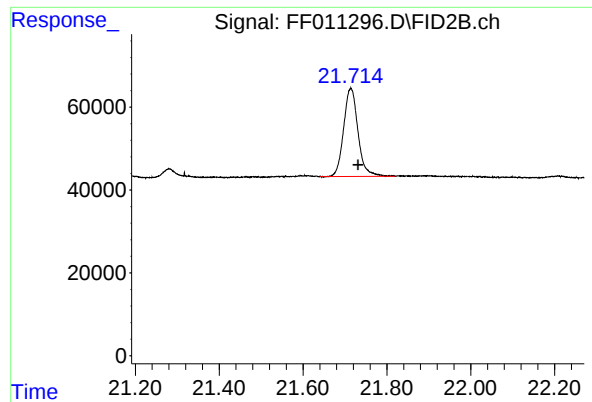

#18 N-TETRACONTANE

R.T.: 21.714 min
Delta R.T.: -0.018 min
Response: 505599
Conc: 4.61 ug/ml

Instrument :

FID_F

ClientSampleId :